

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF062323AL\  
 Data File : FF012991.D  
 Signal(s) : FID2B.ch  
 Acq On : 23 Jun 2023 23:44  
 Operator : YP\AJ  
 Sample : 03365-42  
 Misc :  
 ALS Vial : 76 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :  
 TP3-H

Integration File: autoint1.e  
 Quant Time: Jun 24 04:07:46 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\Aliphatic EPH 062023.M  
 Quant Title : GC Extractables  
 QLast Update : Tue Jun 20 13:45:06 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response | Conc Units   |
|--------------------------------|--------|----------|--------------|
| -----                          |        |          |              |
| System Monitoring Compounds    |        |          |              |
| 9) S ortho-Terphenyl (SURR)    | 10.874 | 4100972  | 27.793 ug/ml |
| Spiked Amount                  | 50.000 | Recovery | = 55.59%     |
| 12) S 1-chlorooctadecane (S... | 12.306 | 3217772  | 30.372 ug/ml |
| Spiked Amount                  | 50.000 | Recovery | = 60.74%     |

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF062323AL\  
Data File : FF012991.D  
Signal(s) : FID2B.ch  
Acq On : 23 Jun 2023 23:44  
Operator : YP\AJ  
Sample : 03365-42  
Misc :  
ALS Vial : 76 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
TP3-H

Integration File: autoint1.e  
Quant Time: Jun 24 04:07:46 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\Aliphatic EPH 062023.M  
Quant Title : GC Extractables  
QLast Update : Tue Jun 20 13:45:06 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

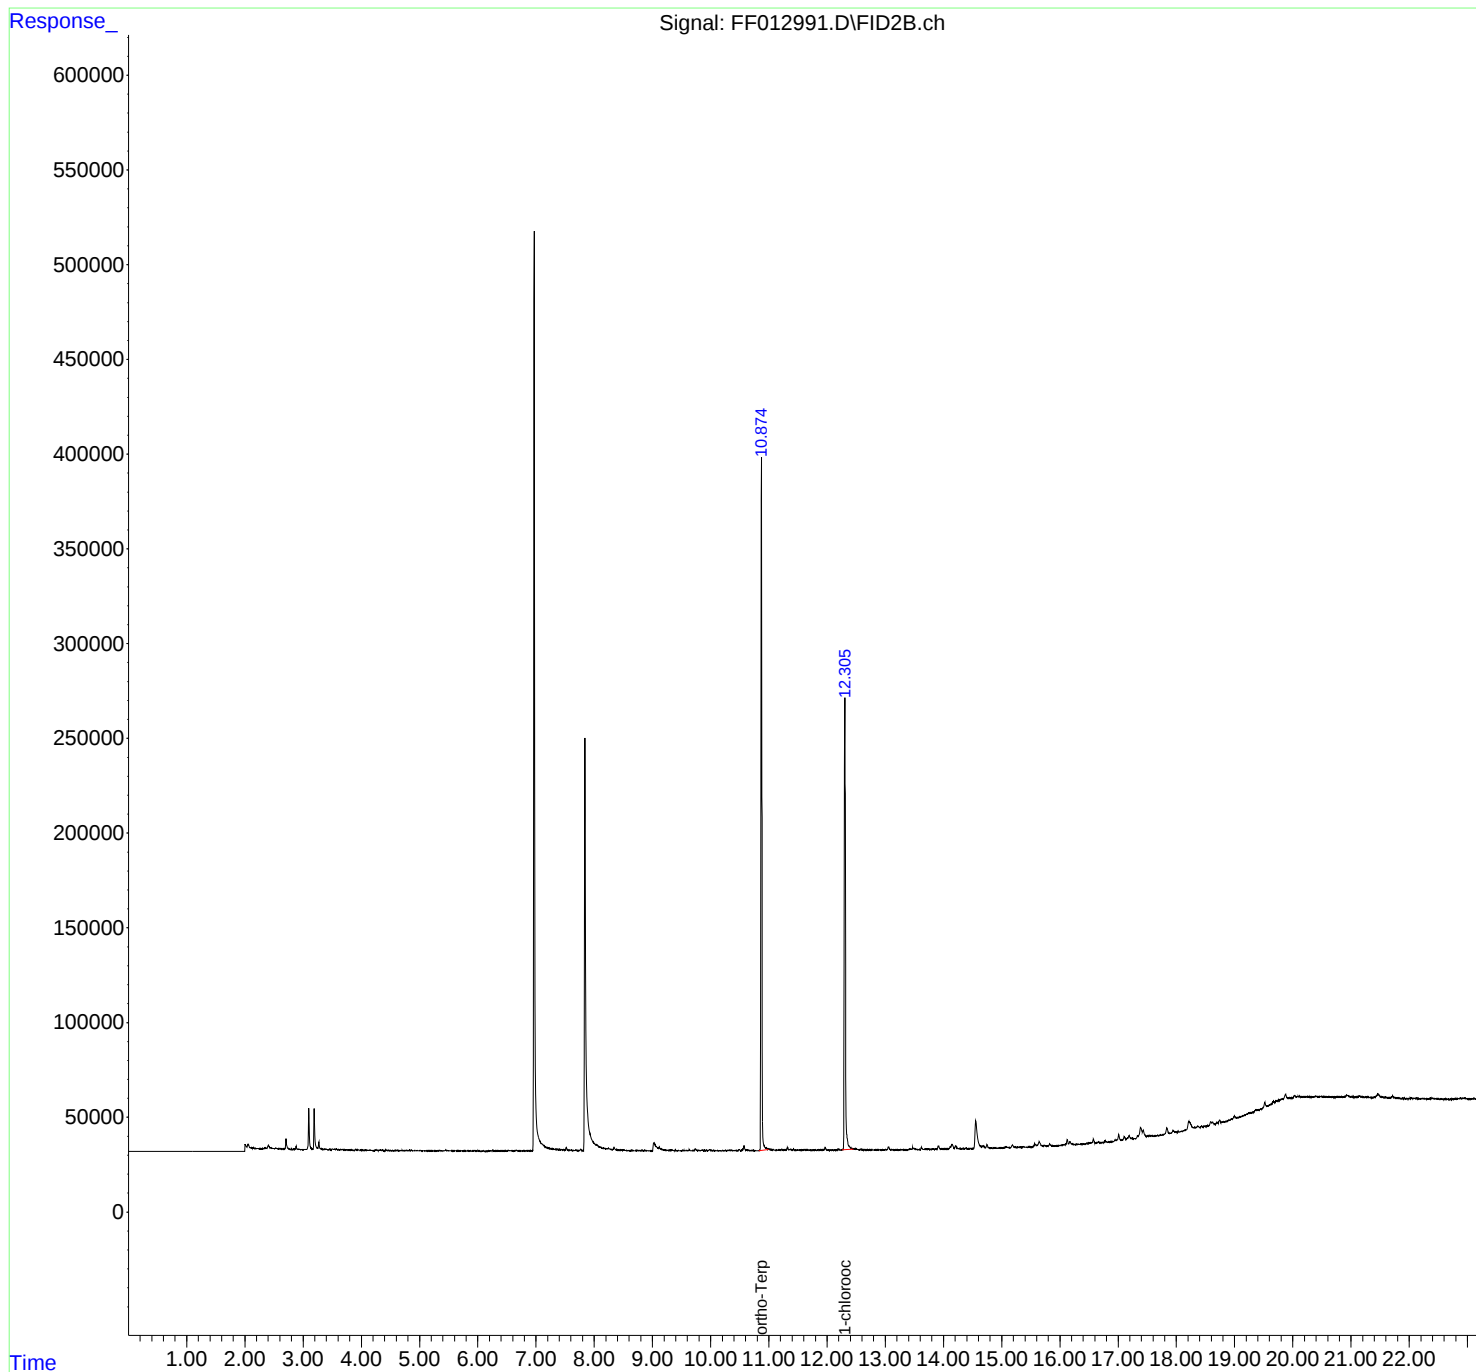


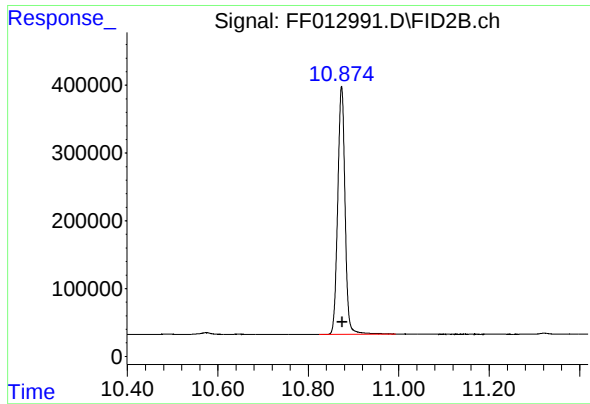

#9 ortho-Terphenyl (SURR)

R.T.: 10.874 min  
Delta R.T.: -0.002 min  
Response: 4100972  
Conc: 27.79 ug/ml

Instrument :  
FID\_F  
ClientSampleId :  
TP3-H

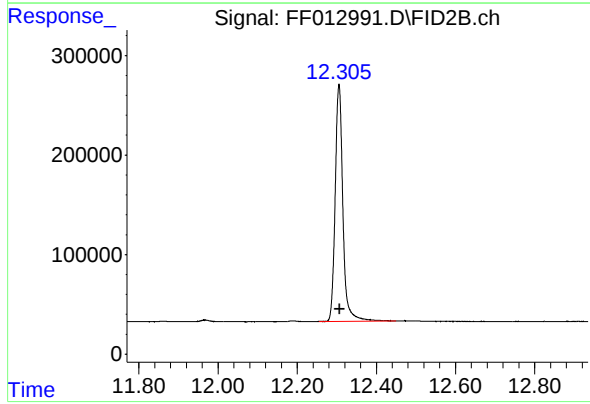

#12 1-chlorooctadecane (SURR)

R.T.: 12.306 min  
Delta R.T.: -0.001 min  
Response: 3217772  
Conc: 30.37 ug/ml