

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062422\
Data File : FF010839.D
Signal(s) : FID2B.ch
Acq On : 24 Jun 2022 08:38
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 24 23:39:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.728	234343	1.931 ug/ml
16)	N-HEXATRIACONTANE	20.276	143528	1.669 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062422\
Data File : FF010839.D
Signal(s) : FID2B.ch
Acq On : 24 Jun 2022 08:38
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 24 23:39:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

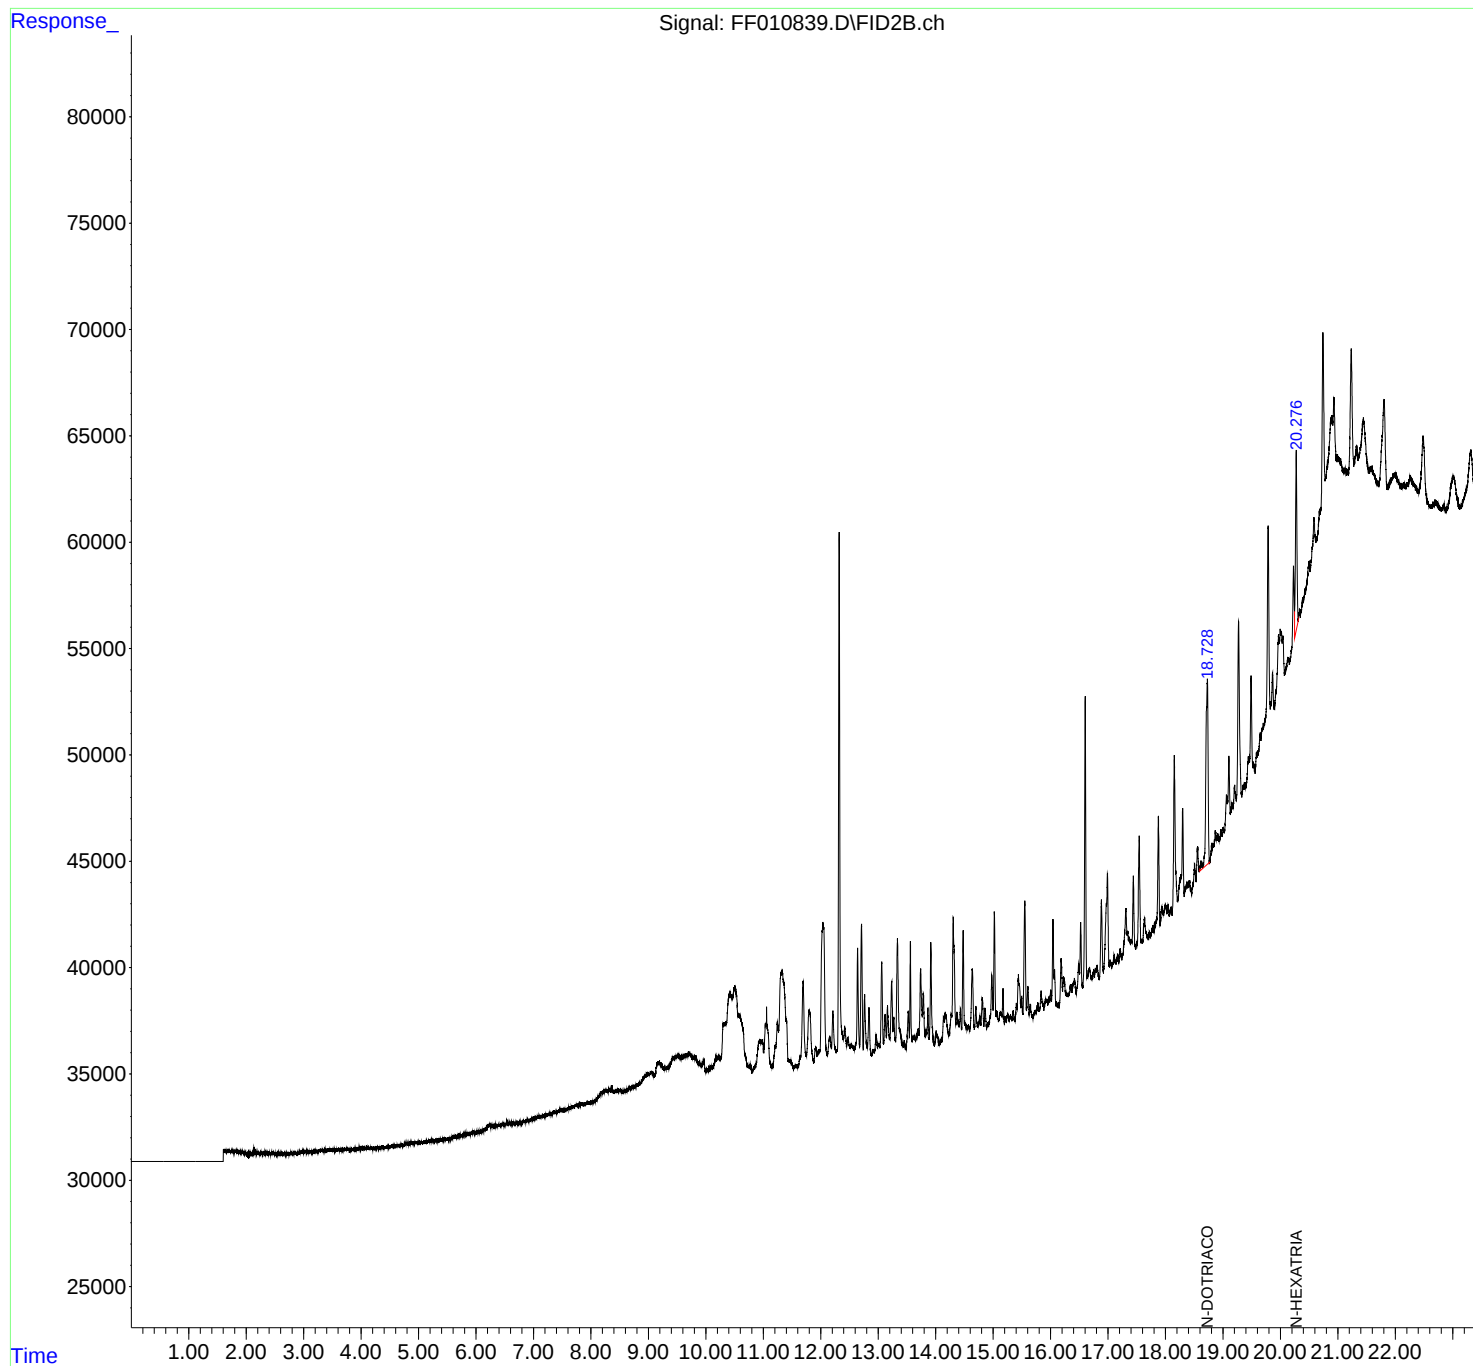


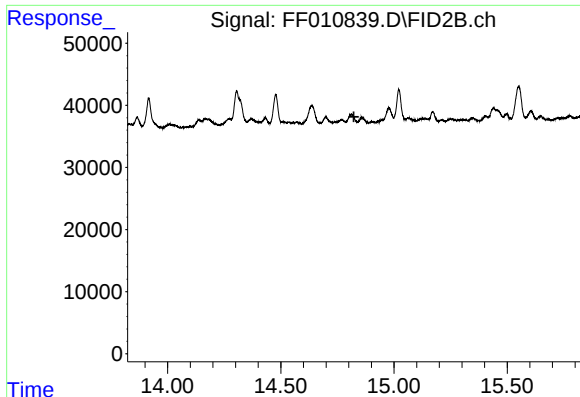

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.823 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

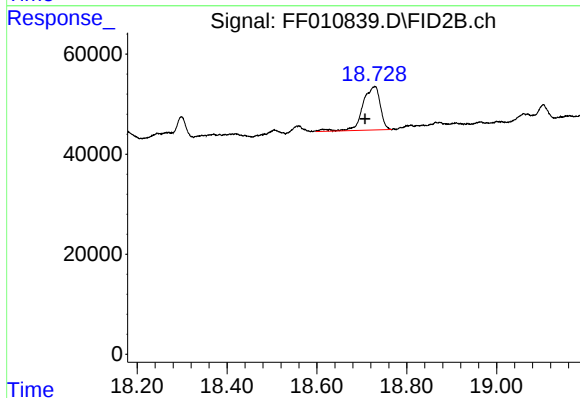

#14 N-DOTRIACONTANE

R.T.: 18.728 min
Delta R.T.: 0.021 min
Response: 234343
Conc: 1.93 ug/ml

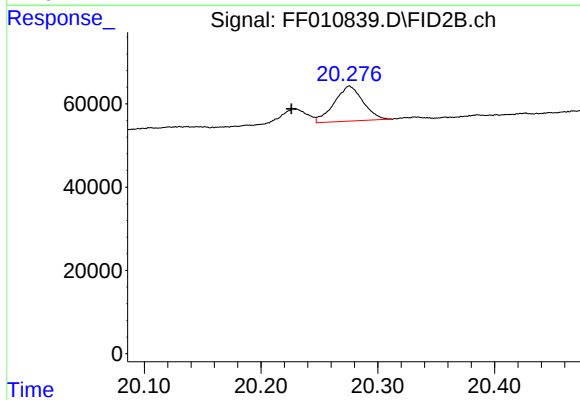

#16 N-HEXATRIACONTANE

R.T.: 20.276 min
Delta R.T.: 0.050 min
Response: 143528
Conc: 1.67 ug/ml