

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062422\
 Data File : FF010840.D
 Signal(s) : FID2B.ch
 Acq On : 24 Jun 2022 09:07
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 24 23:40:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
 Quant Title :
 QLast Update : Tue Jun 07 09:12:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.822	2522107	22.312 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.878	137508	1.122 ug/ml
14) N-DOTRIACONTANE	18.709	181163	1.493 ug/ml
15) N-TETRATRIACONTANE	19.491	126874	1.221 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062422\
Data File : FF010840.D
Signal(s) : FID2B.ch
Acq On : 24 Jun 2022 09:07
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 24 23:40:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

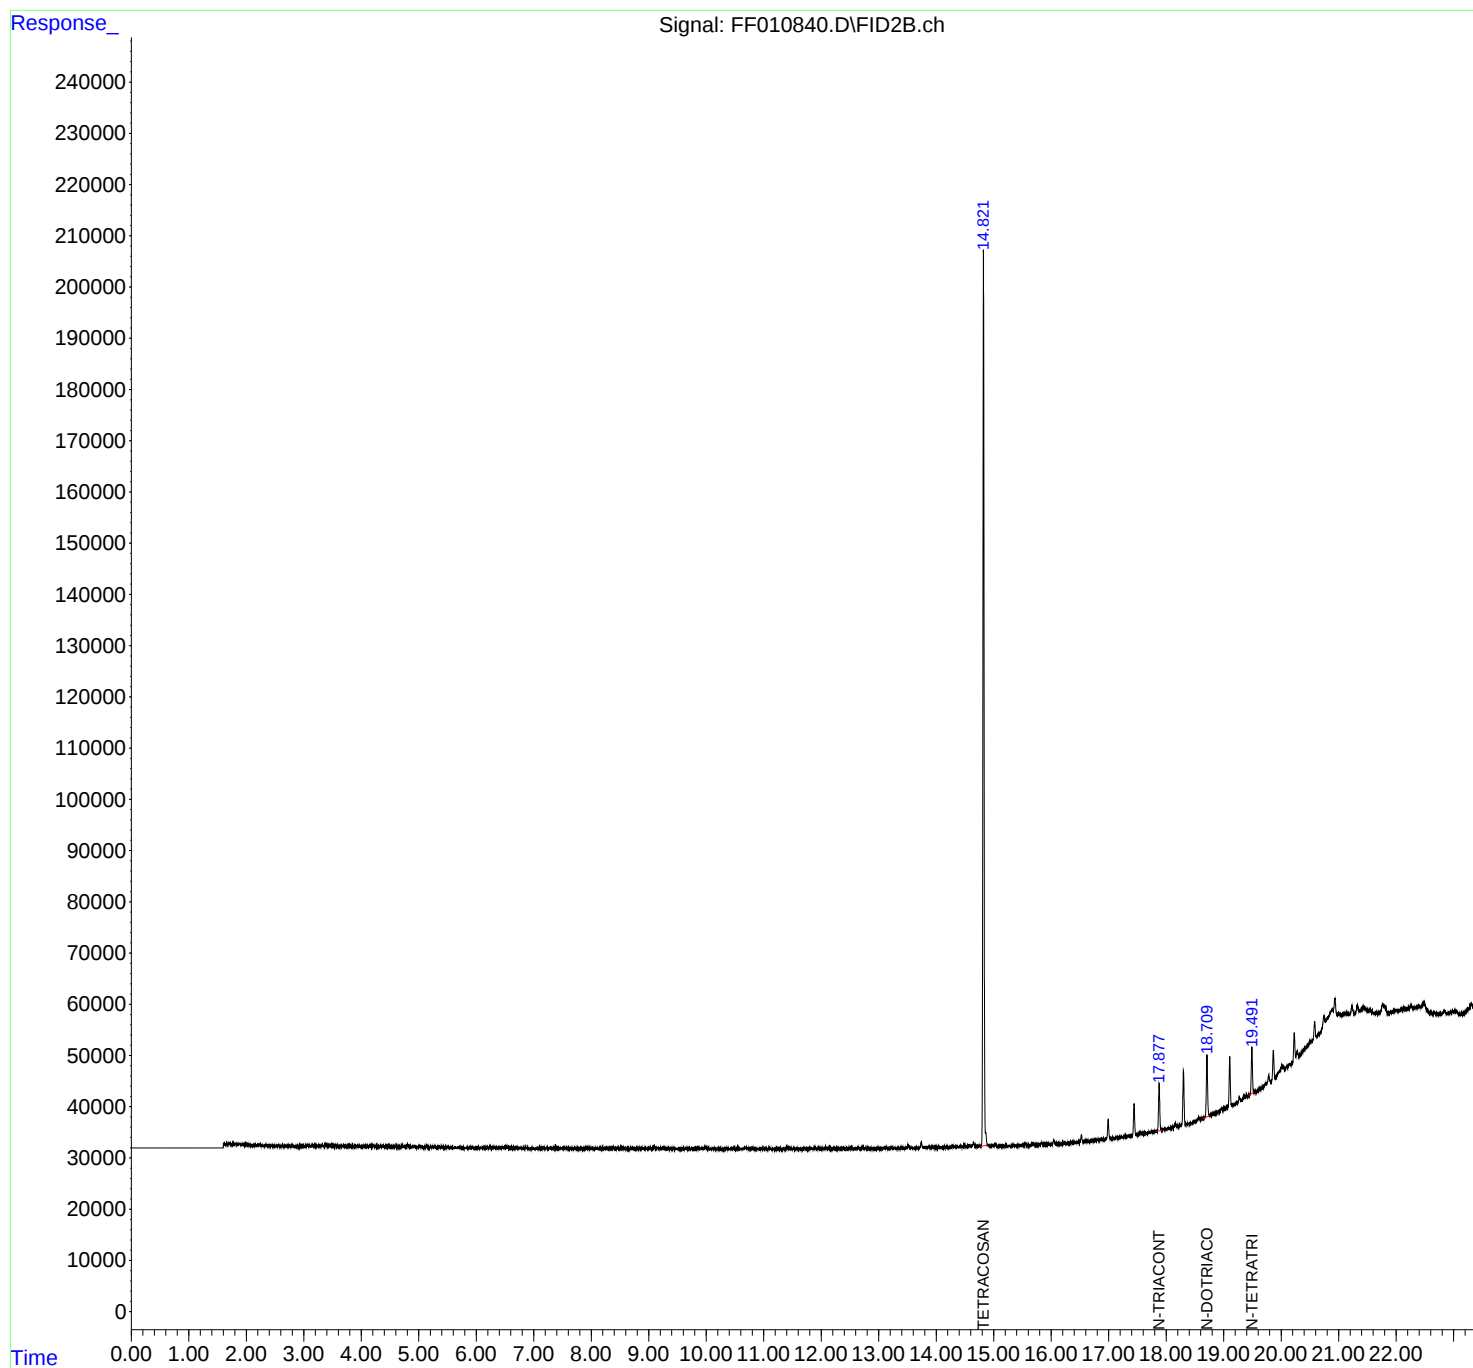


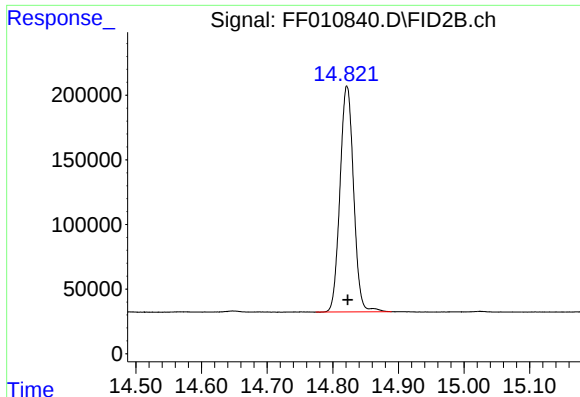

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.822 min
Delta R.T.: -0.001 min
Response: 2522107
Conc: 22.31 ug/ml

Instrument :
FID_F
ClientSampleId :

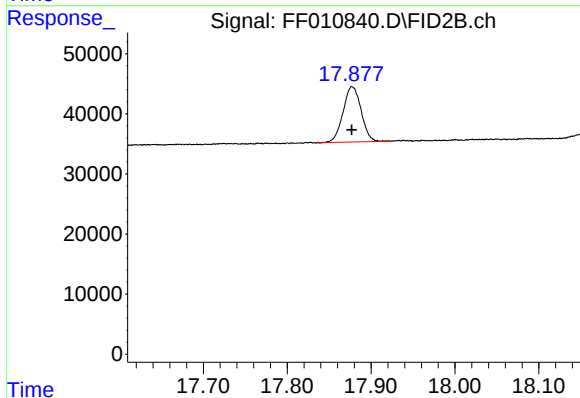


#13 N-TRIACONTANE

R.T.: 17.878 min
Delta R.T.: 0.000 min
Response: 137508
Conc: 1.12 ug/ml

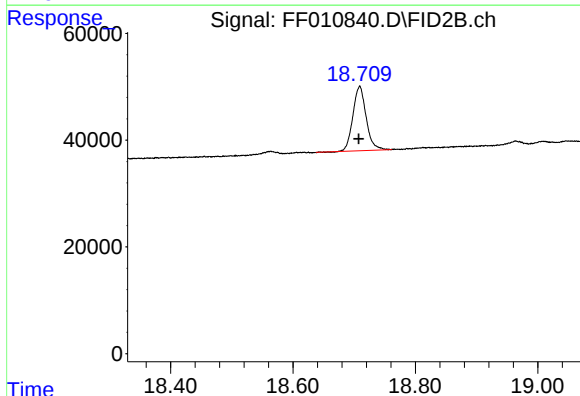

#14 N-DOTRIACONTANE

R.T.: 18.709 min
Delta R.T.: 0.001 min
Response: 181163
Conc: 1.49 ug/ml

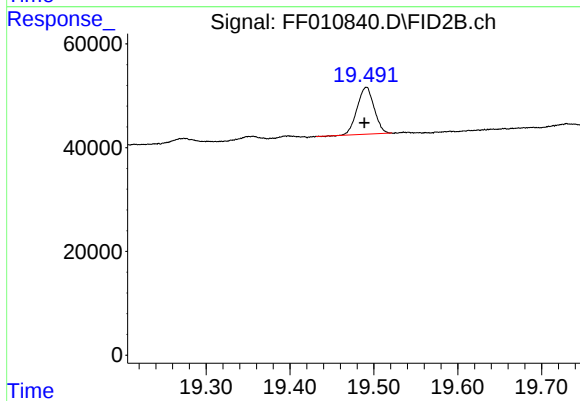

#15 N-TETRATRIACONTANE

R.T.: 19.491 min
Delta R.T.: 0.002 min
Response: 126874
Conc: 1.22 ug/ml