

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF062422\  
Data File : FF010846.D  
Signal(s) : FID2B.ch  
Acq On : 24 Jun 2022 17:39  
Operator : AJ\MA  
Sample : PB145810BL  
Misc :  
ALS Vial : 55 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jun 24 23:43:43 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF060622.M  
Quant Title :  
QLast Update : Tue Jun 07 09:12:29 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.822 | 3980132  | 35.211 ug/ml |

Target Compounds  
-----

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF062422\  
Data File : FF010846.D  
Signal(s) : FID2B.ch  
Acq On : 24 Jun 2022 17:39  
Operator : AJ\MA  
Sample : PB145810BL  
Misc :  
ALS Vial : 55 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jun 24 23:43:43 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF060622.M  
Quant Title :  
QLast Update : Tue Jun 07 09:12:29 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

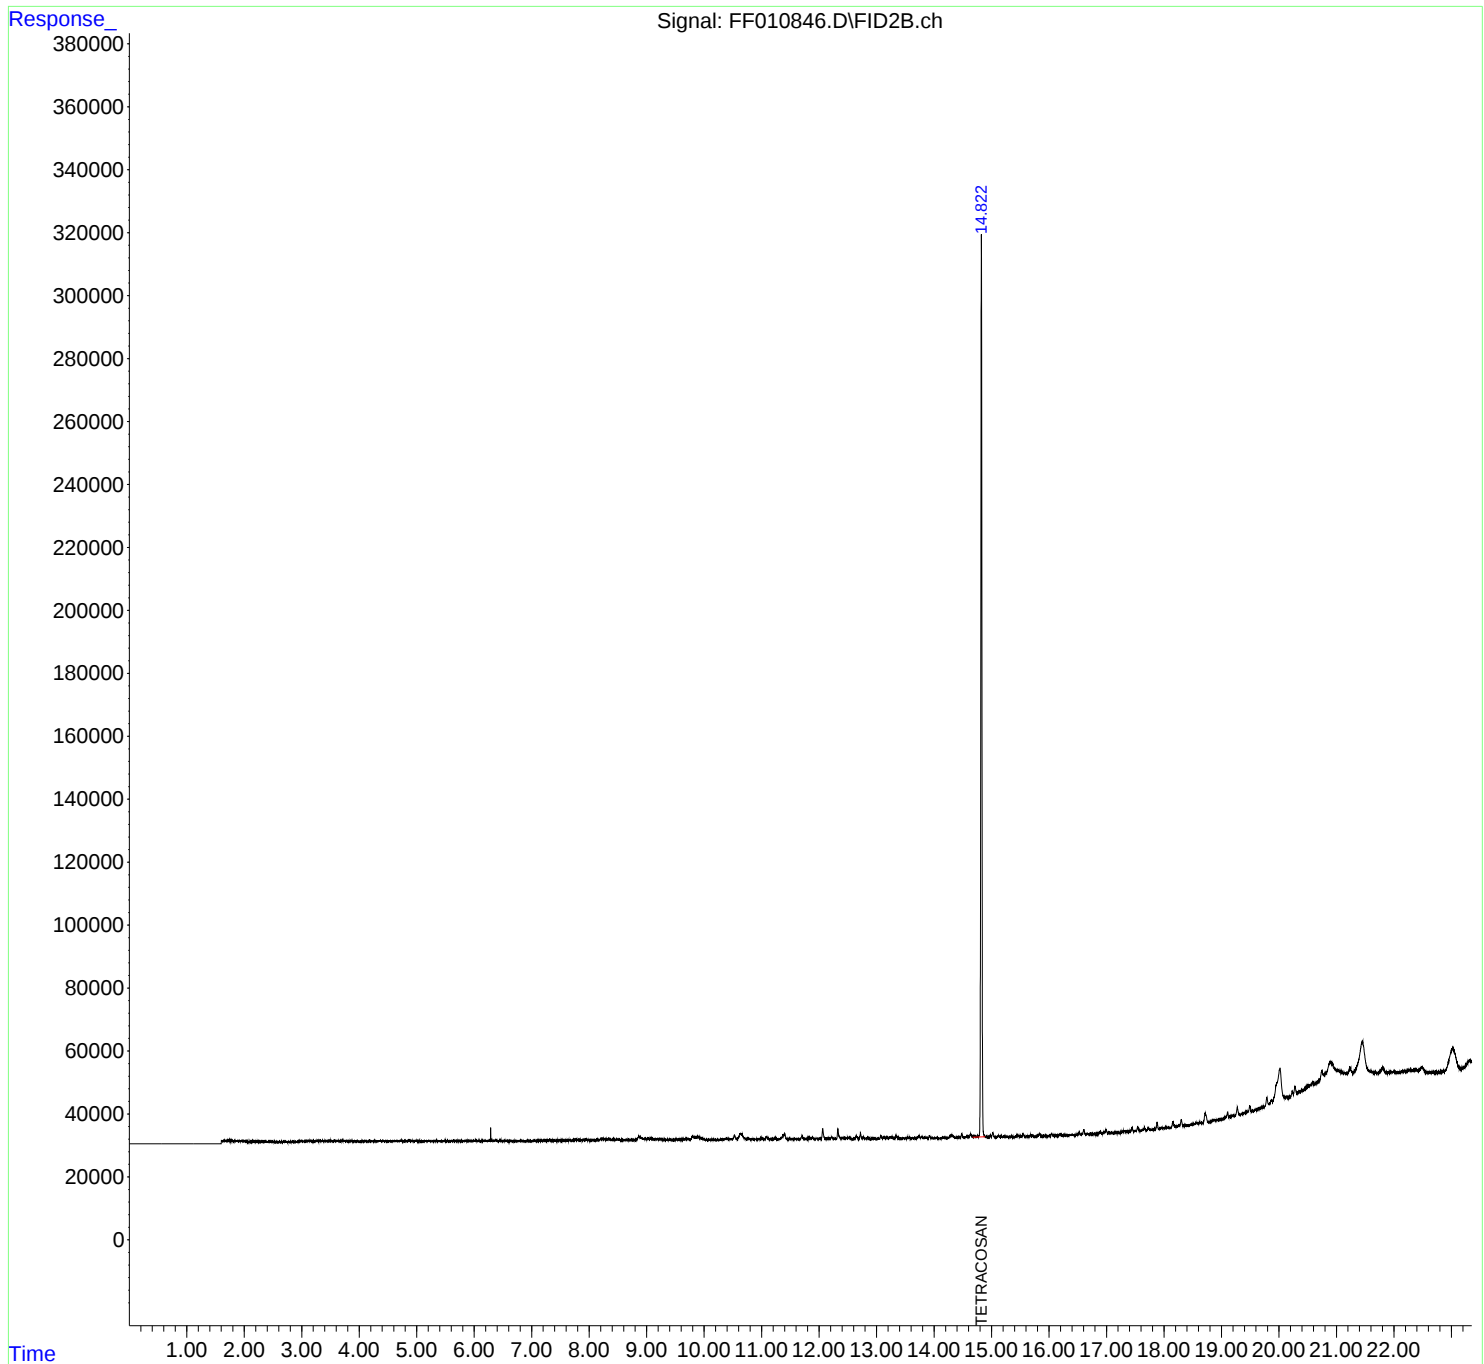

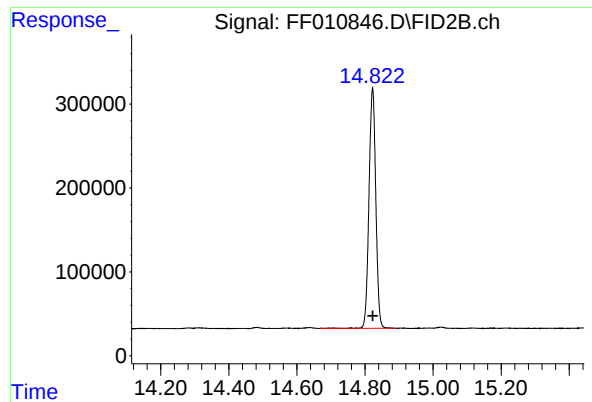

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.822 min  
Delta R.T.: 0.000 min  
Response: 3980132  
Conc: 35.21 ug/ml

Instrument :  
FID\_F  
ClientSampleId :