

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062422\
 Data File : FF010860.D
 Signal(s) : FID2B.ch
 Acq On : 25 Jun 2022 01:27
 Operator : AJ\MA
 Sample : N3455-01 10X
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 25 03:36:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
 Quant Title :
 QLast Update : Tue Jun 07 09:12:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.829	165569	1.465 ug/ml
Target Compounds			
6) N-OCTADECANE	11.441	136611	1.068 ug/ml
7) N-EICOSANE	12.744	302279	2.390 ug/ml
8) N-DOCOSANE	13.935	388699	3.078 ug/ml
11) N-HEXACOSANE	16.054	549427	4.338 ug/ml
12) N-OCTACOSANE	17.000	42070	0.345 ug/ml
14) N-DOTRIACONTANE	18.736	191915	1.582 ug/ml
16) N-HEXATRIACONTANE	20.285f	930541	10.820 ug/ml
18) N-TETRACONTANE	21.814f	816729	10.453 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062422\
Data File : FF010860.D
Signal(s) : FID2B.ch
Acq On : 25 Jun 2022 01:27
Operator : AJ\MA
Sample : N3455-01 10X
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 25 03:36:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

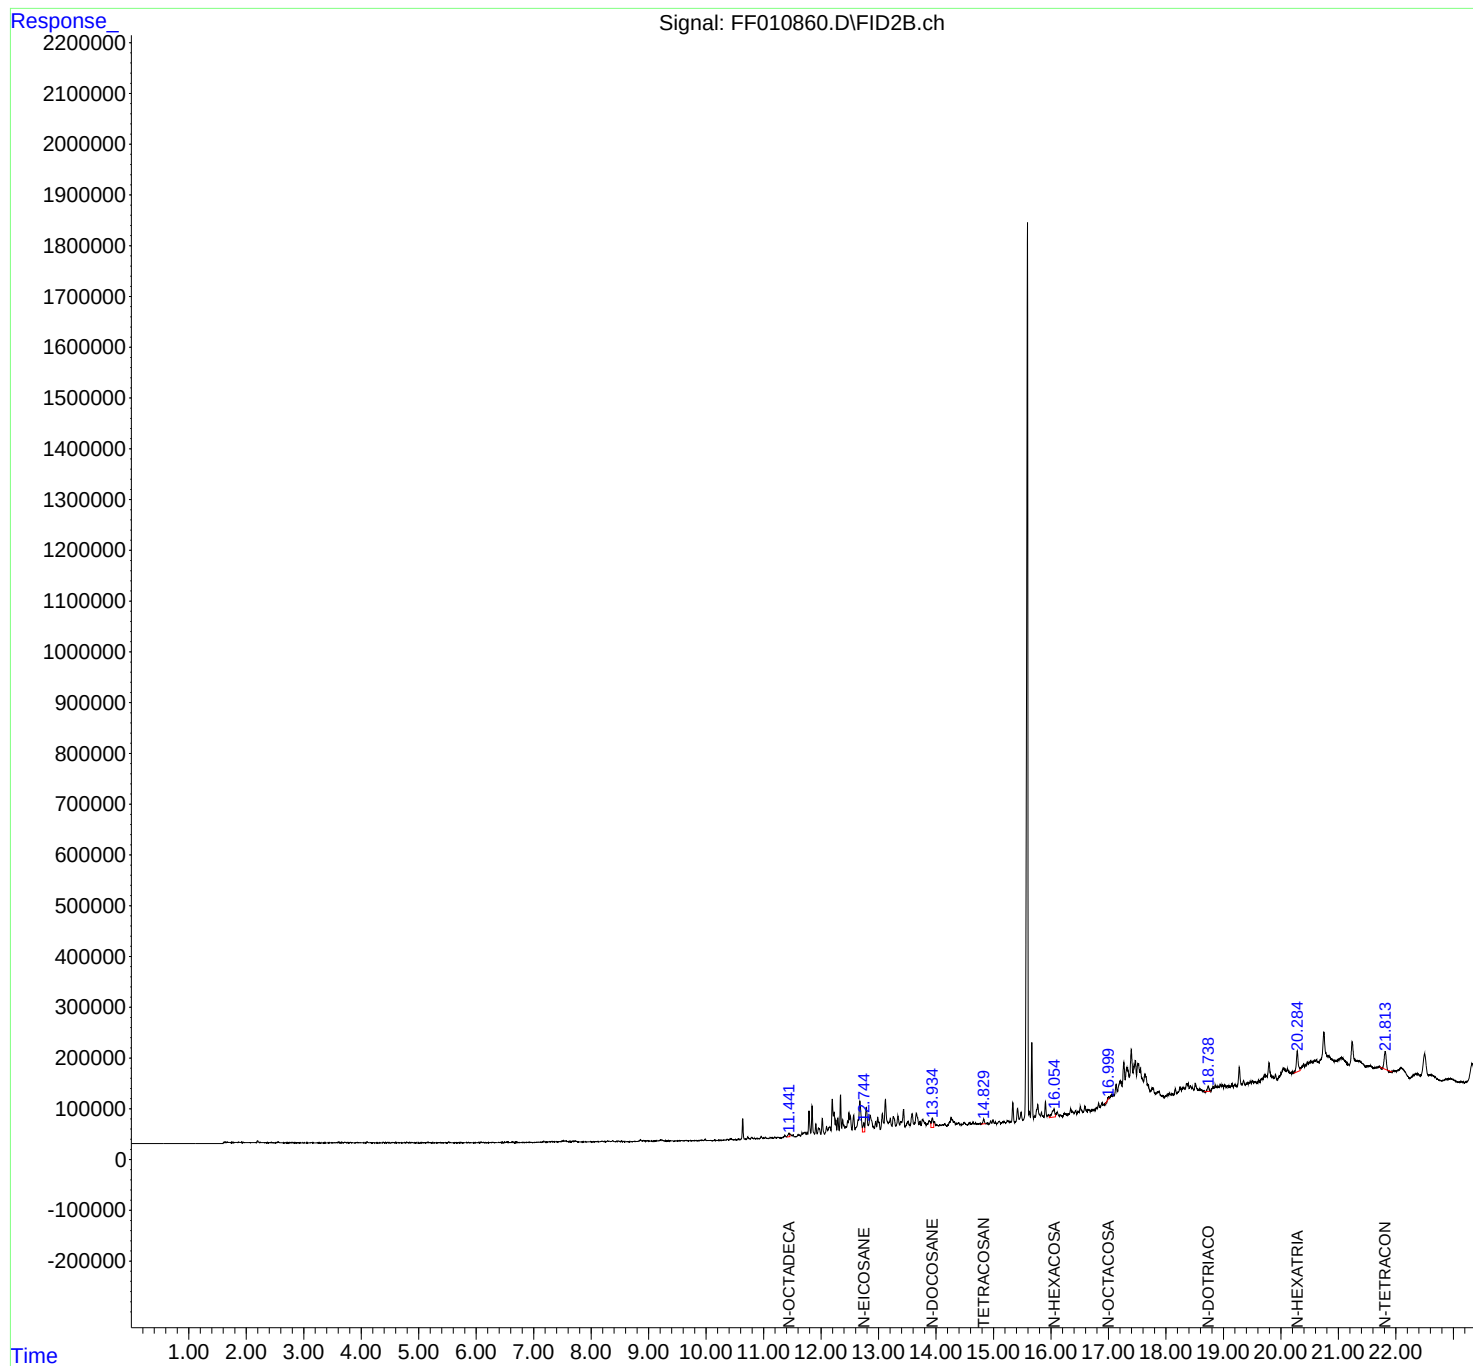


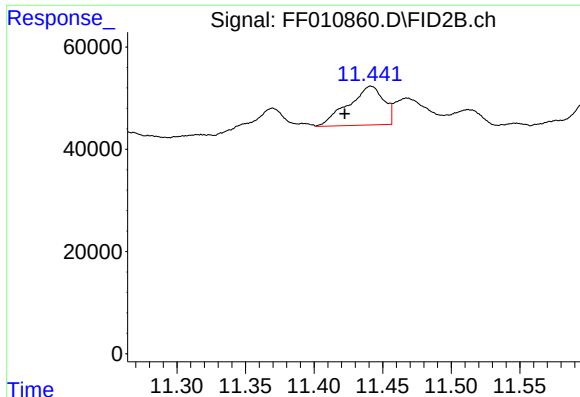

#6 N-OCTADECANE


R.T.: 11.441 min
Delta R.T.: 0.019 min
Response: 136611
Conc: 1.07 ug/ml

Instrument :
FID_F
ClientSampleId :

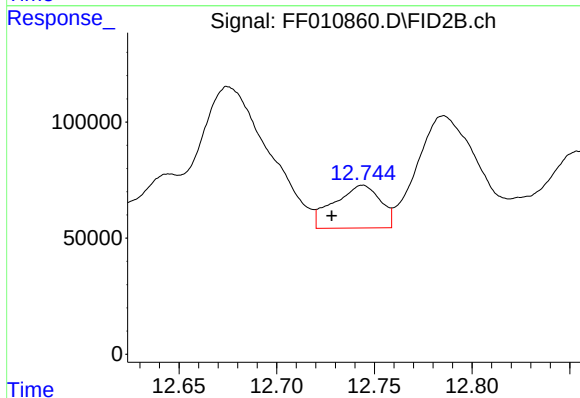


#7 N-EICOSANE

R.T.: 12.744 min
Delta R.T.: 0.016 min
Response: 302279
Conc: 2.39 ug/ml

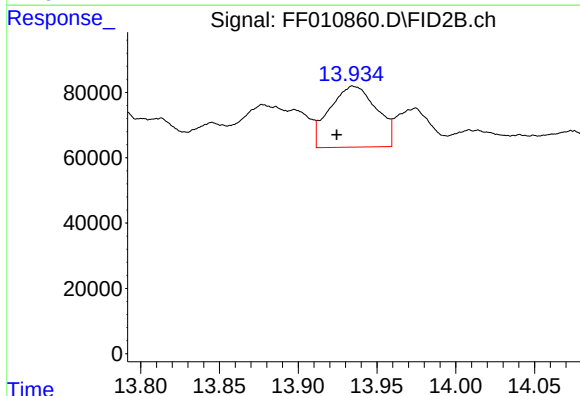


#8 N-DOCOSANE

R.T.: 13.935 min
Delta R.T.: 0.011 min
Response: 388699
Conc: 3.08 ug/ml

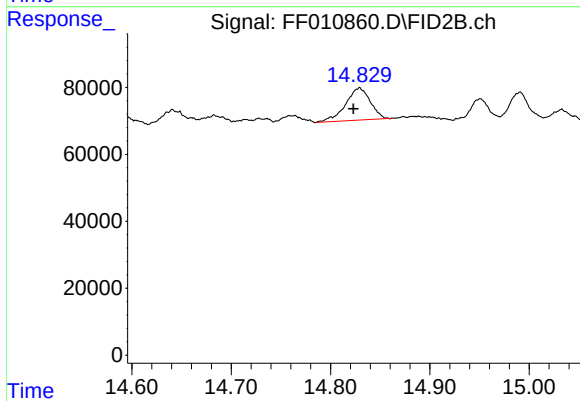

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.829 min
Delta R.T.: 0.006 min
Response: 165569
Conc: 1.46 ug/ml

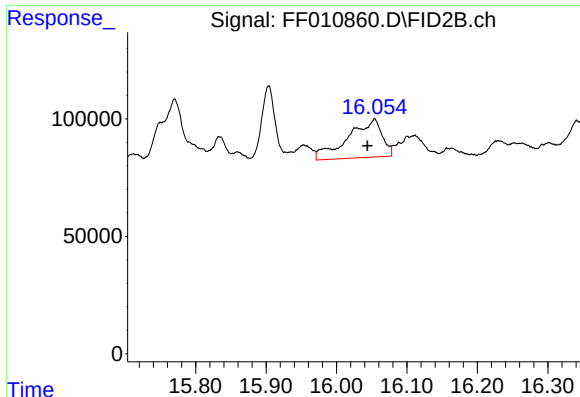

#11 N-HEXACOSANE


R.T.: 16.054 min
Delta R.T.: 0.010 min
Response: 549427
Conc: 4.34 ug/ml

Instrument :
FID_F
ClientSampleId :

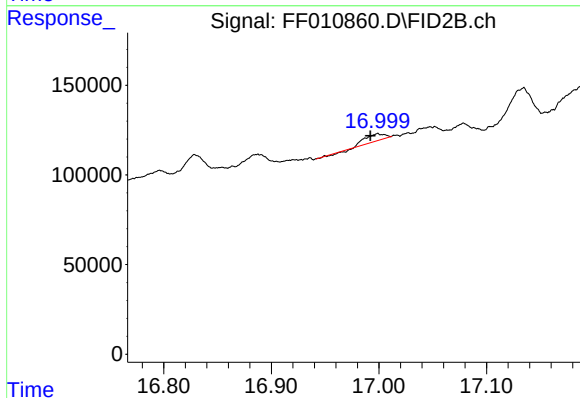


#12 N-OCTACOSANE

R.T.: 17.000 min
Delta R.T.: 0.007 min
Response: 42070
Conc: 0.34 ug/ml

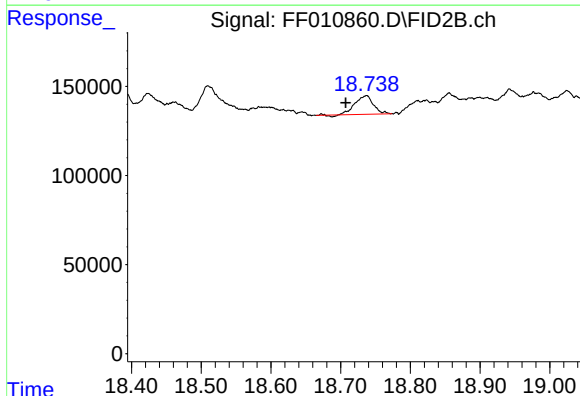


#14 N-DOTRIACONTANE

R.T.: 18.736 min
Delta R.T.: 0.029 min
Response: 191915
Conc: 1.58 ug/ml

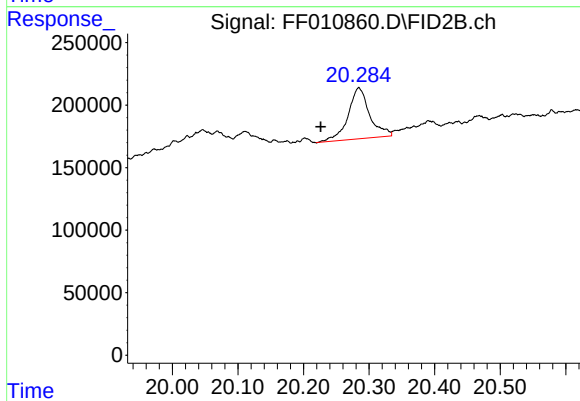

#16 N-HEXATRIACONTANE

R.T.: 20.285 min
Delta R.T.: 0.059 min
Response: 930541
Conc: 10.82 ug/ml

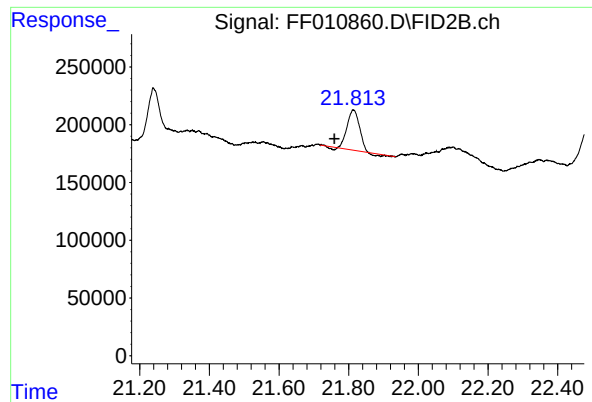

#18 N-TETRACONTANE

R.T.: 21.814 min
Delta R.T.: 0.054 min
Response: 816729
Conc: 10.45 ug/ml

Instrument :

FID_F

ClientSampleId :