

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062422\
 Data File : FF010862.D
 Signal(s) : FID2B.ch
 Acq On : 25 Jun 2022 02:26
 Operator : AJ\MA
 Sample : N3455-13 10X
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 25 03:37:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
 Quant Title :
 QLast Update : Tue Jun 07 09:12:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.628f	184212	1.516 ug/ml
4) N-TETRADECANE	8.347	476930	3.847 ug/ml
5) N-HEXADECANE	9.982	317111	2.536 ug/ml
6) N-OCTADECANE	11.421	519480	4.060 ug/ml
7) N-EICOSANE	12.732	287171	2.271 ug/ml
8) N-DOCOSANE	13.933	246188	1.949 ug/ml
11) N-HEXACOSANE	16.054	90120	0.711 ug/ml
12) N-OCTACOSANE	17.012	222247	1.821 ug/ml
13) N-TRIACONTANE	17.880	162363	1.325 ug/ml
14) N-DOTRIACONTANE	18.733	164189	1.353 ug/ml
15) N-TETRATRIACONTANE	19.519	190111	1.829 ug/ml
16) N-HEXATRIACONTANE	20.285f	275601	3.205 ug/ml
18) N-TETRACONTANE	21.810f	448420	5.739 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062422\
Data File : FF010862.D
Signal(s) : FID2B.ch
Acq On : 25 Jun 2022 02:26
Operator : AJ\MA
Sample : N3455-13 10X
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 25 03:37:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

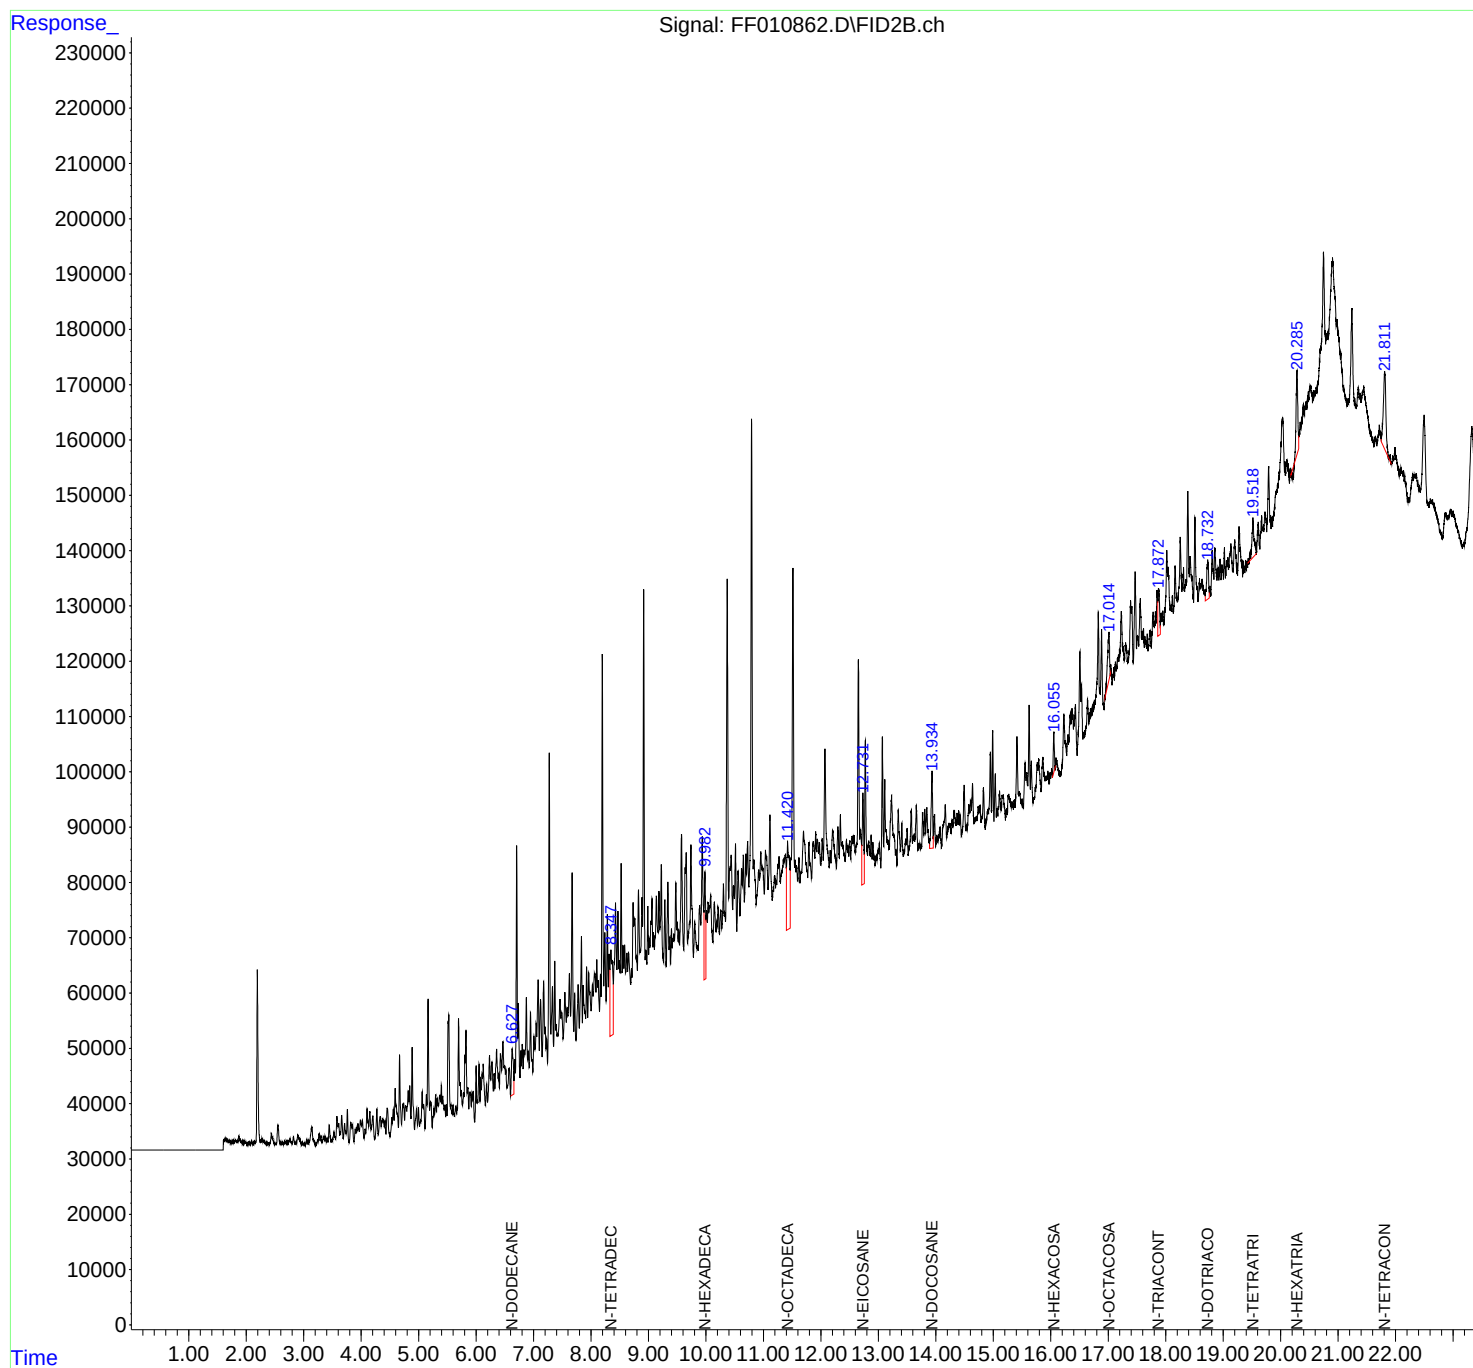


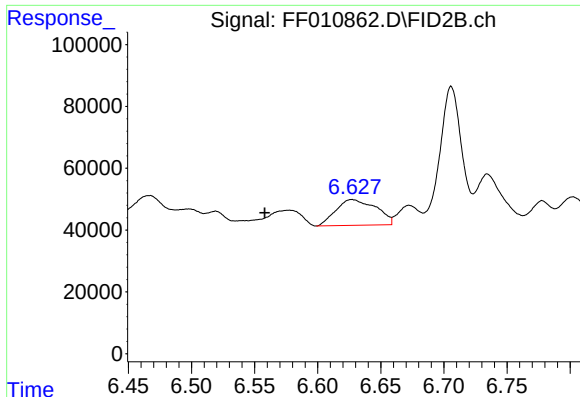

#3 N-DODECANE


R.T.: 6.628 min
Delta R.T.: 0.070 min
Response: 184212
Conc: 1.52 ug/ml

Instrument :
FID_F
ClientSampleId :

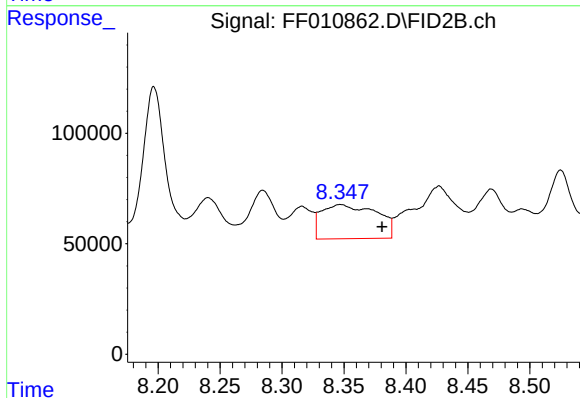


#4 N-TETRADECANE

R.T.: 8.347 min
Delta R.T.: -0.034 min
Response: 476930
Conc: 3.85 ug/ml

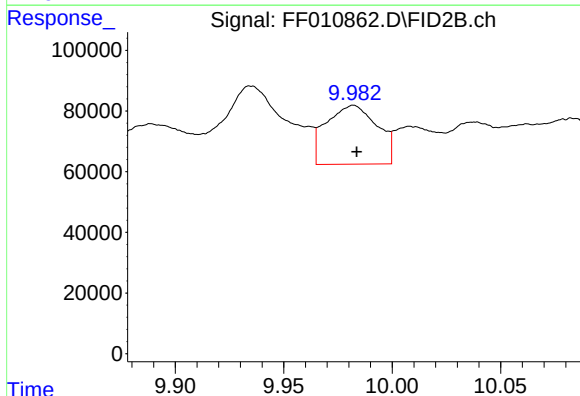


#5 N-HEXADECANE

R.T.: 9.982 min
Delta R.T.: -0.002 min
Response: 317111
Conc: 2.54 ug/ml

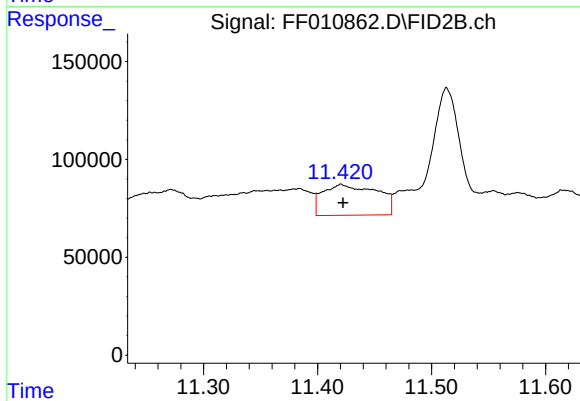

#6 N-OCTADECANE


R.T.: 11.421 min
Delta R.T.: -0.001 min
Response: 519480
Conc: 4.06 ug/ml

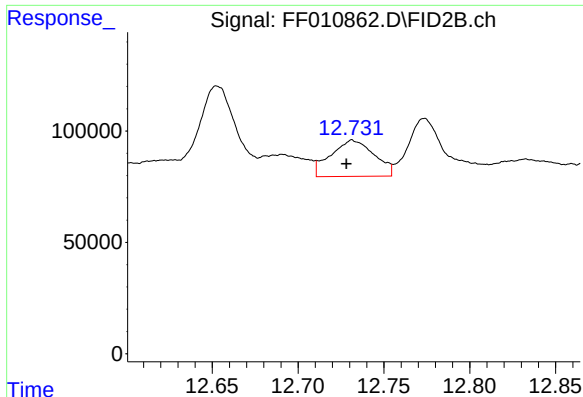

#7 N-EICOSANE


R.T.: 12.732 min
Delta R.T.: 0.004 min
Response: 287171
Conc: 2.27 ug/ml

Instrument :
FID_F
ClientSampleId :

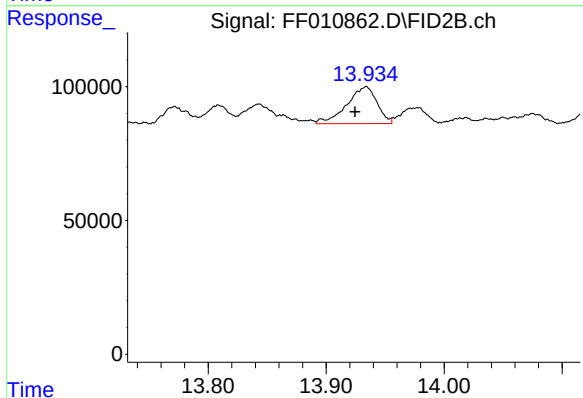


#8 N-DOCOSANE

R.T.: 13.933 min
Delta R.T.: 0.009 min
Response: 246188
Conc: 1.95 ug/ml

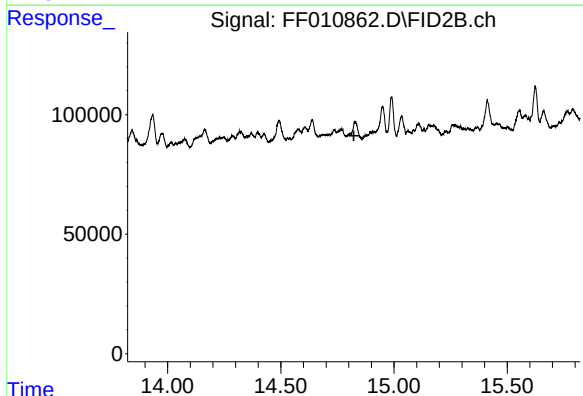


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.823 min
Response: 0
Conc: N.D.

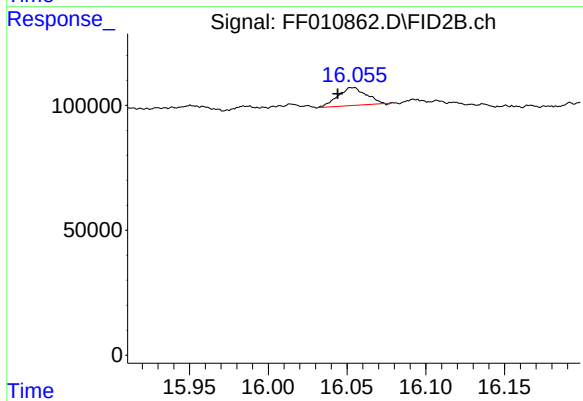

#11 N-HEXACOSANE


R.T.: 16.054 min
Delta R.T.: 0.009 min
Response: 90120
Conc: 0.71 ug/ml

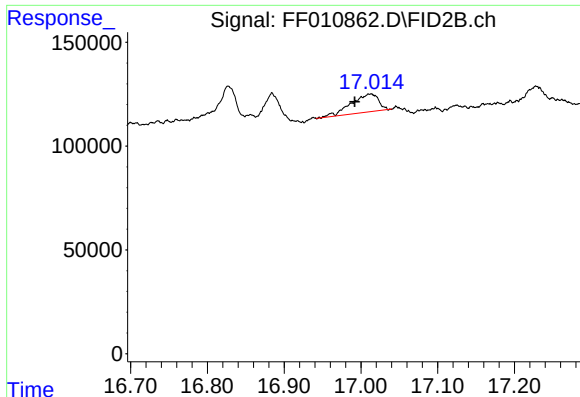

#12 N-OCTACOSANE


R.T.: 17.012 min
Delta R.T.: 0.020 min
Response: 222247
Conc: 1.82 ug/ml

Instrument :
FID_F
ClientSampleId :

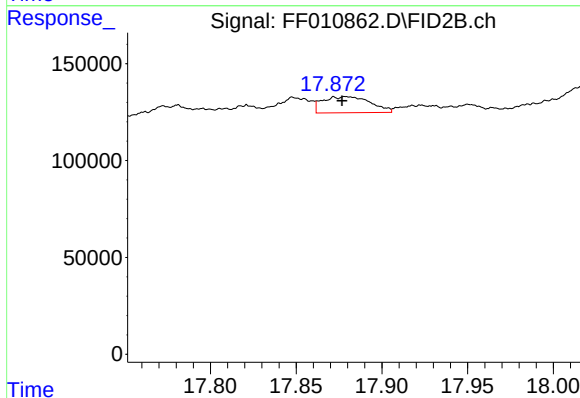


#13 N-TRIACONTANE

R.T.: 17.880 min
Delta R.T.: 0.003 min
Response: 162363
Conc: 1.32 ug/ml

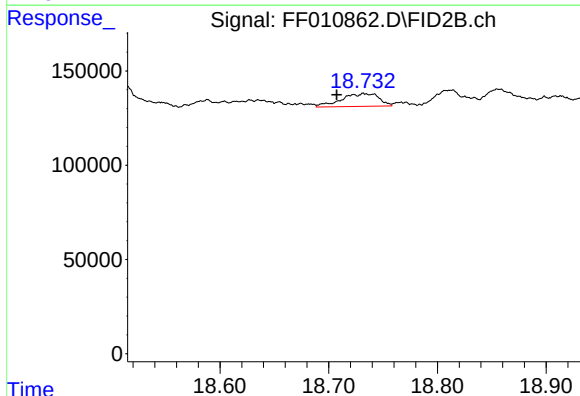


#14 N-DOTRIACONTANE

R.T.: 18.733 min
Delta R.T.: 0.026 min
Response: 164189
Conc: 1.35 ug/ml

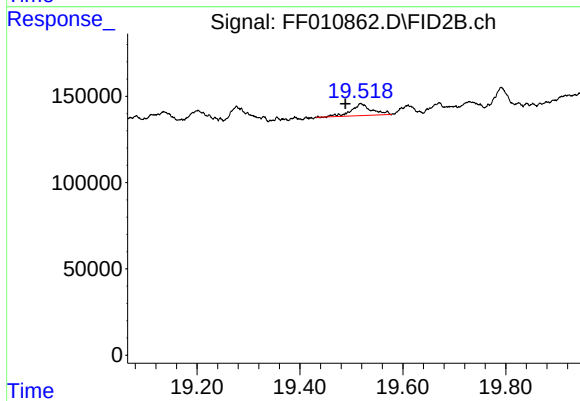

#15 N-TETRATRIACONTANE


R.T.: 19.519 min
Delta R.T.: 0.030 min
Response: 190111
Conc: 1.83 ug/ml

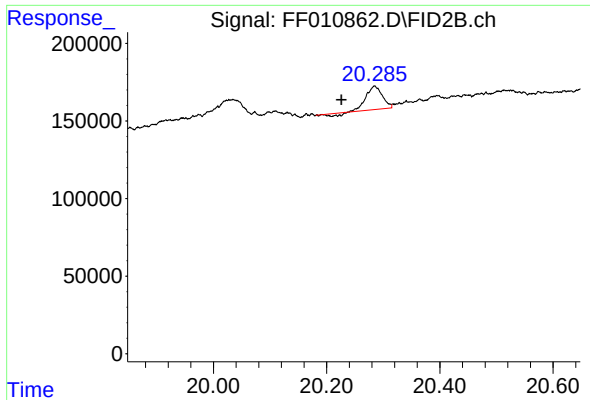

#16 N-HEXATRIACONTANE

R.T.: 20.285 min
Delta R.T.: 0.059 min
Response: 275601
Conc: 3.20 ug/ml

Instrument :
FID_F
ClientSampleId :

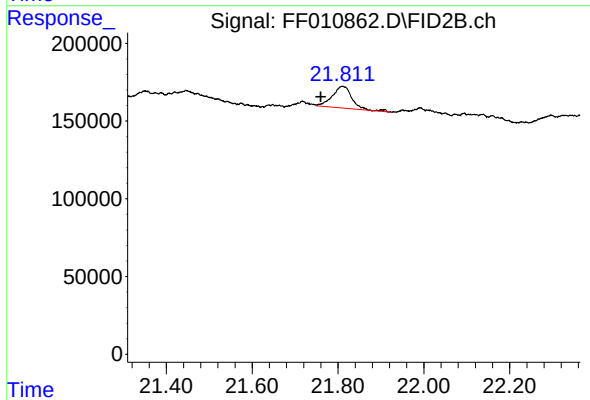

#18 N-TETRACONTANE

R.T.: 21.810 min
Delta R.T.: 0.051 min
Response: 448420
Conc: 5.74 ug/ml