

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062423\
 Data File : FF012994.D
 Signal(s) : FID2B.ch
 Acq On : 24 Jun 2023 13:42
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 25 03:43:59 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062423.M
 Quant Title :
 QLast Update : Sun Jun 25 03:41:21 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
10) N-TETRACOSANE	15.135	78679	0.514 ug/ml
14) N-DOTRIACONTANE	18.835	57277	0.399 ug/ml
15) N-TETRATRIACONTANE	19.616	74835	0.537 ug/ml
17) N-OCTATRIACONTANE	21.076	53621	0.402 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062423\
Data File : FF012994.D
Signal(s) : FID2B.ch
Acq On : 24 Jun 2023 13:42
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 25 03:43:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062423.M
Quant Title :
QLast Update : Sun Jun 25 03:41:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

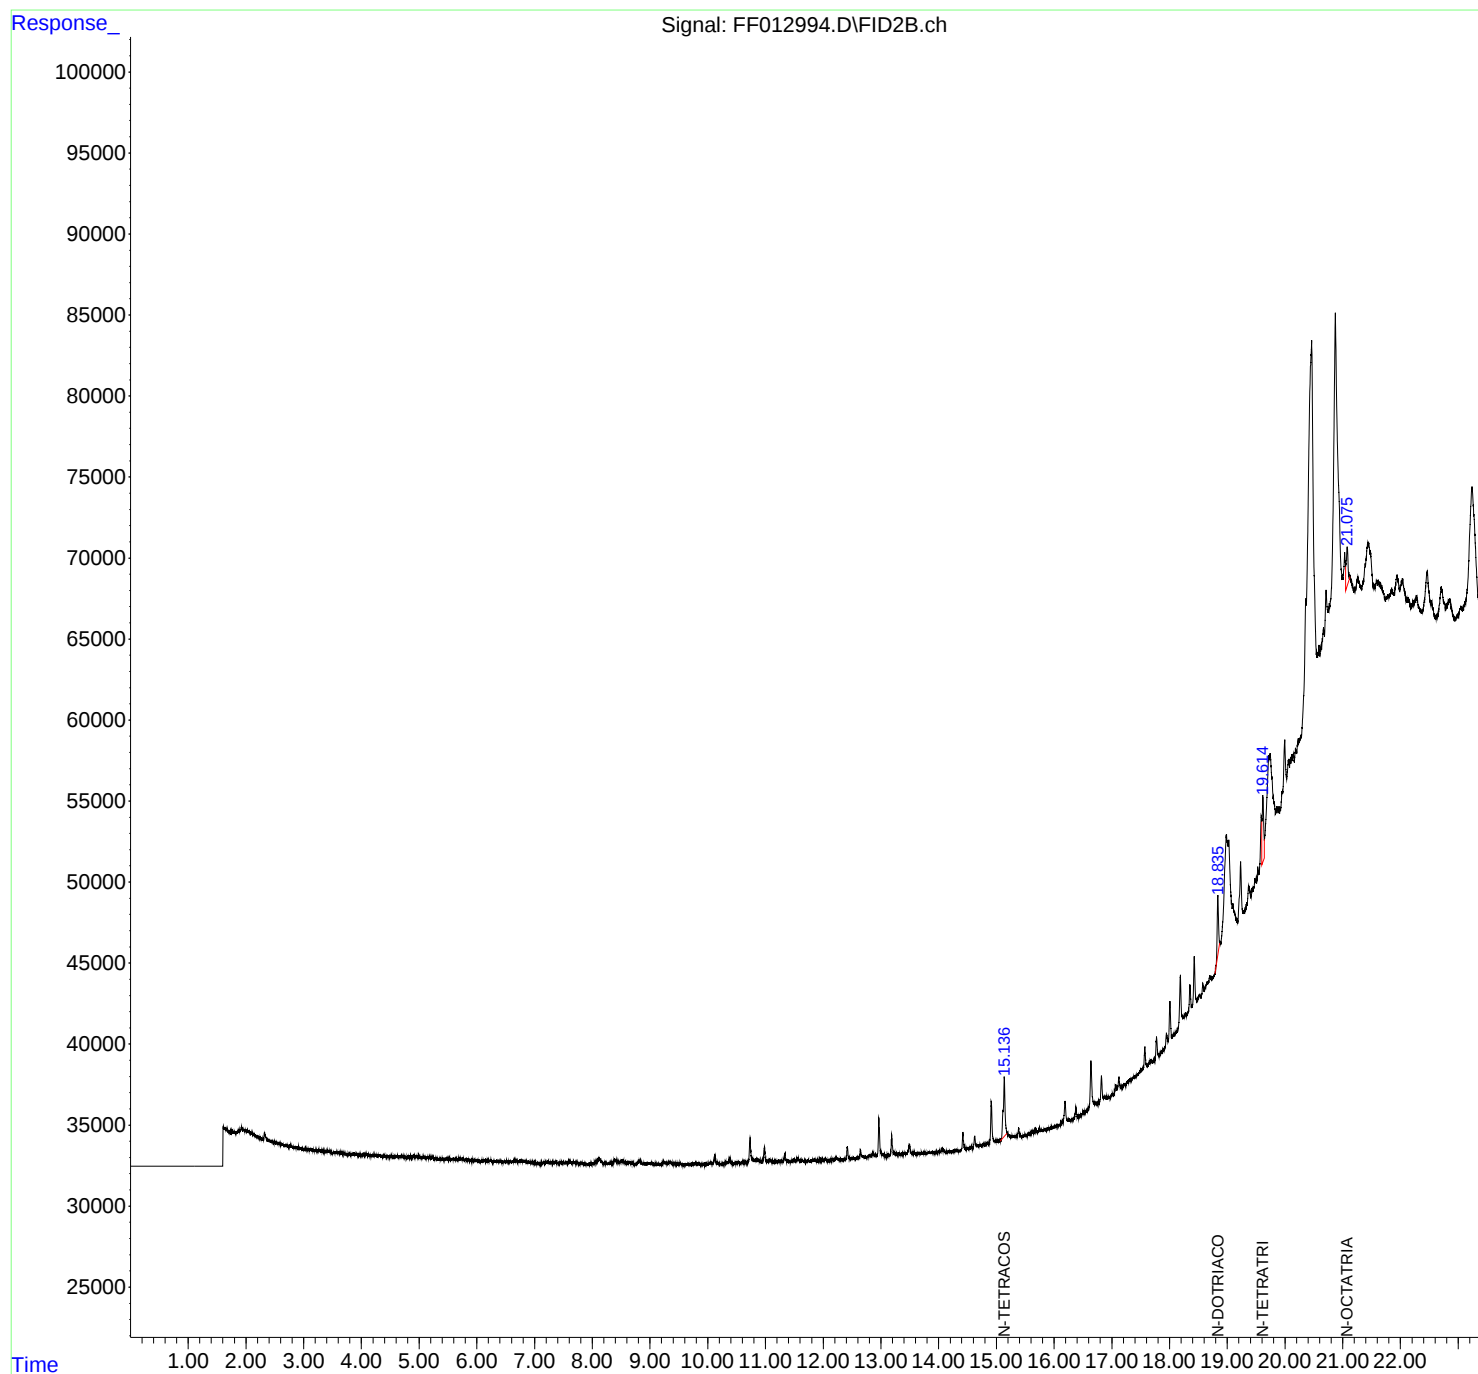


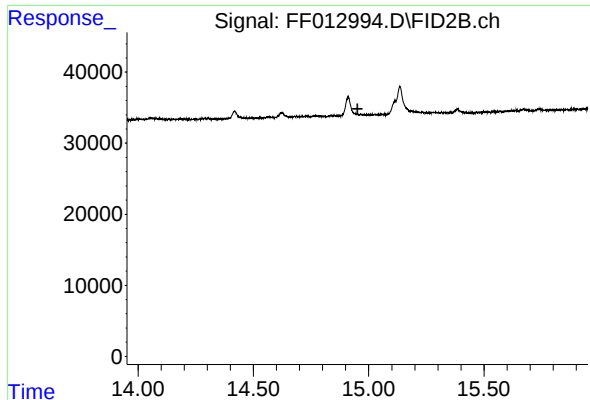

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.952 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

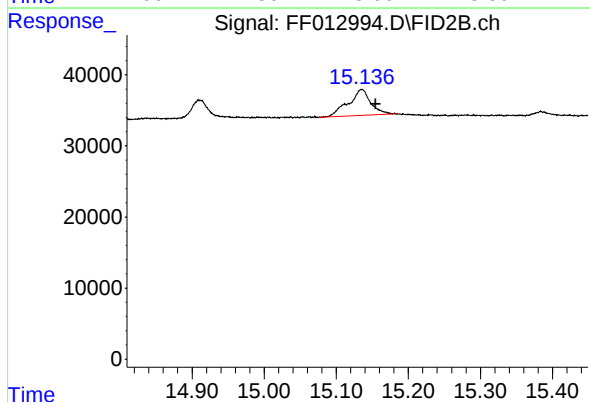


#10 N-TETRACOSANE

R.T.: 15.135 min
Delta R.T.: -0.019 min
Response: 78679
Conc: 0.51 ug/ml

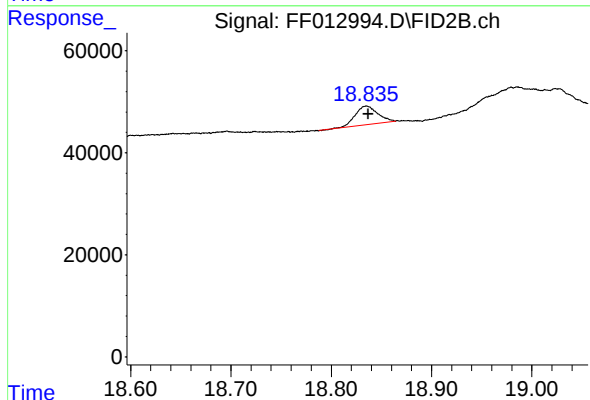


#14 N-DOTRIACONTANE

R.T.: 18.835 min
Delta R.T.: -0.002 min
Response: 57277
Conc: 0.40 ug/ml

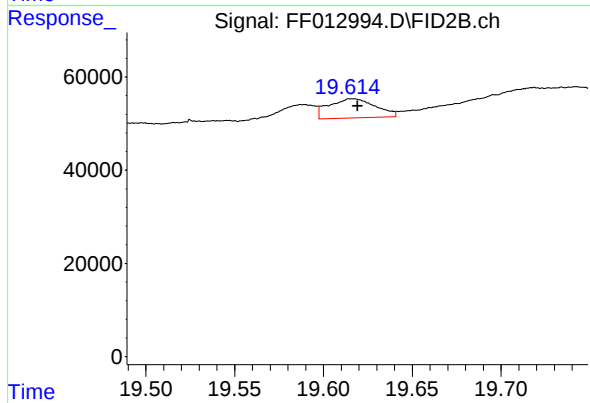

#15 N-TETRATRIACONTANE

R.T.: 19.616 min
Delta R.T.: -0.003 min
Response: 74835
Conc: 0.54 ug/ml

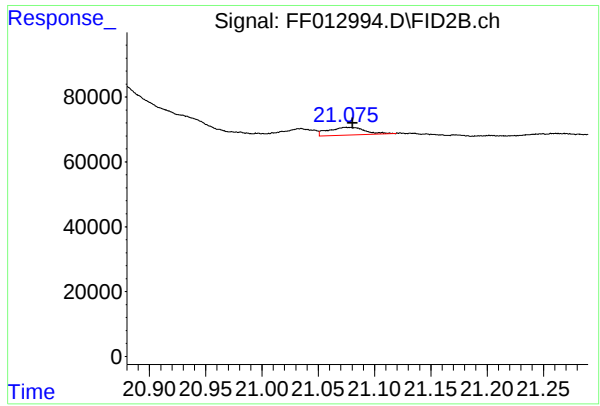

#17 N-OCTATRIACONTANE

R.T.: 21.076 min
Delta R.T.: -0.004 min
Response: 53621
Conc: 0.40 ug/ml

Instrument :
FID_F
ClientSampleId :