

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062518\
 Data File : FF001100.D
 Signal(s) : FID2B.ch
 Acq On : 25 Jun 2018 11:55
 Operator : UA\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jun 26 01:47:19 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.475	6279397	54.450 ug/ml
Target Compounds			
2) N-DECANE	4.239	8942953	63.825 ug/ml
3) N-DODECANE	6.252	8514646	60.753 ug/ml
4) N-TETRADECANE	8.040	8112841	58.269 ug/ml
5) N-HEXADECANE	9.636	7797635	56.555 ug/ml
6) N-OCTADECANE	11.075	7577757	55.493 ug/ml
7) N-EICOSANE	12.382	7346428	54.833 ug/ml
8) N-DOCOSANE	13.578	7211397	54.538 ug/ml
10) N-TETRACOSANE	14.679	7145563	55.089 ug/ml
11) N-HEXACOSANE	15.698	7124421	55.467 ug/ml
12) N-OCTACOSANE	16.648	7163348	56.334 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062518\
Data File : FF001100.D
Signal(s) : FID2B.ch
Acq On : 25 Jun 2018 11:55
Operator : UA\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 26 01:47:19 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

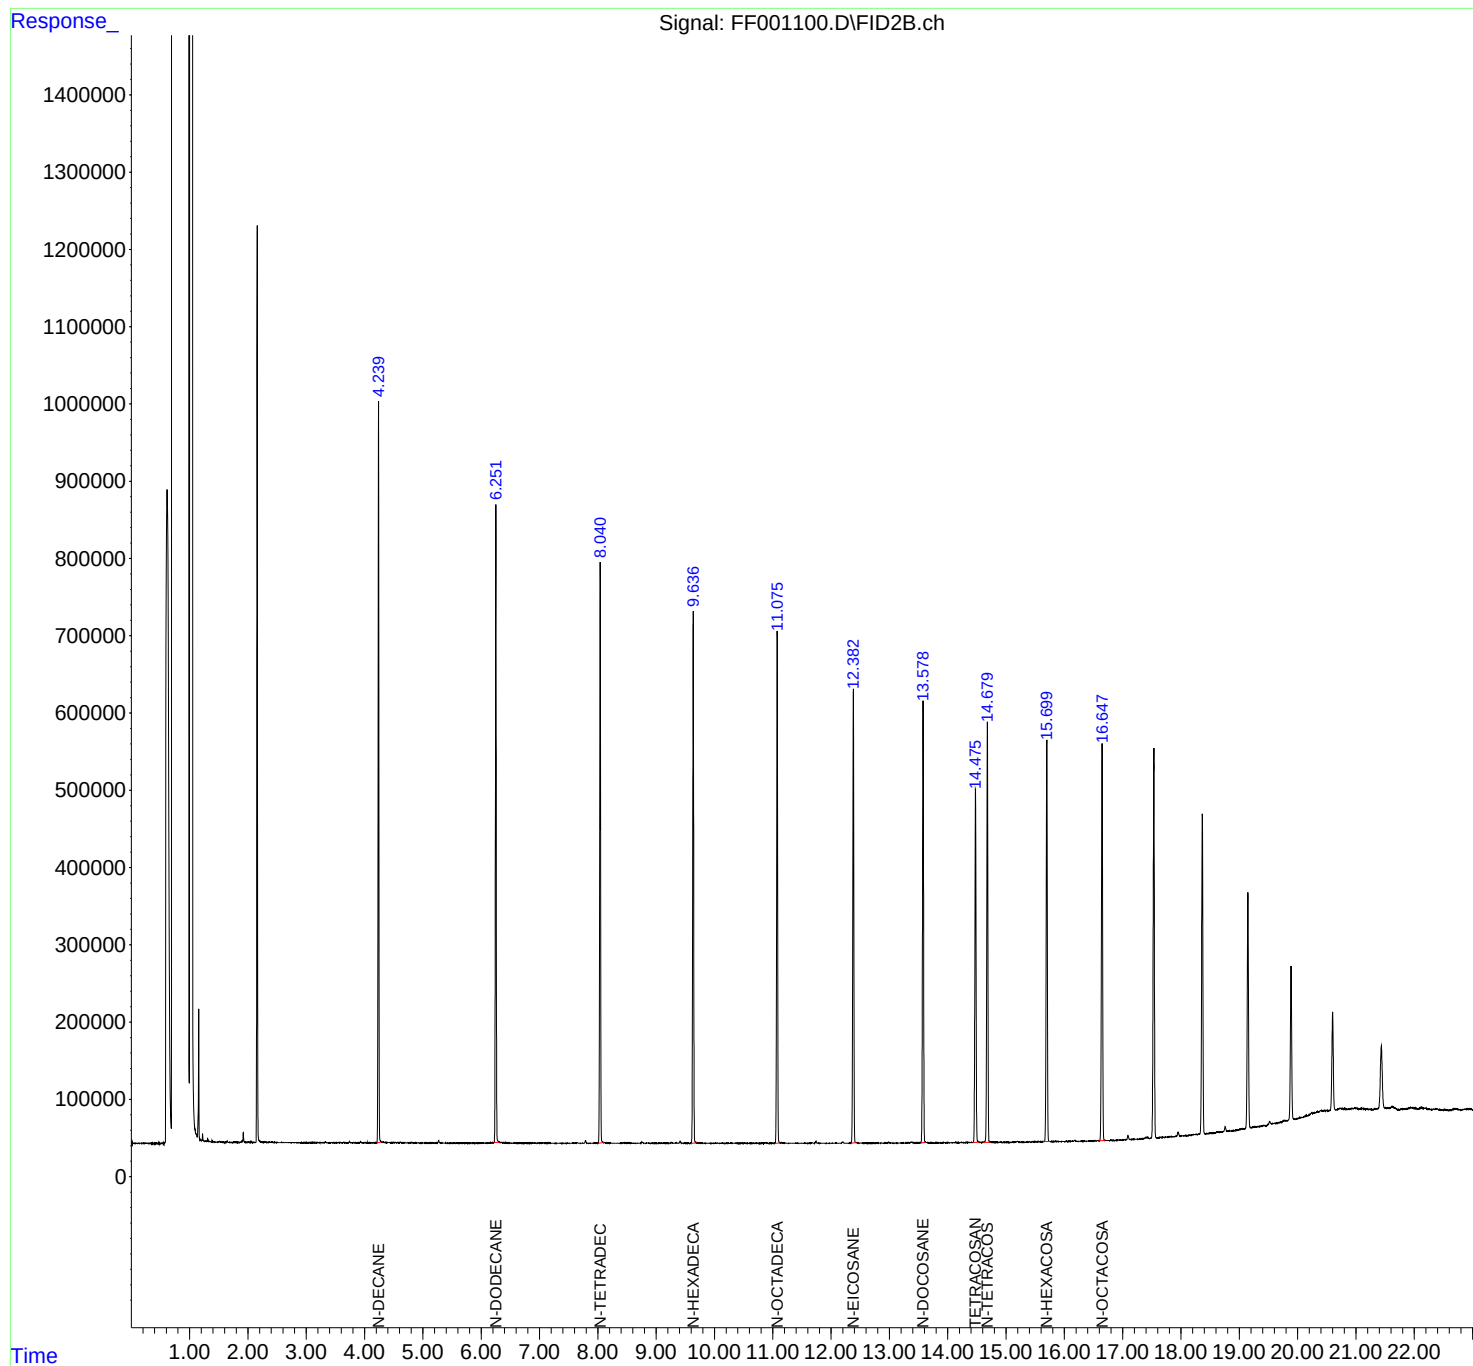

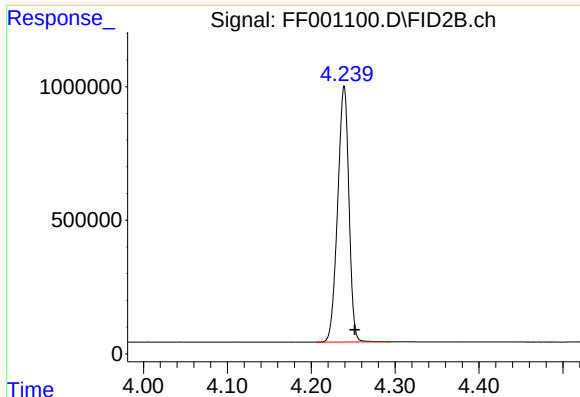


#2 N-DECANE

R.T.: 4.239 min
Delta R.T.: -0.013 min
Response: 8942953
Conc: 63.83 ug/ml

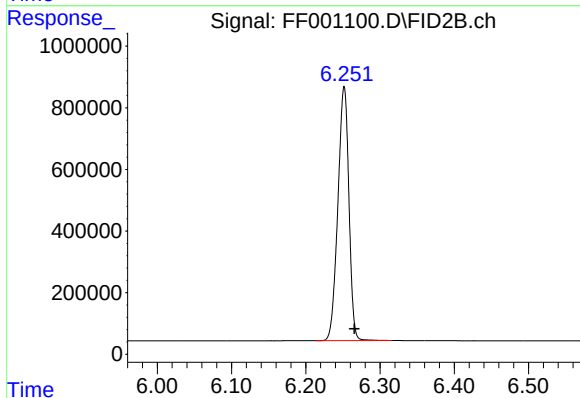


#3 N-DODECANE

R.T.: 6.252 min
Delta R.T.: -0.014 min
Response: 8514646
Conc: 60.75 ug/ml

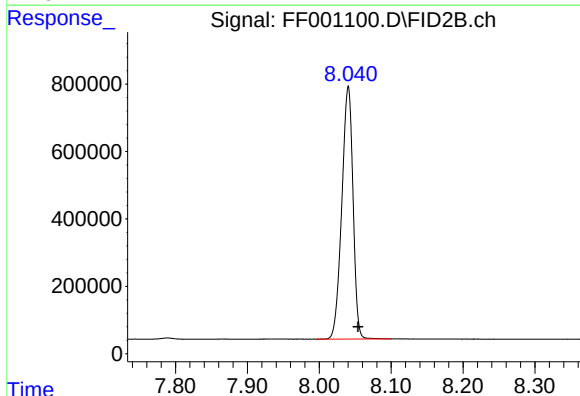


#4 N-TETRADECANE

R.T.: 8.040 min
Delta R.T.: -0.014 min
Response: 8112841
Conc: 58.27 ug/ml

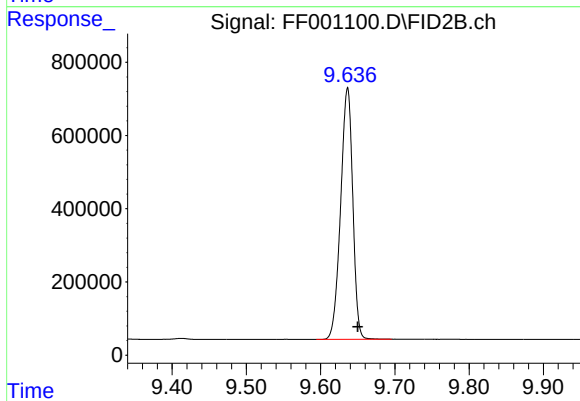


#5 N-HEXADECANE

R.T.: 9.636 min
Delta R.T.: -0.014 min
Response: 7797635
Conc: 56.55 ug/ml

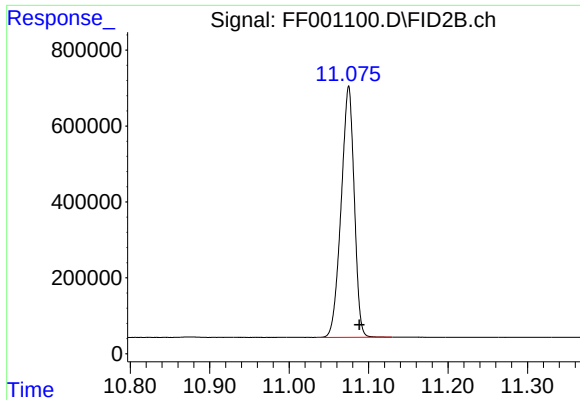


#6 N-OCTADECANE

R.T.: 11.075 min
Delta R.T.: -0.013 min
Response: 7577757
Conc: 55.49 ug/ml

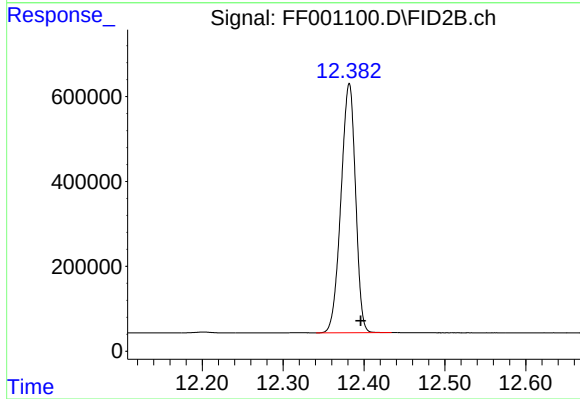


#7 N-EICOSANE

R.T.: 12.382 min
Delta R.T.: -0.014 min
Response: 7346428
Conc: 54.83 ug/ml

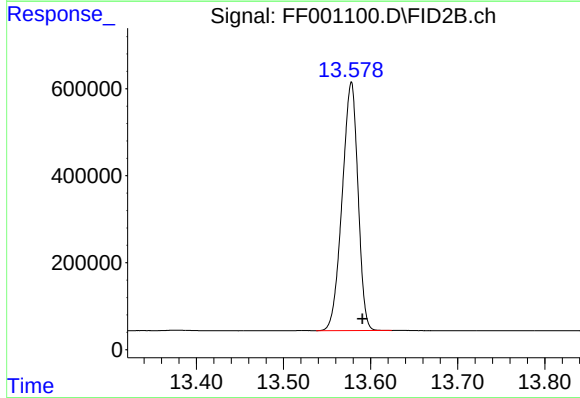


#8 N-DOCOSANE

R.T.: 13.578 min
Delta R.T.: -0.013 min
Response: 7211397
Conc: 54.54 ug/ml

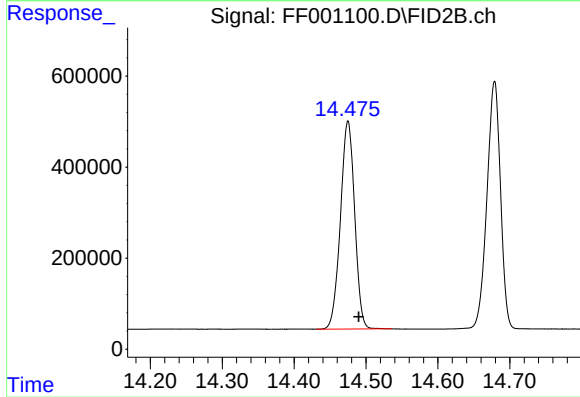


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.475 min
Delta R.T.: -0.015 min
Response: 6279397
Conc: 54.45 ug/ml

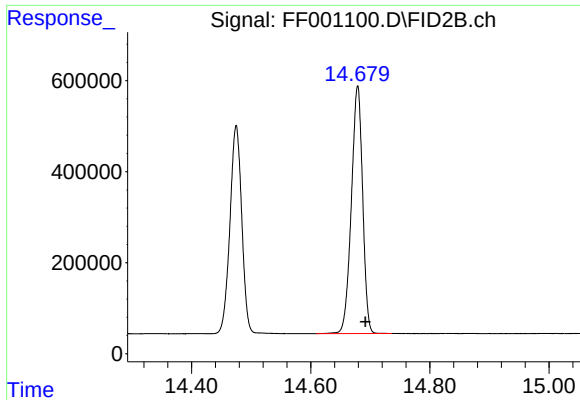


#10 N-TETRACOSANE

R.T.: 14.679 min
Delta R.T.: -0.013 min
Response: 7145563
Conc: 55.09 ug/ml

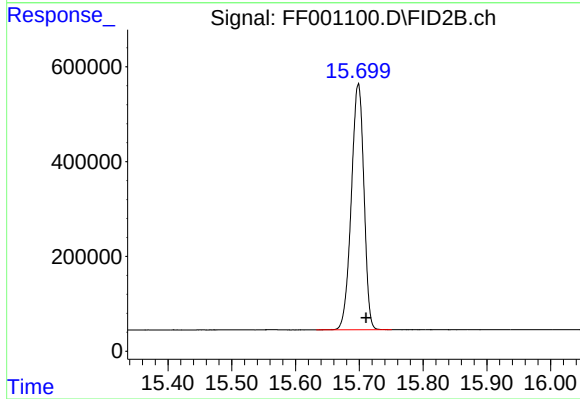

#11 N-HEXACOSANE

R.T.: 15.698 min
Delta R.T.: -0.012 min
Response: 7124421
Conc: 55.47 ug/ml

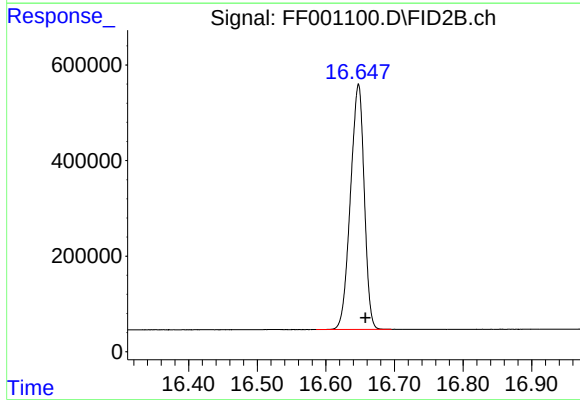

#12 N-OCTACOSANE

R.T.: 16.648 min
Delta R.T.: -0.010 min
Response: 7163348
Conc: 56.33 ug/ml