

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062619\
 Data File : FF004860.D
 Signal(s) : FID2B.ch
 Acq On : 26 Jun 2019 16:08
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Jun 27 01:39:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
 Quant Title :
 QLast Update : Wed Jun 26 14:27:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.428	4935238	38.896 ug/ml
12) N-OCTACOSANE	16.876	4506904	40.406 ug/ml
13) N-TRIACONTANE	17.767	264058	2.351 ug/ml
14) N-DOTRIACONTANE	18.621	1004568	8.820 ug/ml
15) N-TETRATRIACONTANE	19.398	181466	1.672 ug/ml
16) N-HEXATRIACONTANE	20.148	90444	0.873 ug/ml
18) N-TETRACONTANE	21.866	484307	4.166 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062619\
Data File : FF004860.D
Signal(s) : FID2B.ch
Acq On : 26 Jun 2019 16:08
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Jun 27 01:39:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

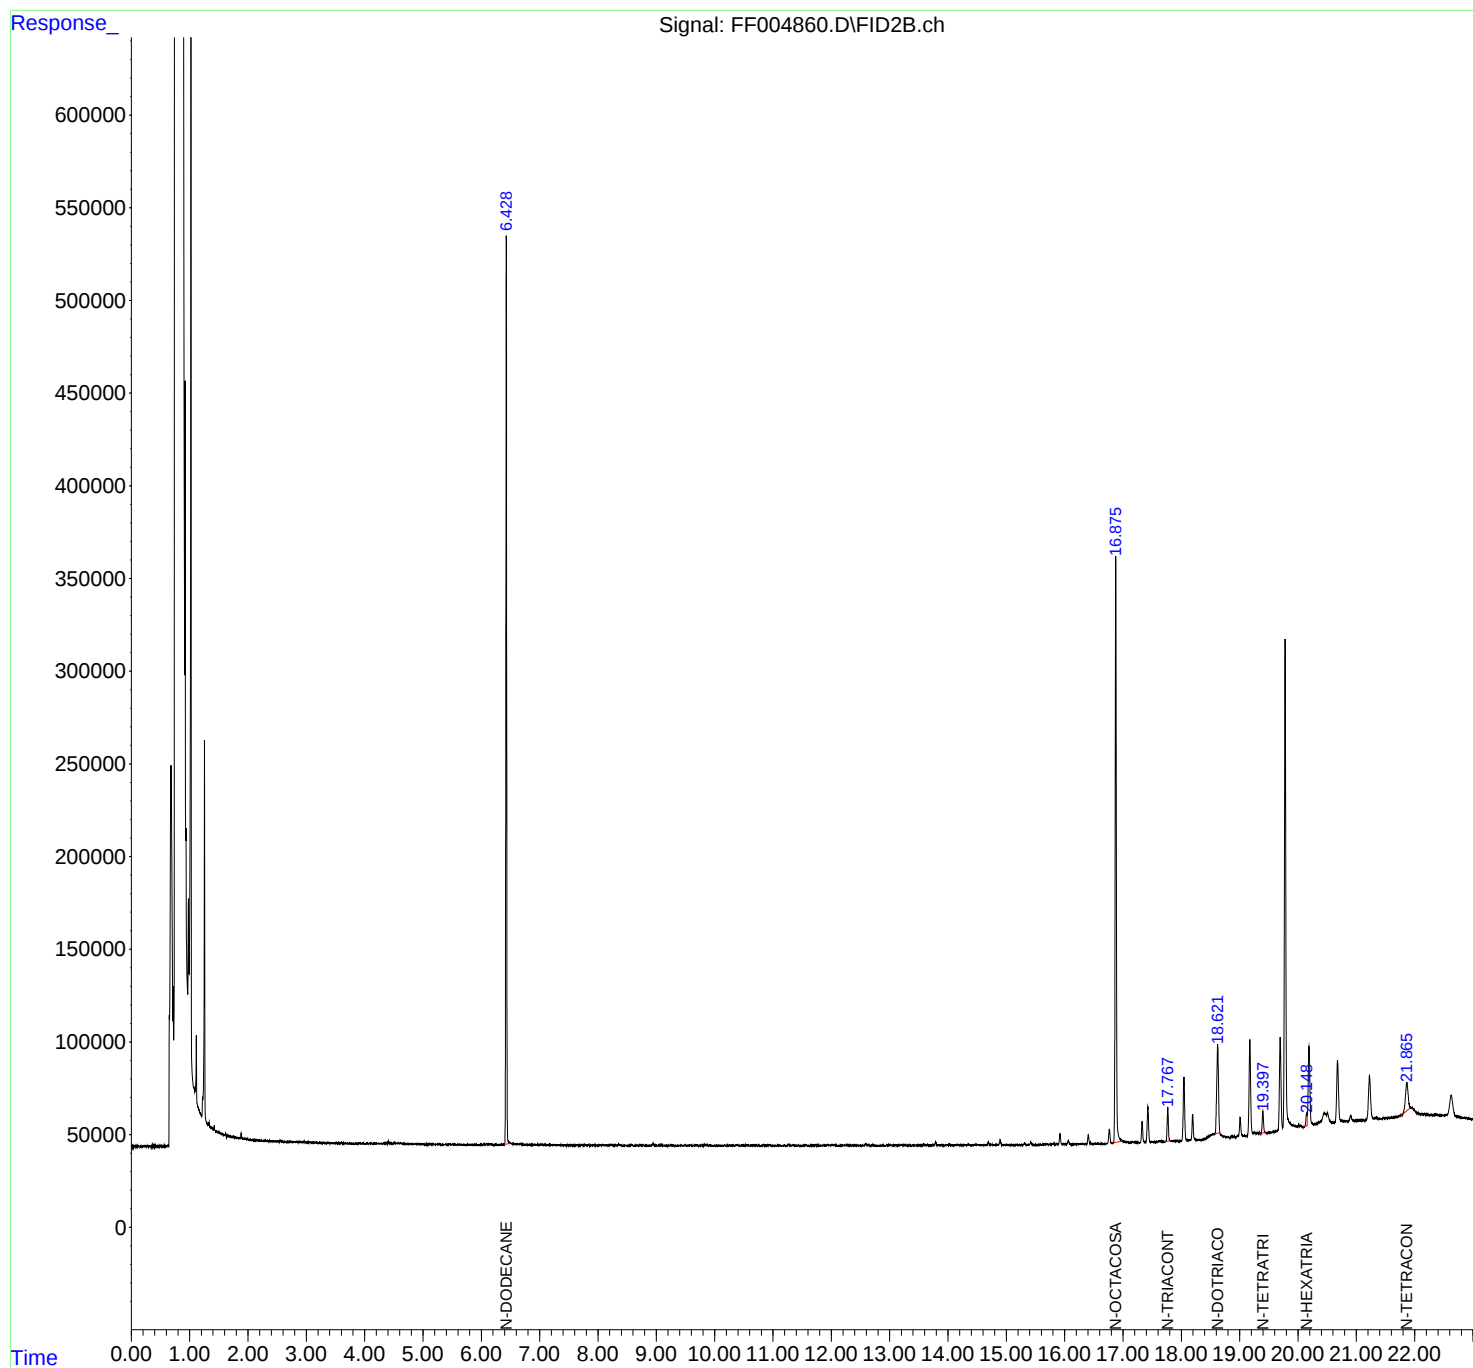


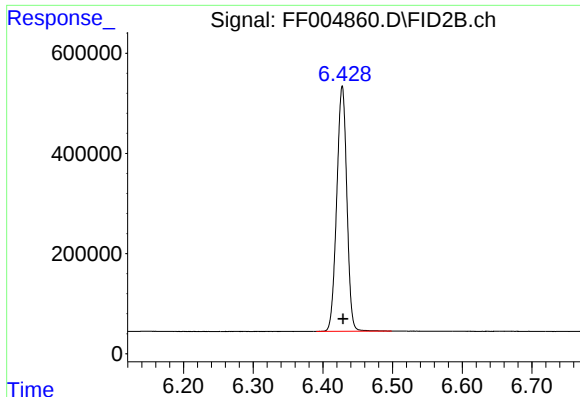

#3 N-DODECANE


R.T.: 6.428 min
Delta R.T.: 0.000 min
Response: 4935238
Conc: 38.90 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

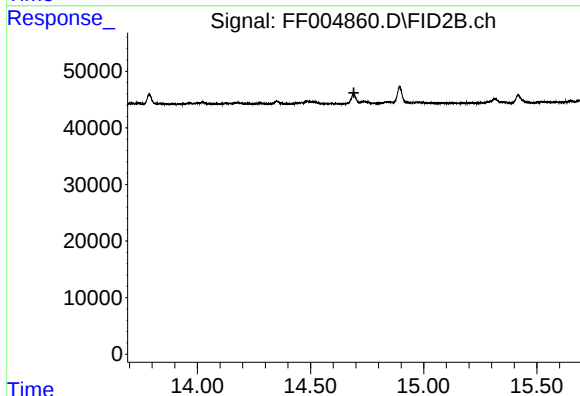


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.692 min
Response: 0
Conc: N.D.

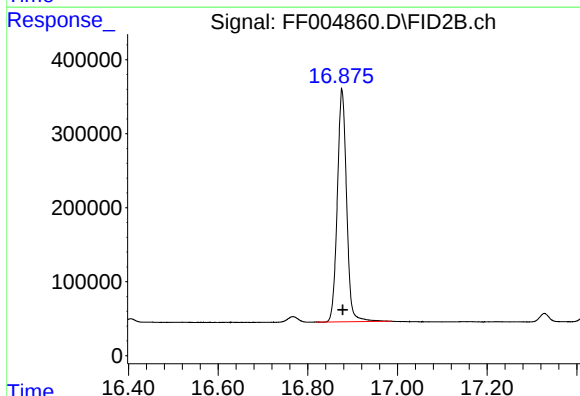


#12 N-OCTACOSANE

R.T.: 16.876 min
Delta R.T.: -0.002 min
Response: 4506904
Conc: 40.41 ug/ml

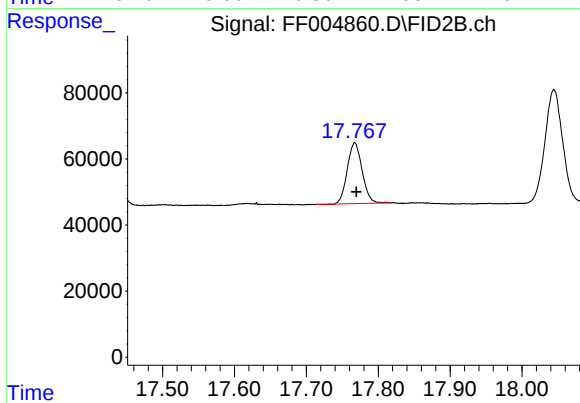

#13 N-TRIACONTANE


R.T.: 17.767 min
Delta R.T.: -0.002 min
Response: 264058
Conc: 2.35 ug/ml

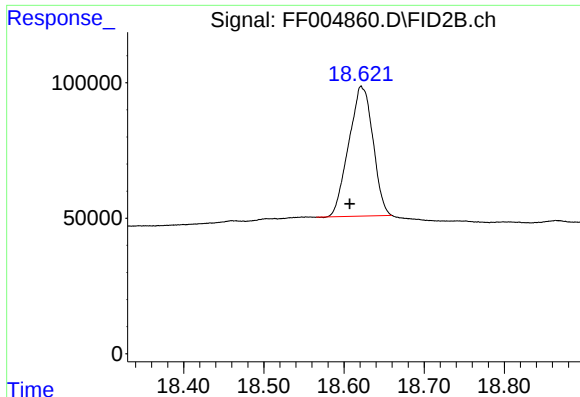

#14 N-DOTRIACONTANE


R.T.: 18.621 min
Delta R.T.: 0.014 min
Response: 1004568
Conc: 8.82 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

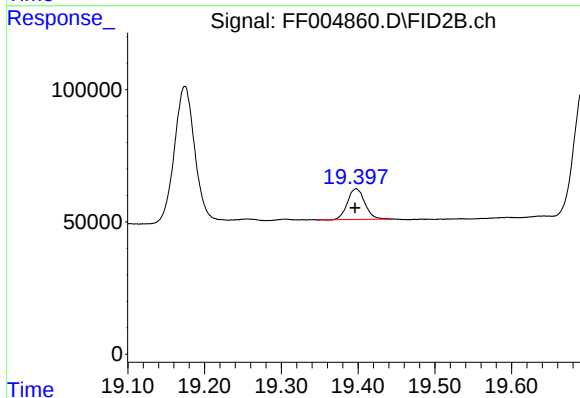


#15 N-TETRATRIACONTANE

R.T.: 19.398 min
Delta R.T.: 0.001 min
Response: 181466
Conc: 1.67 ug/ml

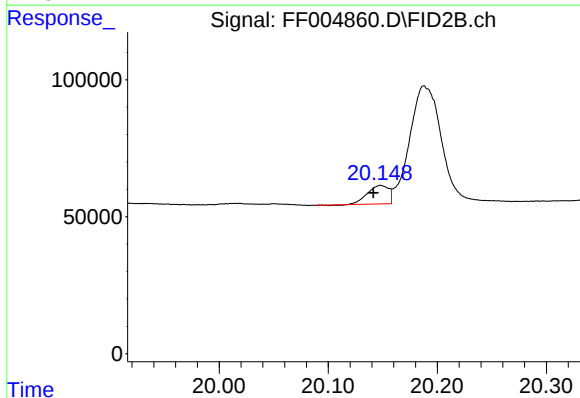

#16 N-HEXATRIACONTANE

R.T.: 20.148 min
Delta R.T.: 0.007 min
Response: 90444
Conc: 0.87 ug/ml

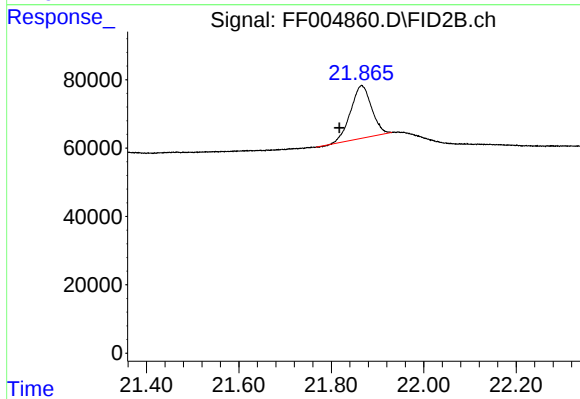

#18 N-TETRACONTANE

R.T.: 21.866 min
Delta R.T.: 0.048 min
Response: 484307
Conc: 4.17 ug/ml