

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF062619\  
 Data File : FF004861.D  
 Signal(s) : FID2B.ch  
 Acq On : 26 Jun 2019 16:38  
 Operator : DD\AJ  
 Sample : PB120728BL  
 Misc :  
 ALS Vial : 55 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Jun 27 01:40:00 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF062619.M  
 Quant Title :  
 QLast Update : Wed Jun 26 14:27:24 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.691 | 2039318  | 20.968 ug/ml |
| Target Compounds              |        |          |              |
| 14) N-DOTRIACONTANE           | 18.622 | 220039   | 1.932 ug/ml  |
| 16) N-HEXATRIACONTANE         | 20.190 | 669994   | 6.470 ug/ml  |
| 18) N-TETRACONTANE            | 21.865 | 560220   | 4.819 ug/ml  |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF062619\  
Data File : FF004861.D  
Signal(s) : FID2B.ch  
Acq On : 26 Jun 2019 16:38  
Operator : DD\AJ  
Sample : PB120728BL  
Misc :  
ALS Vial : 55 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jun 27 01:40:00 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF062619.M  
Quant Title :  
QLast Update : Wed Jun 26 14:27:24 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

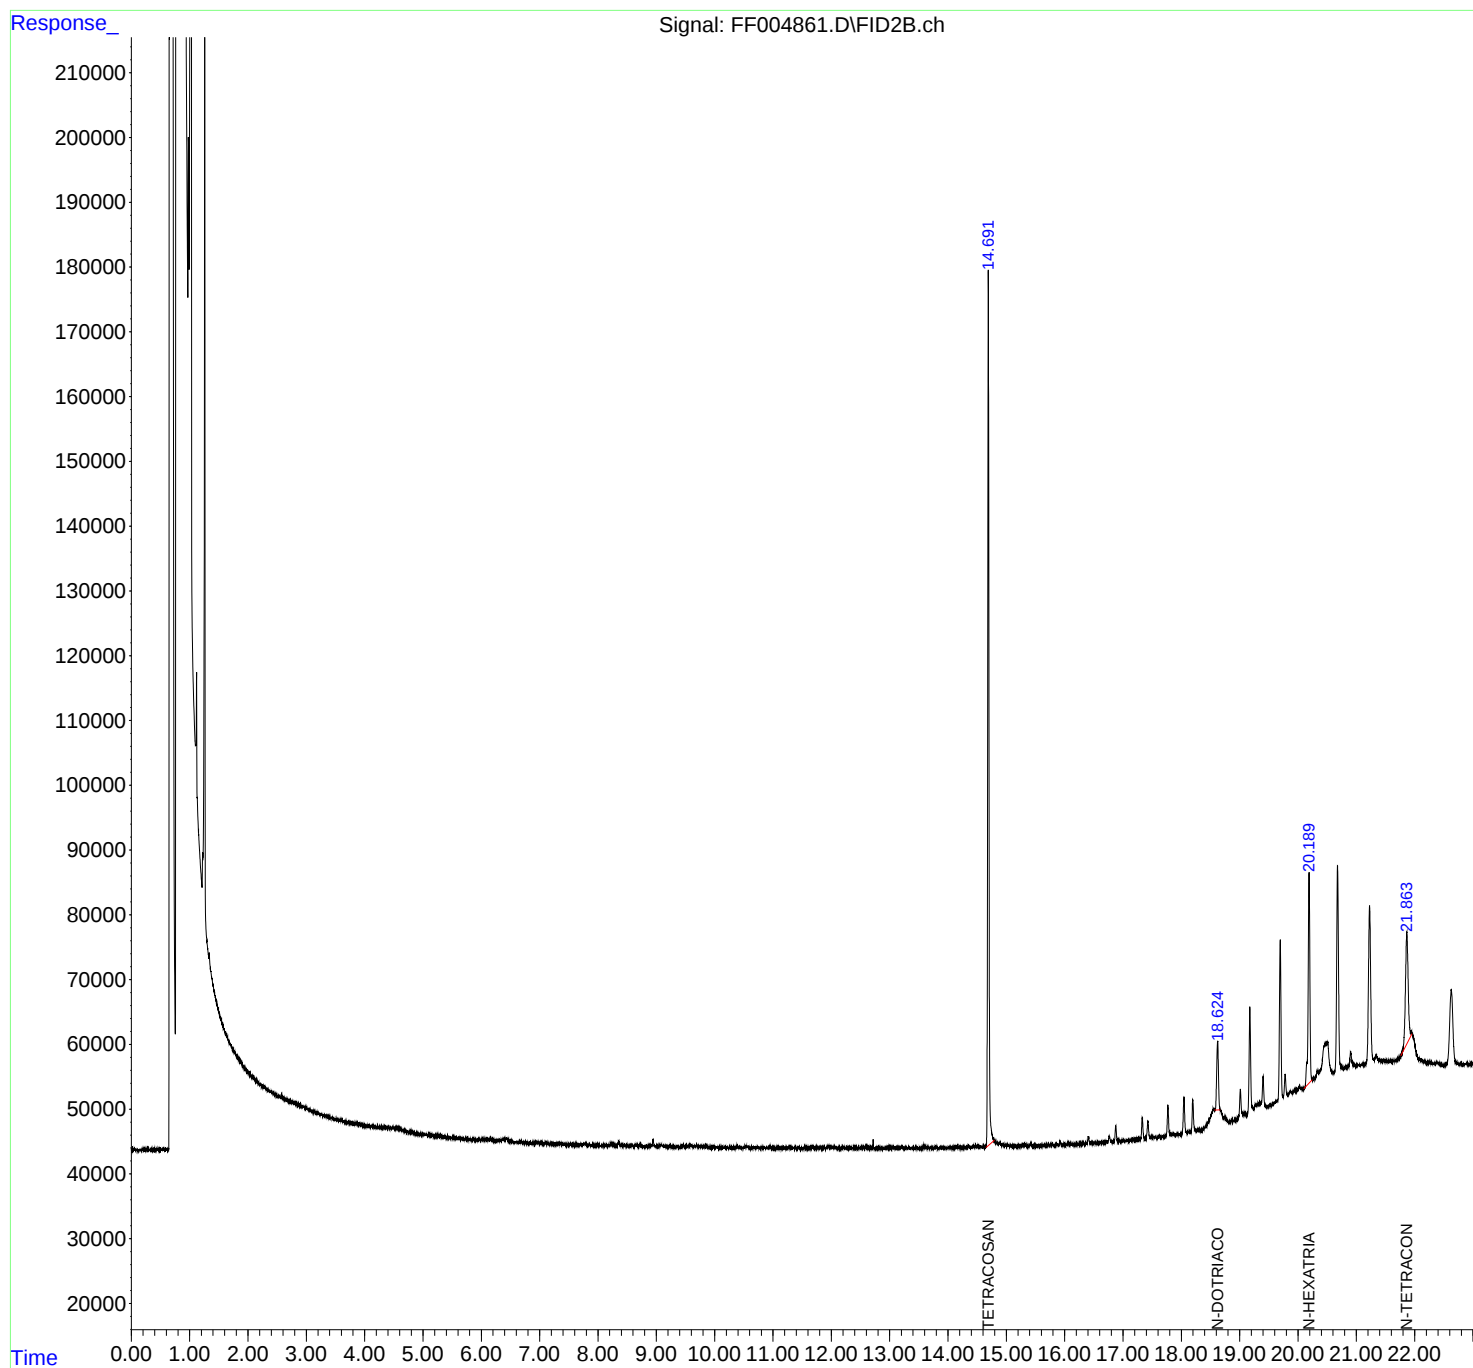


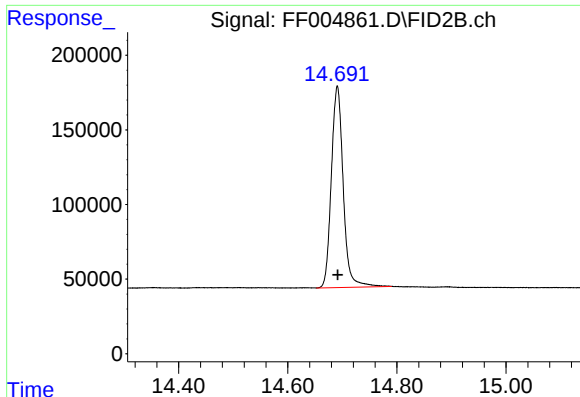

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.691 min  
Delta R.T.: 0.000 min  
Response: 2039318  
Conc: 20.97 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

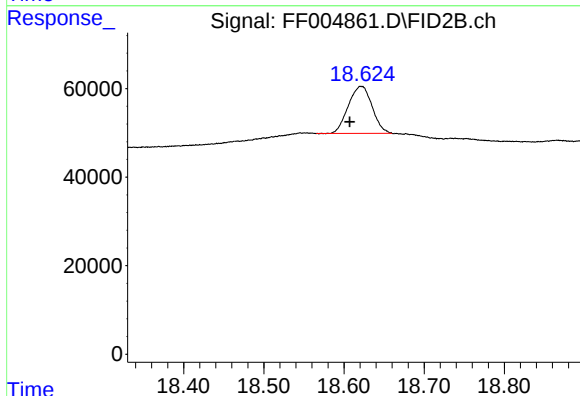


#14 N-DOTRIACONTANE

R.T.: 18.622 min  
Delta R.T.: 0.014 min  
Response: 220039  
Conc: 1.93 ug/ml

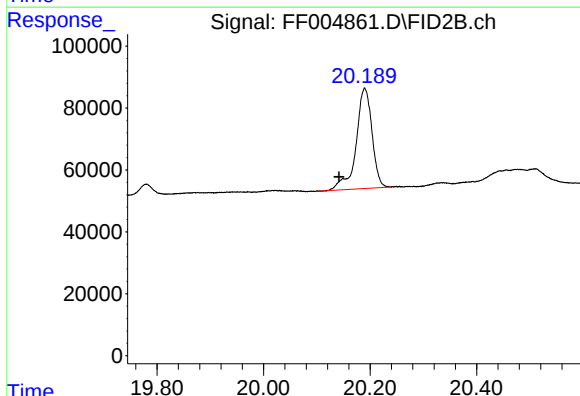

#16 N-HEXATRIACONTANE

R.T.: 20.190 min  
Delta R.T.: 0.048 min  
Response: 669994  
Conc: 6.47 ug/ml

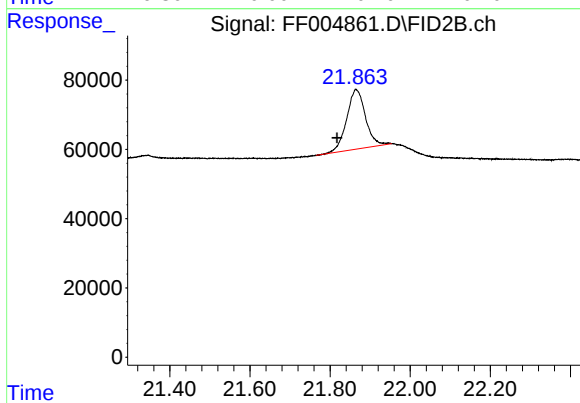

#18 N-TETRACONTANE

R.T.: 21.865 min  
Delta R.T.: 0.048 min  
Response: 560220  
Conc: 4.82 ug/ml