

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062619\
Data File : FF004866.D
Signal(s) : FID2B.ch
Acq On : 26 Jun 2019 23:01
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 27 01:40:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.616	120798	1.061 ug/ml
16)	N-HEXATRIACONTANE	20.180	215126	2.077 ug/ml
18)	N-TETRACONTANE	21.849	470953	4.051 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062619\
Data File : FF004866.D
Signal(s) : FID2B.ch
Acq On : 26 Jun 2019 23:01
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Jun 27 01:40:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

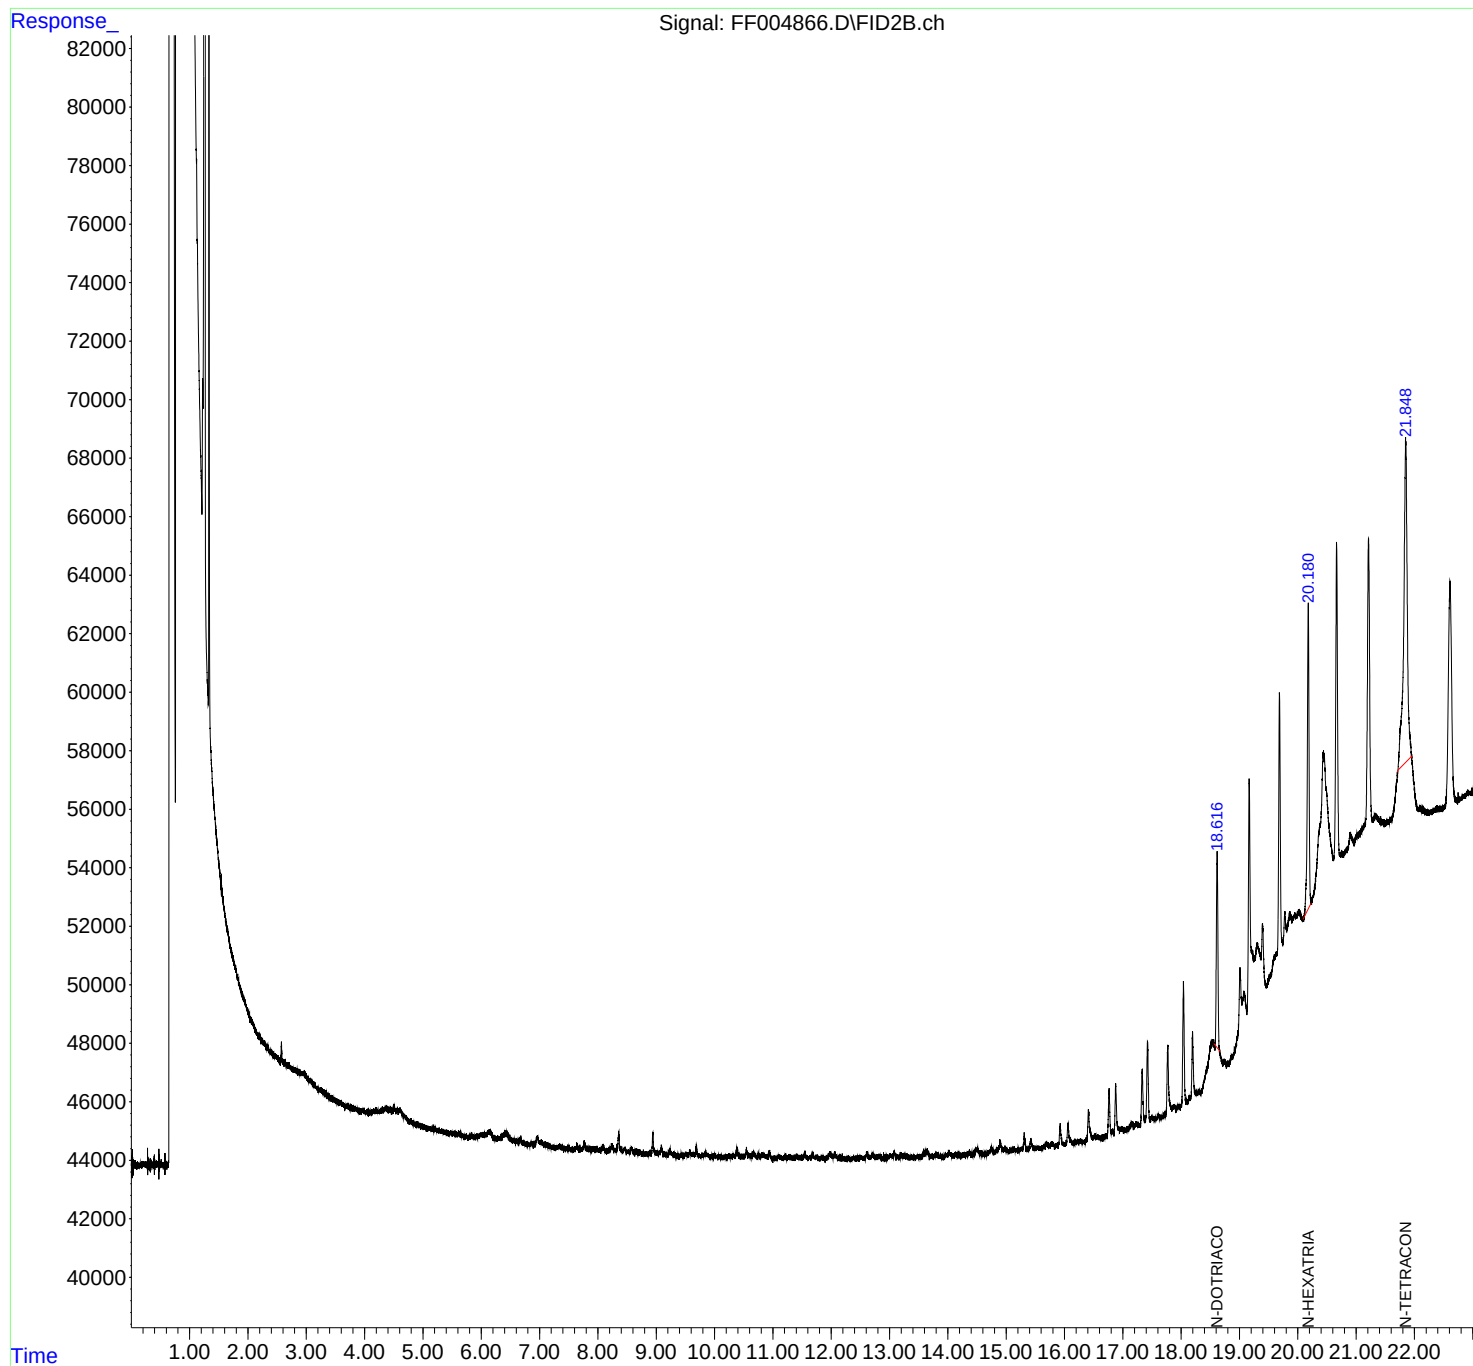


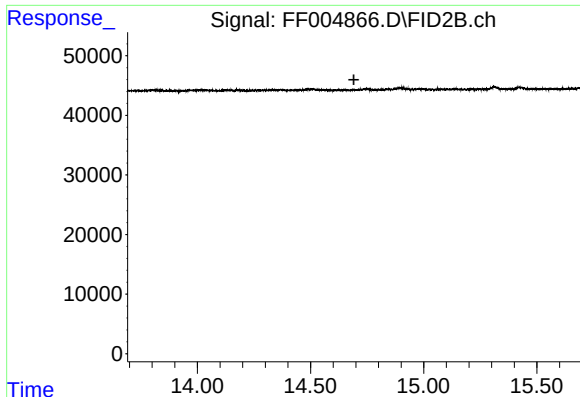

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.692 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

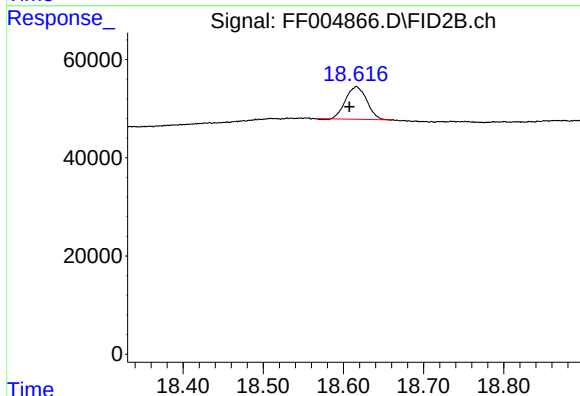


#14 N-DOTRIACONTANE

R.T.: 18.616 min
Delta R.T.: 0.009 min
Response: 120798
Conc: 1.06 ug/ml

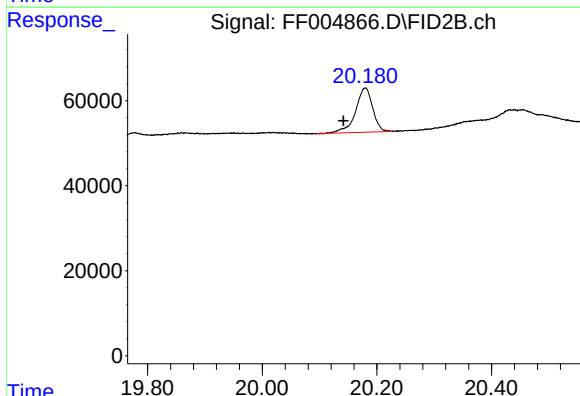

#16 N-HEXATRIACONTANE

R.T.: 20.180 min
Delta R.T.: 0.038 min
Response: 215126
Conc: 2.08 ug/ml

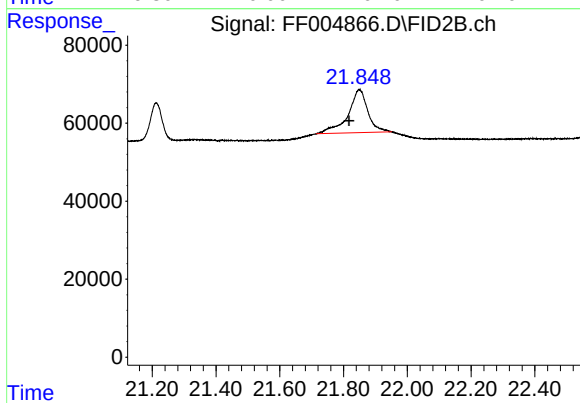

#18 N-TETRACONTANE

R.T.: 21.849 min
Delta R.T.: 0.032 min
Response: 470953
Conc: 4.05 ug/ml