

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF062619\  
Data File : FF004860.D  
Signal(s) : FID2B.ch  
Acq On : 26 Jun 2019 16:08  
Operator : DD\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 54 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
RT MARKER

Integration File: autoint1.e  
Quant Time: Jun 27 01:39:51 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF062619.M  
Quant Title :  
QLast Update : Wed Jun 26 14:27:24 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    |              | R.T.   | Response | Conc Units   |
|-----------------------------|--------------|--------|----------|--------------|
| -----                       |              |        |          |              |
| System Monitoring Compounds |              |        |          |              |
| Target Compounds            |              |        |          |              |
| 3)                          | N-DODECANE   | 6.428  | 4935238  | 38.896 ug/ml |
| 12)                         | N-OCTACOSANE | 16.876 | 4506904  | 40.406 ug/ml |
| -----                       |              |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF062619\  
Data File : FF004860.D  
Signal(s) : FID2B.ch  
Acq On : 26 Jun 2019 16:08  
Operator : DD\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 54 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
RT MARKER

Integration File: autoint1.e  
Quant Time: Jun 27 01:39:51 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF062619.M  
Quant Title :  
QLast Update : Wed Jun 26 14:27:24 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

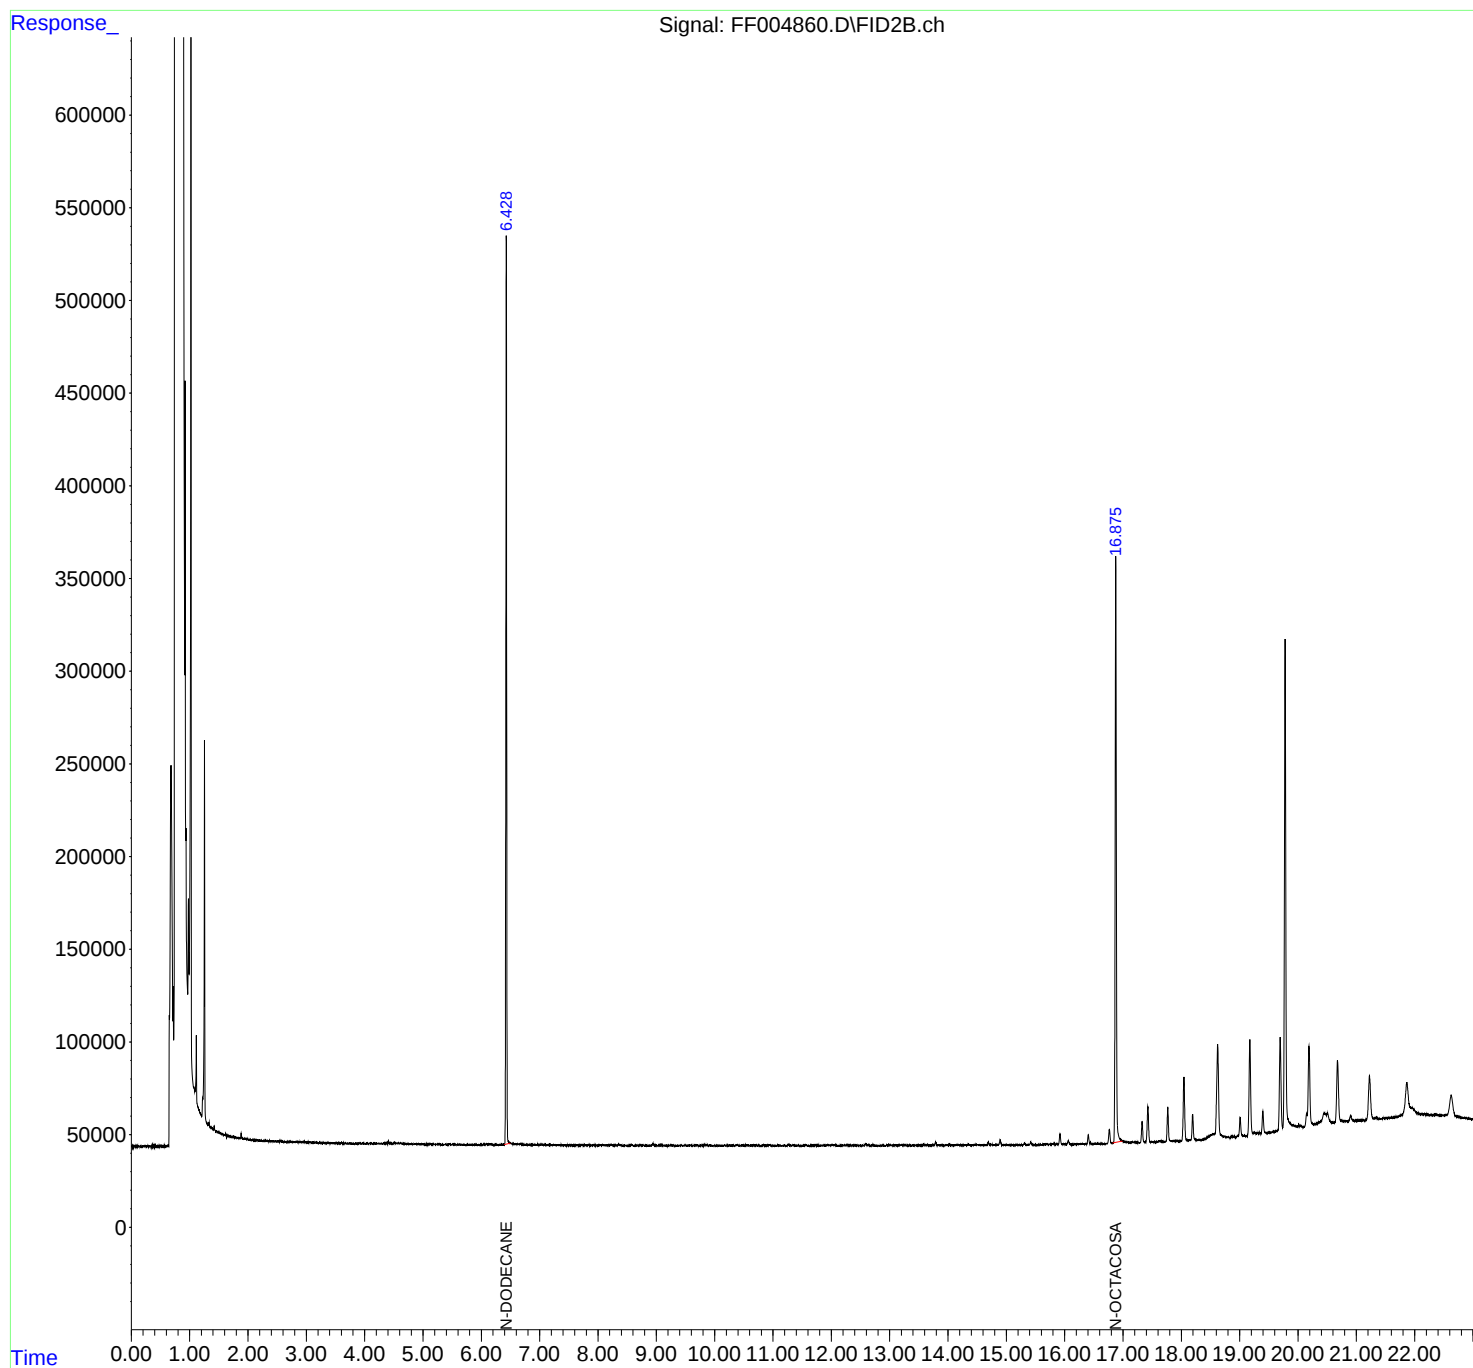


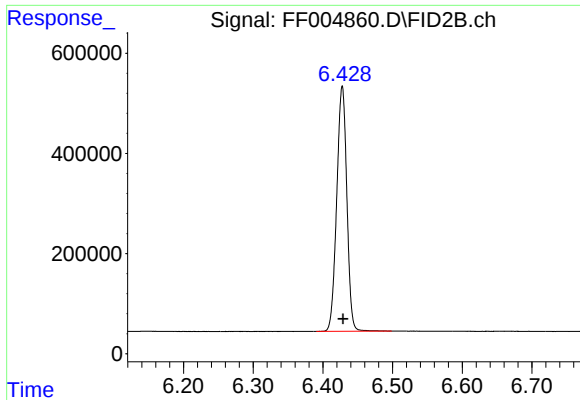

#3 N-DODECANE


R.T.: 6.428 min  
Delta R.T.: 0.000 min  
Response: 4935238  
Conc: 38.90 ug/ml

Instrument :  
FID\_F  
ClientSampleId :  
RT MARKER

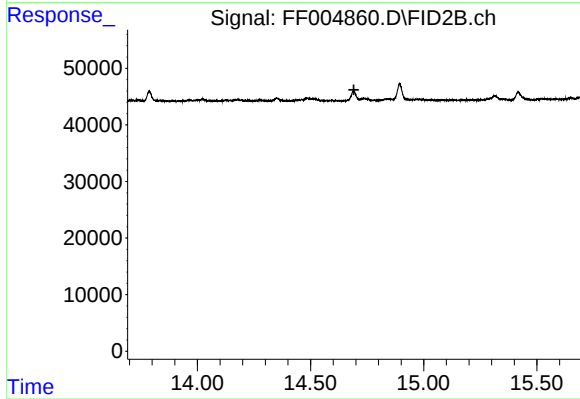

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T. : 14.692 min  
Response: 0  
Conc: N.D.

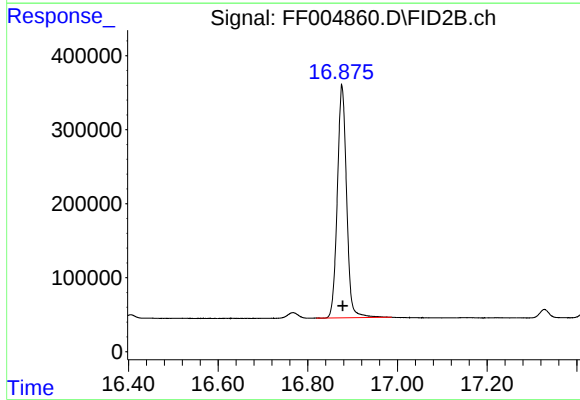

#12 N-OCTACOSANE

R.T.: 16.876 min  
Delta R.T.: -0.002 min  
Response: 4506904  
Conc: 40.41 ug/ml