

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062619\
Data File : FF004861.D
Signal(s) : FID2B.ch
Acq On : 26 Jun 2019 16:38
Operator : DD\AJ
Sample : PB120728BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB120728BL

Integration File: autoint1.e
Quant Time: Jun 27 01:40:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.691	2039318	20.968 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062619\
Data File : FF004861.D
Signal(s) : FID2B.ch
Acq On : 26 Jun 2019 16:38
Operator : DD\AJ
Sample : PB120728BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB120728BL

Integration File: autoint1.e
Quant Time: Jun 27 01:40:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

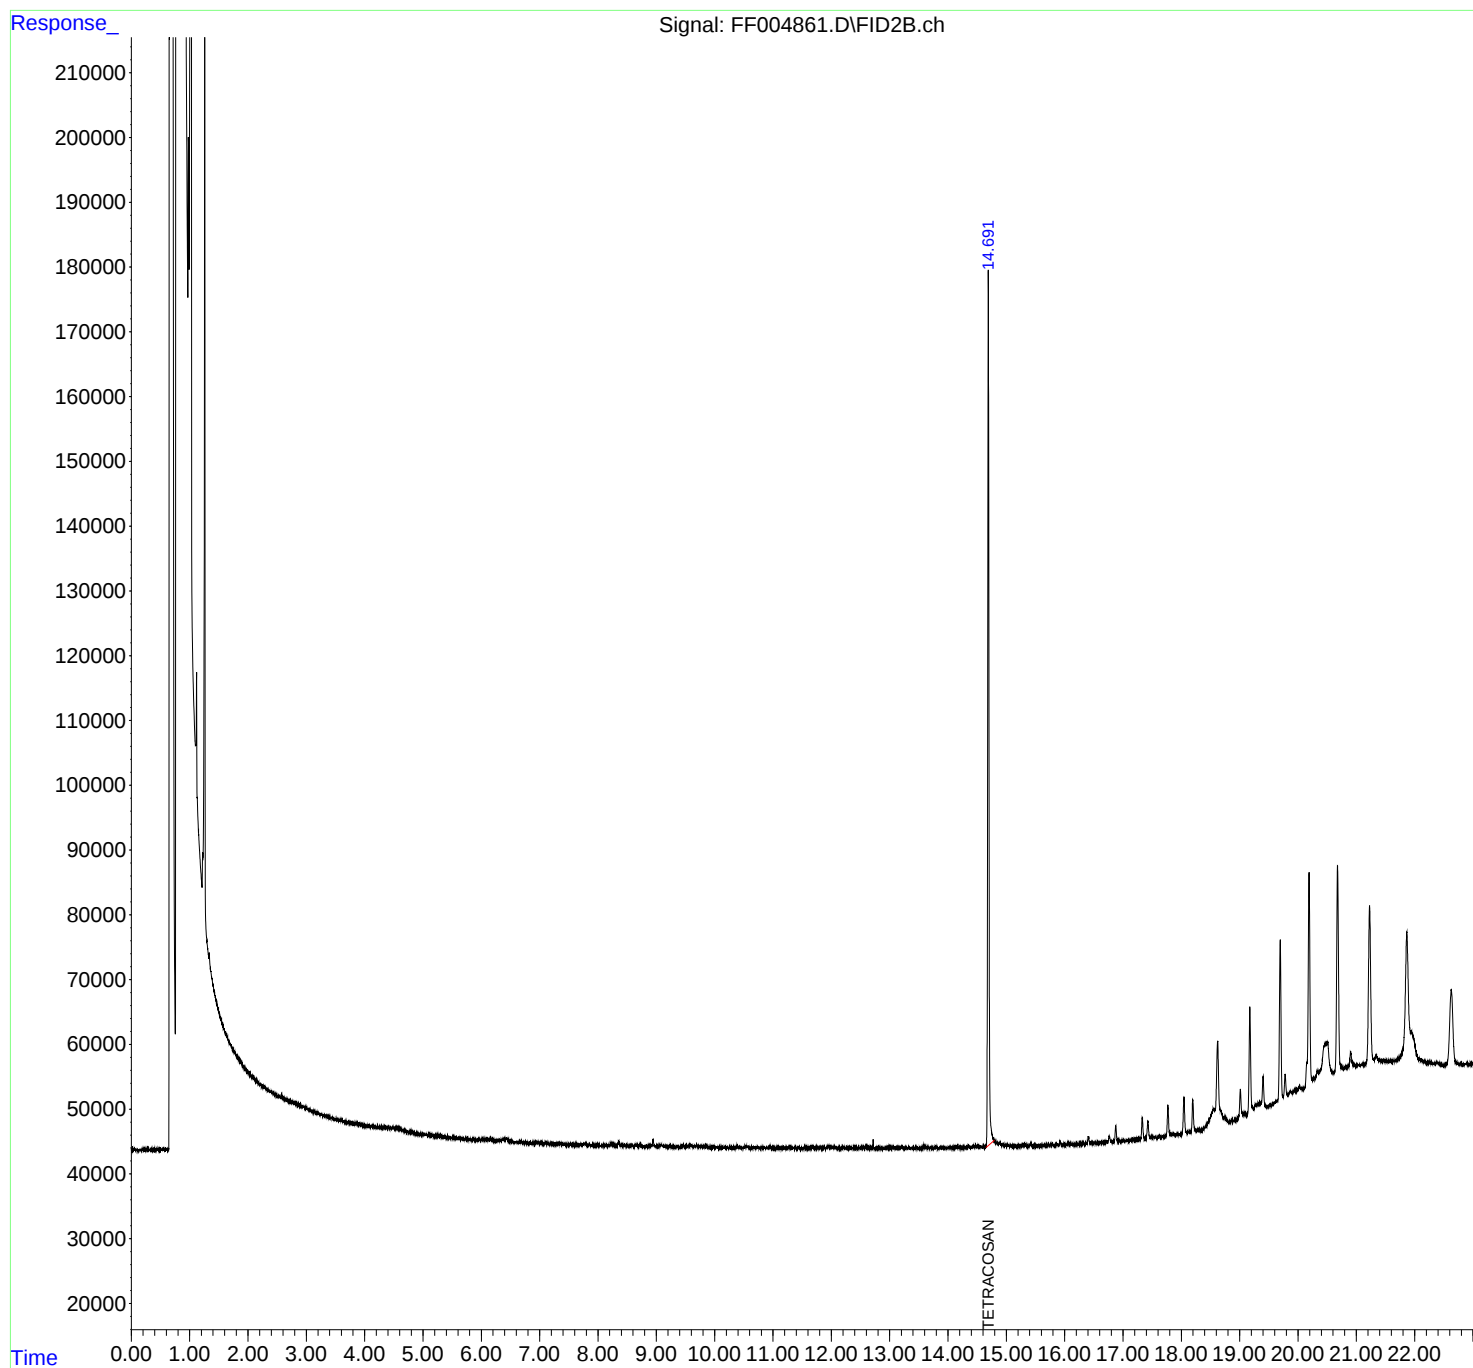

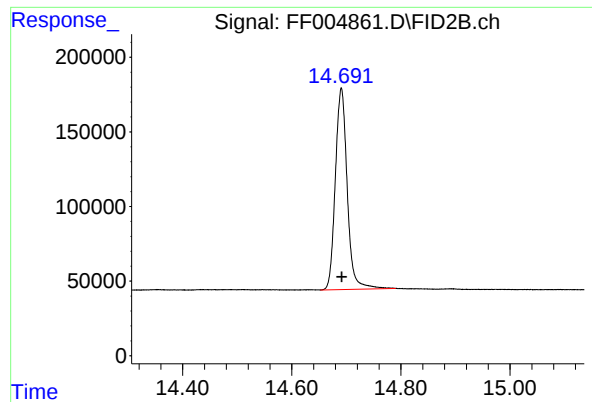

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.691 min
Delta R.T.: 0.000 min
Response: 2039318
Conc: 20.97 ug/ml

Instrument :
FID_F
ClientSampleId :
PB120728BL