

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062623AL\
 Data File : FF013003.D
 Signal(s) : FID2B.ch
 Acq On : 26 Jun 2023 12:09
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 27 02:29:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 062023.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 20 13:45:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) T n-Tetracosane (C24)	14.138	41576	0.339 ug/ml
18) T n-Dotriacontane (C32)	17.844	23235	0.199 ug/ml
19) T n-Tetratriacontane (C34)	18.624	12149	0.109 ug/ml
22) T n-Tetracontane (C40)	20.954	1447818	14.944 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062623AL\
Data File : FF013003.D
Signal(s) : FID2B.ch
Acq On : 26 Jun 2023 12:09
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 27 02:29:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 062023.M
Quant Title : GC Extractables
QLast Update : Tue Jun 20 13:45:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

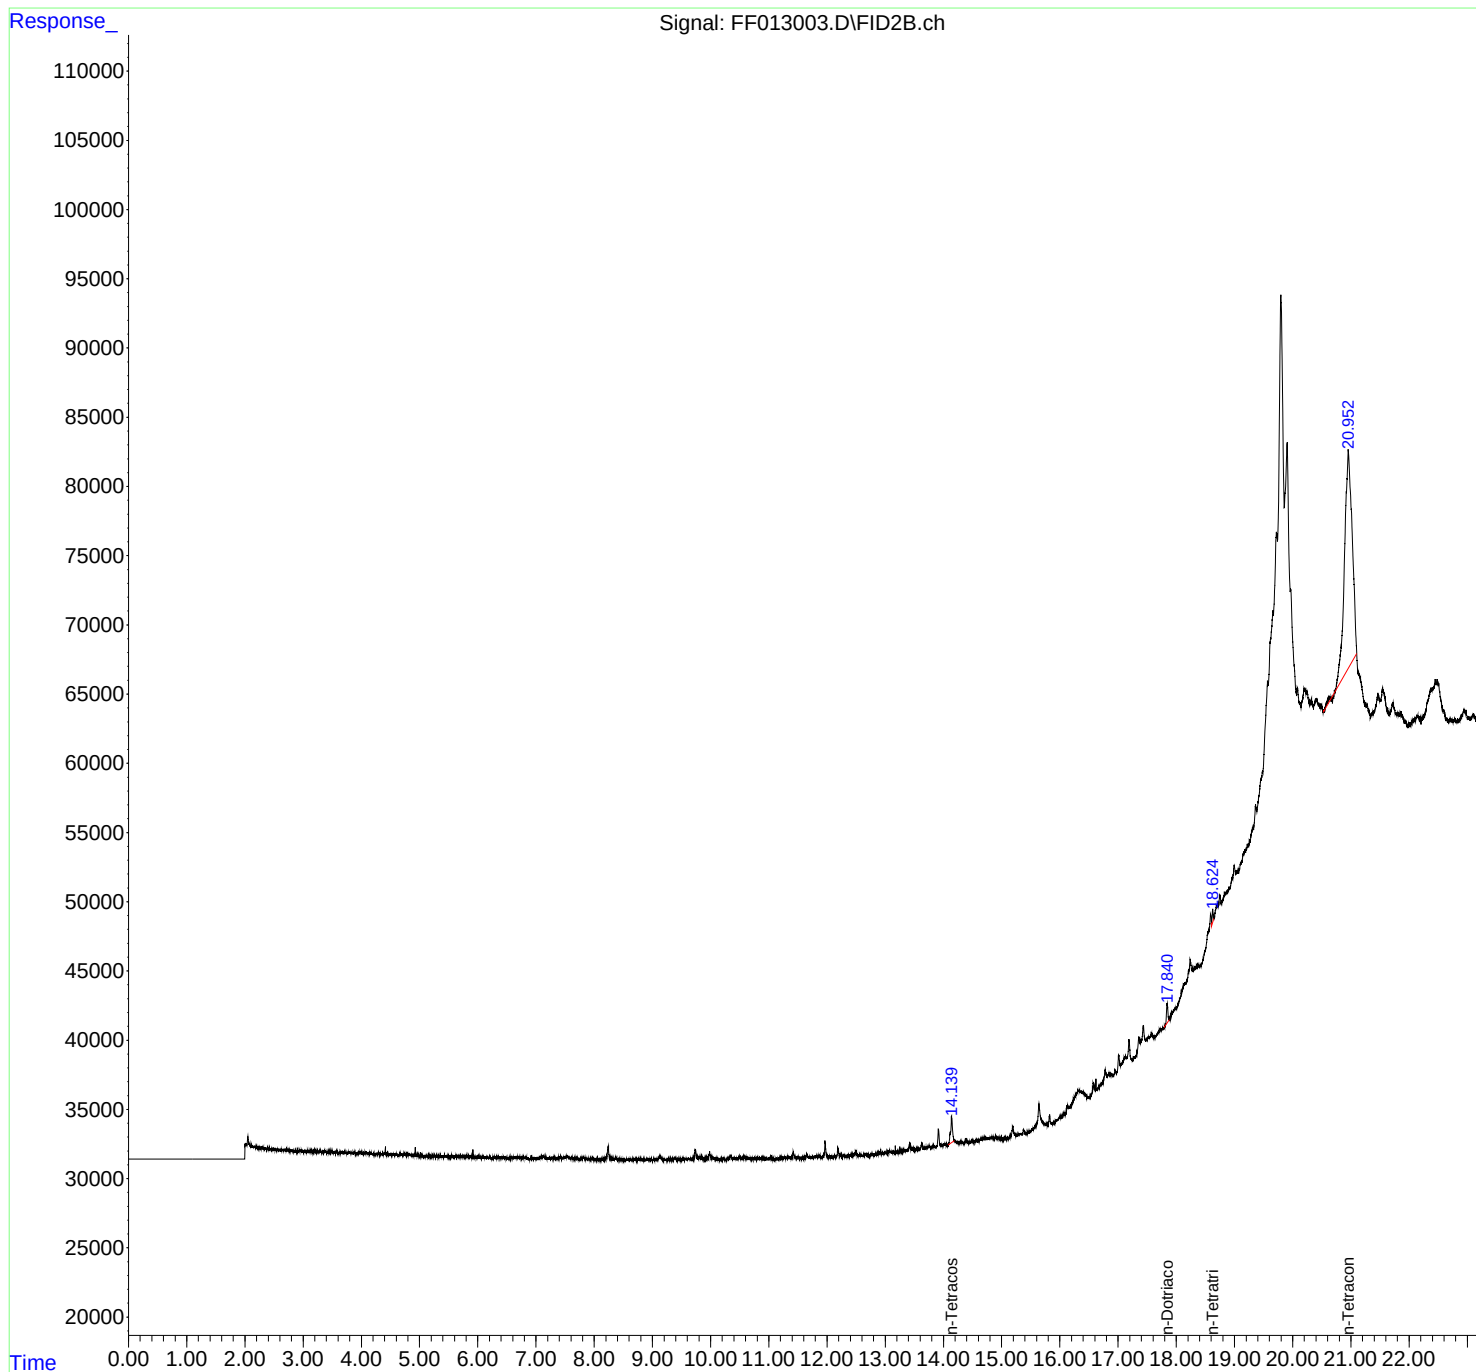


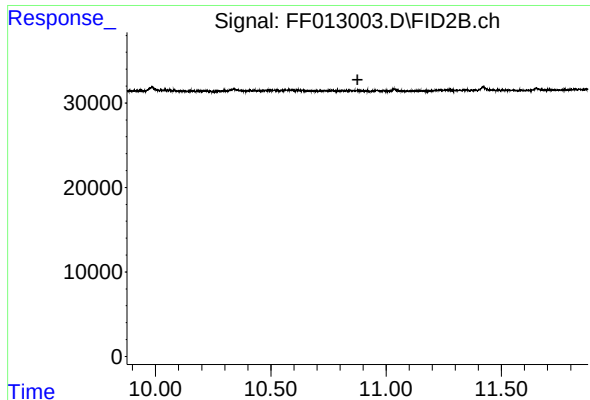

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 10.876 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

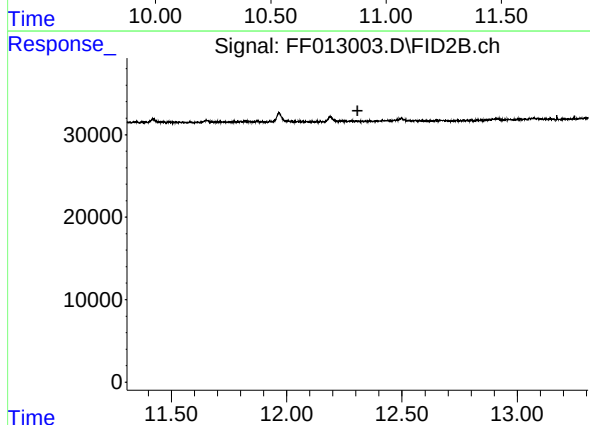


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 12.307 min
Response: 0
Conc: N.D.

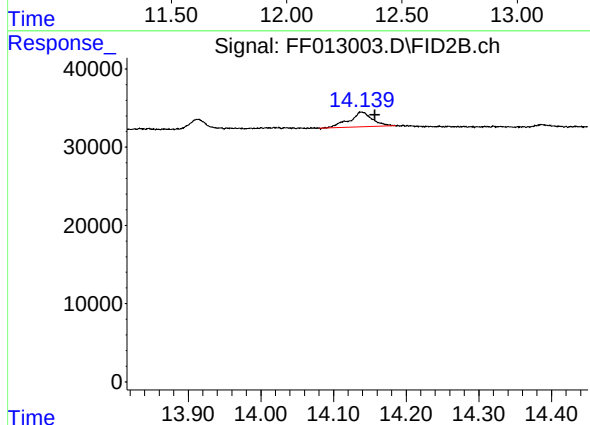


#14 n-Tetracosane (C24)

R.T.: 14.138 min
Delta R.T.: -0.019 min
Response: 41576
Conc: 0.34 ug/ml

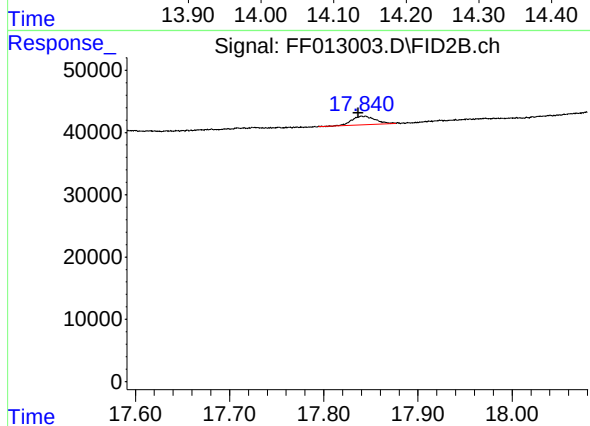

#18 n-Dotriacontane (C32)


R.T.: 17.844 min
Delta R.T.: 0.007 min
Response: 23235
Conc: 0.20 ug/ml

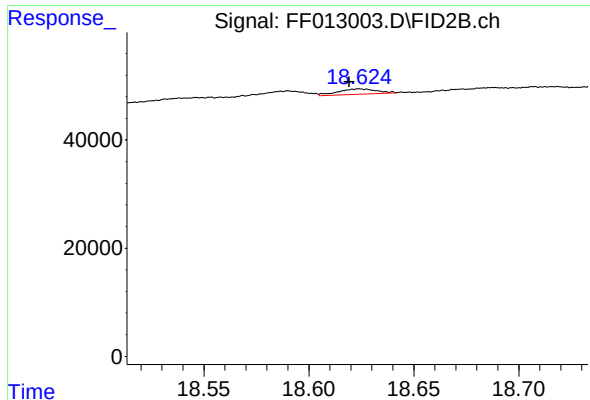

#19 n-Tetratriacontane (C34)

R.T.: 18.624 min
Delta R.T.: 0.005 min
Response: 12149
Conc: 0.11 ug/ml

Instrument :
FID_F
ClientSampleId :

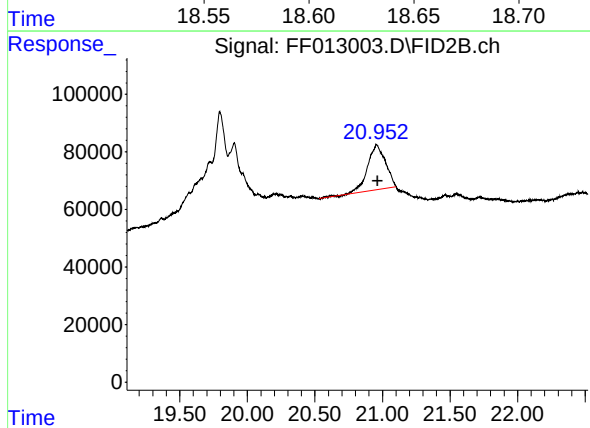

#22 n-Tetracontane (C40)

R.T.: 20.954 min
Delta R.T.: -0.010 min
Response: 1447818
Conc: 14.94 ug/ml