

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062623AL\
 Data File : FF013022.D
 Signal(s) : FID2B.ch
 Acq On : 27 Jun 2023 04:56
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 27 07:52:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 062023.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 20 13:45:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) T n-Tetracosane (C24)	14.111	26144	0.213 ug/ml
15) T n-Hexacosane (C26)	15.189	54501	0.453 ug/ml
17) T n-Tricontane (C30)	16.944f	36372	0.305 ug/ml
19) T n-Tetratriacontane (C34)	18.621	193516	1.743 ug/ml
21) T n-Octatriacontane (C38)	20.085	17783	0.170 ug/ml
22) T n-Tetracontane (C40)	20.932	693655	7.160 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062623AL\
Data File : FF013022.D
Signal(s) : FID2B.ch
Acq On : 27 Jun 2023 04:56
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 27 07:52:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 062023.M
Quant Title : GC Extractables
QLast Update : Tue Jun 20 13:45:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

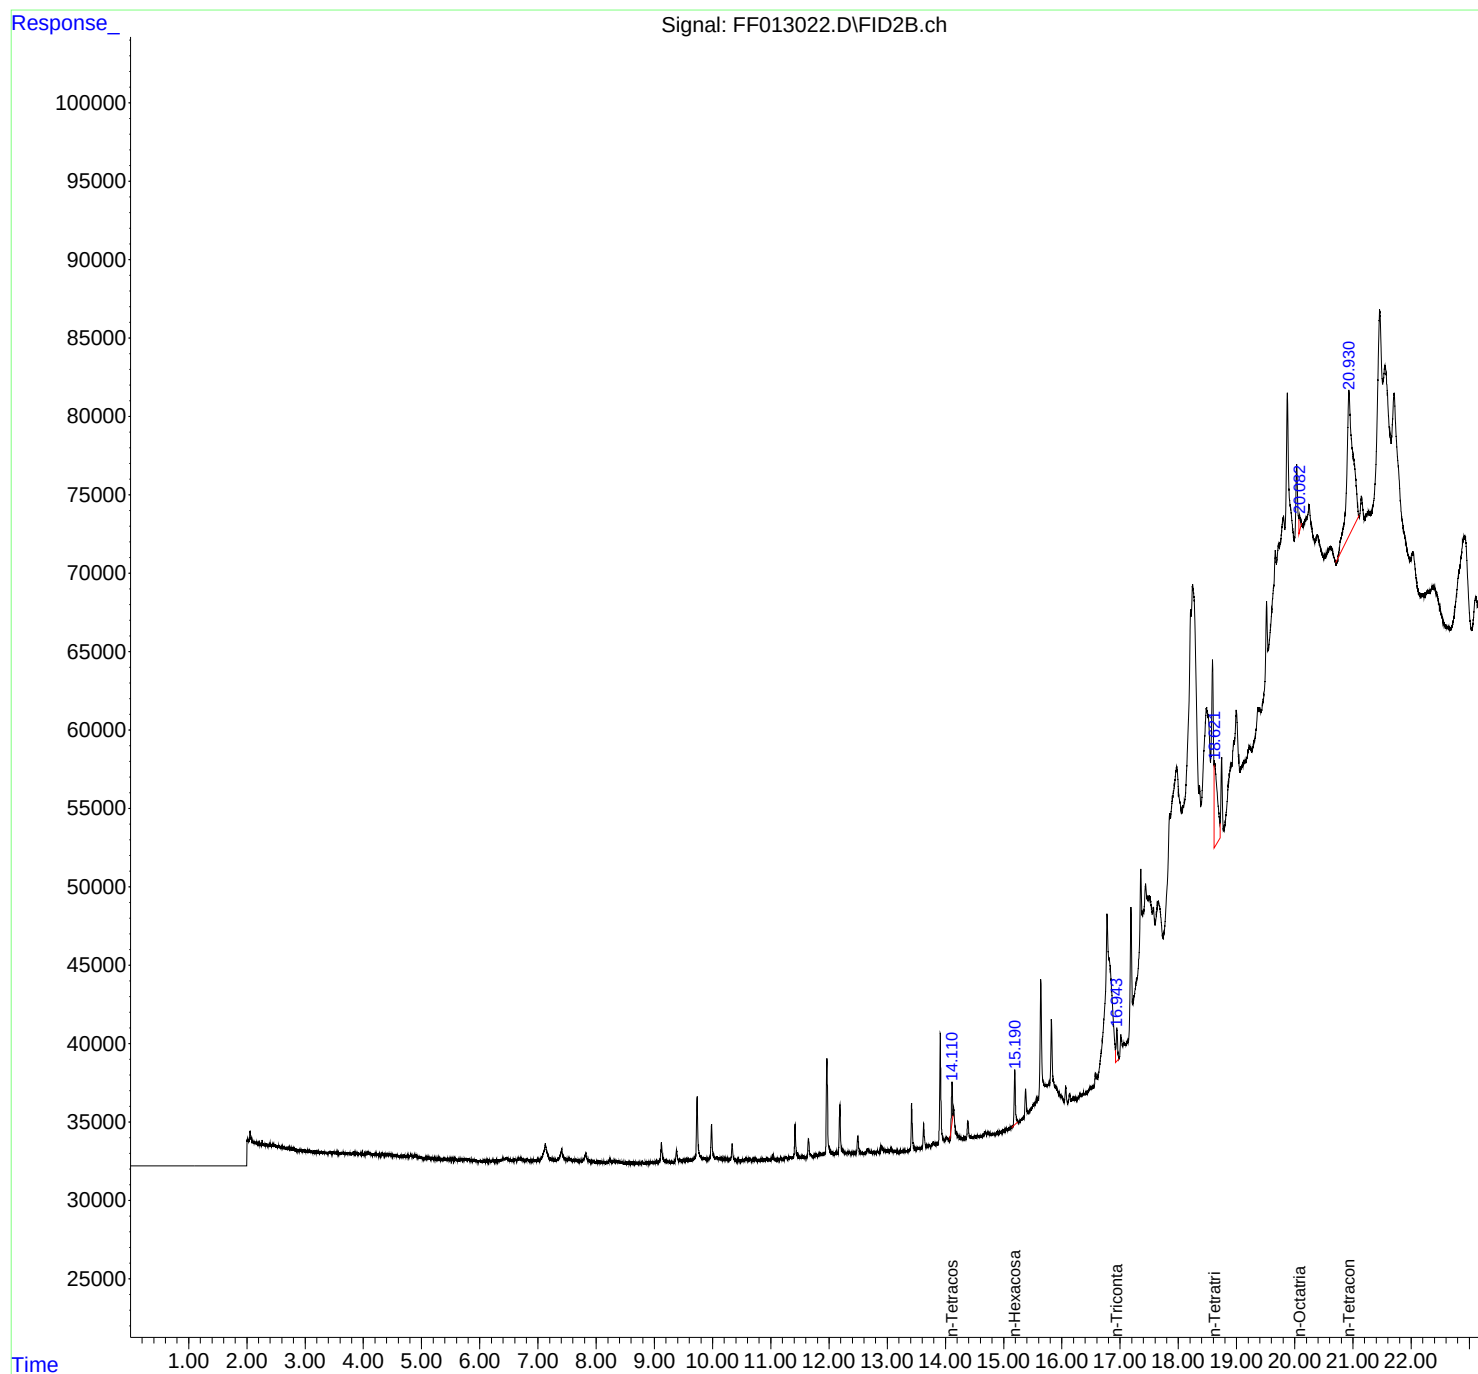


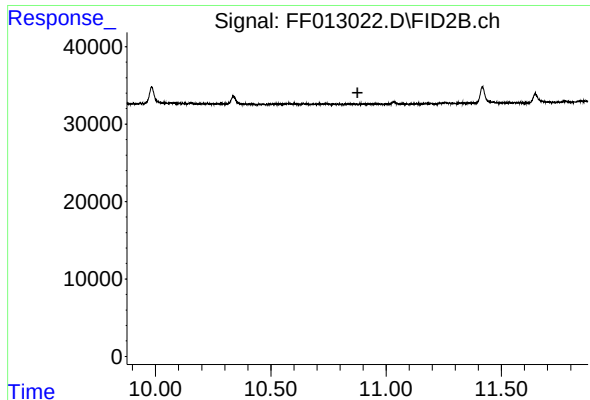

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 10.876 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

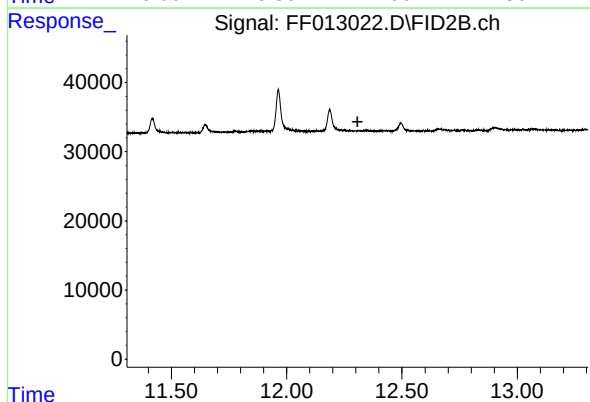


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.307 min
Response: 0
Conc: N.D.

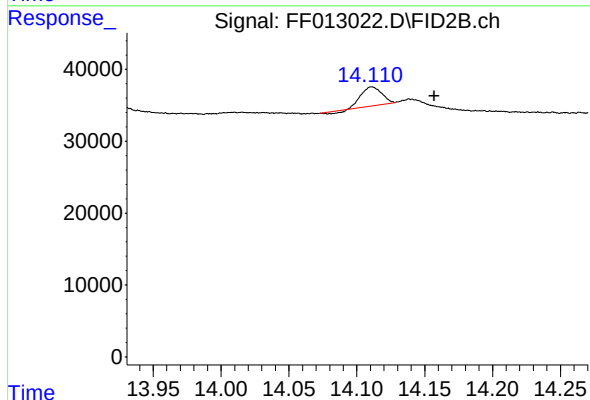


#14 n-Tetracosane (C24)

R.T.: 14.111 min
Delta R.T.: -0.046 min
Response: 26144
Conc: 0.21 ug/ml

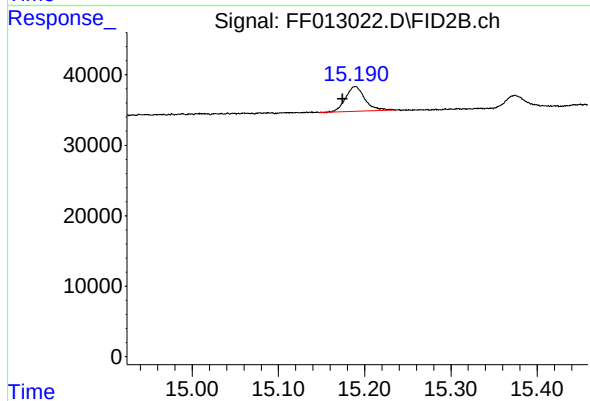

#15 n-Hexacosane (C26)


R.T.: 15.189 min
Delta R.T.: 0.014 min
Response: 54501
Conc: 0.45 ug/ml

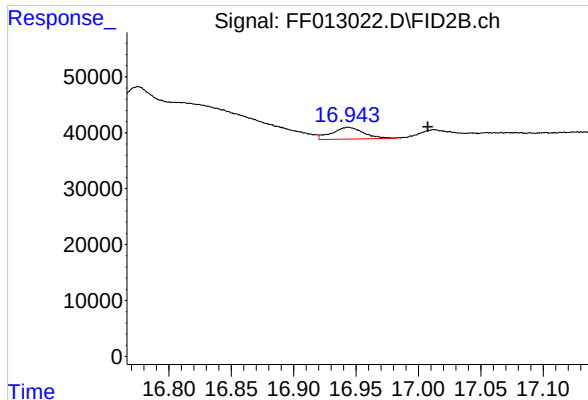

#17 n-Tricontane (C30)


R.T.: 16.944 min
Delta R.T.: -0.064 min
Response: 36372
Conc: 0.31 ug/ml

Instrument :
FID_F
ClientSampleId :

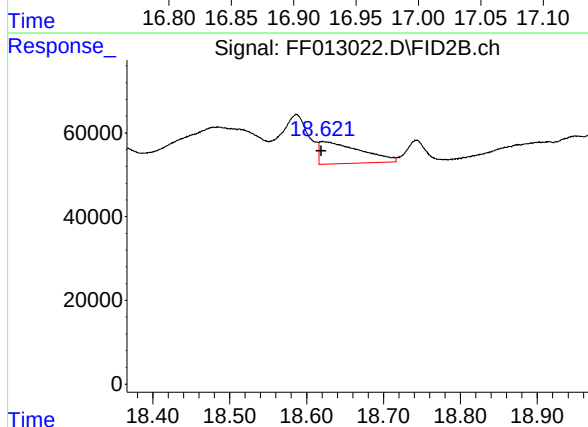


#19 n-Tetratriacontane (C34)

R.T.: 18.621 min
Delta R.T.: 0.002 min
Response: 193516
Conc: 1.74 ug/ml

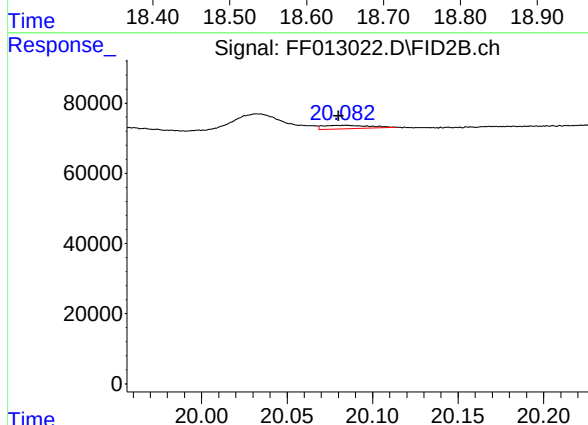

#21 n-Octatriacontane (C38)

R.T.: 20.085 min
Delta R.T.: 0.004 min
Response: 17783
Conc: 0.17 ug/ml

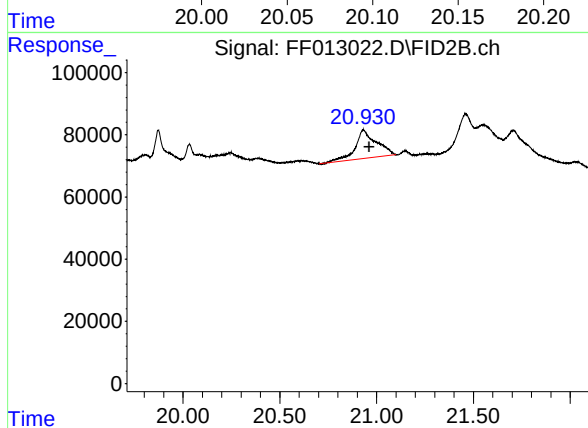

#22 n-Tetracontane (C40)

R.T.: 20.932 min
Delta R.T.: -0.031 min
Response: 693655
Conc: 7.16 ug/ml