

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062718\
 Data File : FF001112.D
 Signal(s) : FID2B.ch
 Acq On : 27 Jun 2018 13:24
 Operator : UA\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 28 02:18:16 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.474	5850003	50.727 ug/ml
Target Compounds			
2) N-DECANE	4.239	8603885	61.405 ug/ml
3) N-DODECANE	6.252	8131015	58.016 ug/ml
4) N-TETRADECANE	8.040	7709512	55.372 ug/ml
5) N-HEXADECANE	9.636	7351411	53.318 ug/ml
6) N-OCTADECANE	11.074	7094130	51.951 ug/ml
7) N-EICOSANE	12.381	6842075	51.069 ug/ml
8) N-DOCOSANE	13.577	6691848	50.609 ug/ml
10) N-TETRACOSANE	14.678	6626684	51.089 ug/ml
11) N-HEXACOSANE	15.697	6611746	51.475 ug/ml
12) N-OCTACOSANE	16.645	6731867	52.940 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062718\
Data File : FF001112.D
Signal(s) : FID2B.ch
Acq On : 27 Jun 2018 13:24
Operator : UA\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 28 02:18:16 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

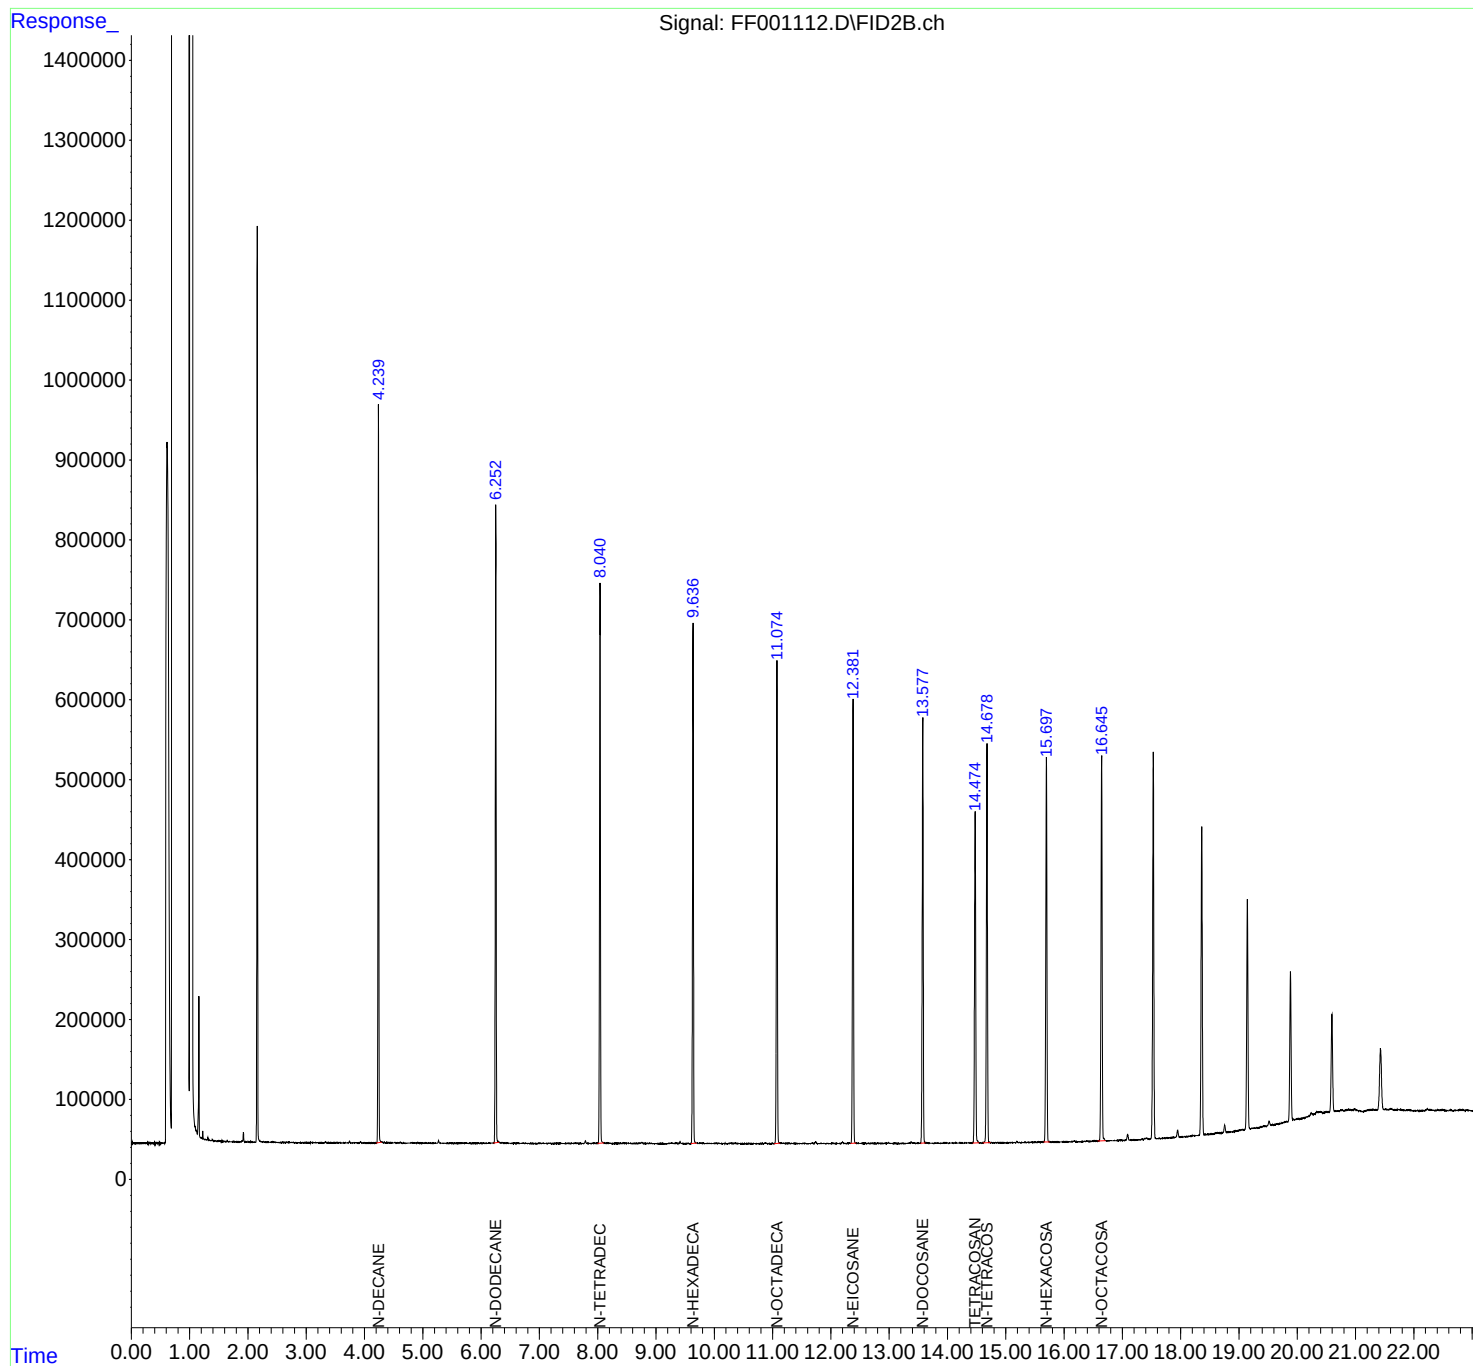


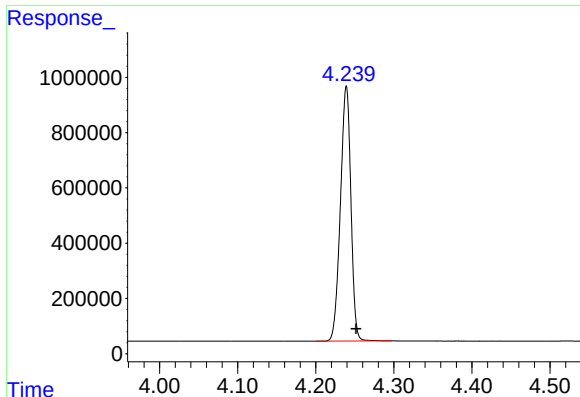

#2 N-DECANE


R.T.: 4.239 min
Delta R.T.: -0.013 min
Response: 8603885
Conc: 61.41 ug/ml

Instrument :
FID_F
ClientSampleId :

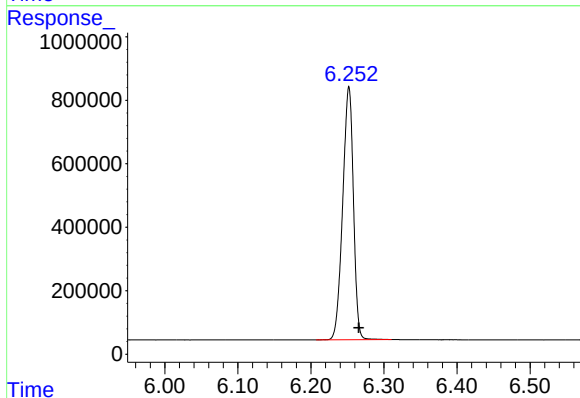


#3 N-DODECANE

R.T.: 6.252 min
Delta R.T.: -0.014 min
Response: 8131015
Conc: 58.02 ug/ml

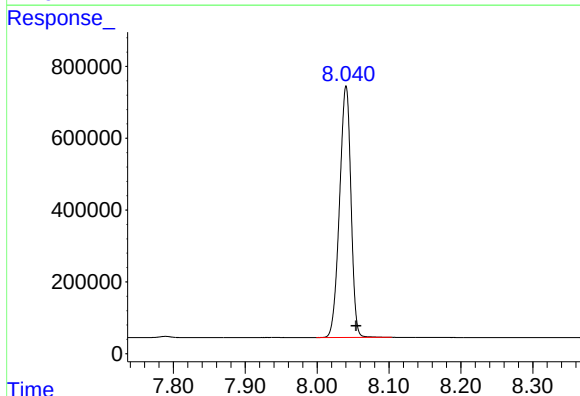


#4 N-TETRADECANE

R.T.: 8.040 min
Delta R.T.: -0.014 min
Response: 7709512
Conc: 55.37 ug/ml

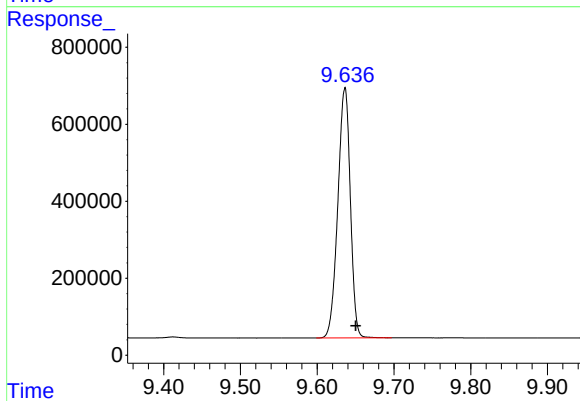

#5 N-HEXADECANE


R.T.: 9.636 min
Delta R.T.: -0.014 min
Response: 7351411
Conc: 53.32 ug/ml

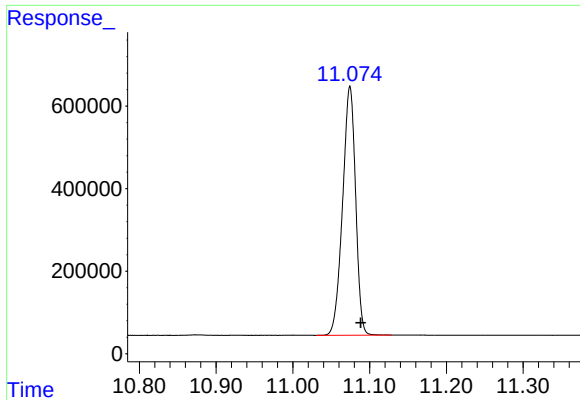

#6 N-OCTADECANE


R.T.: 11.074 min
Delta R.T.: -0.014 min
Response: 7094130
Conc: 51.95 ug/ml

Instrument :
FID_F
ClientSampleId :

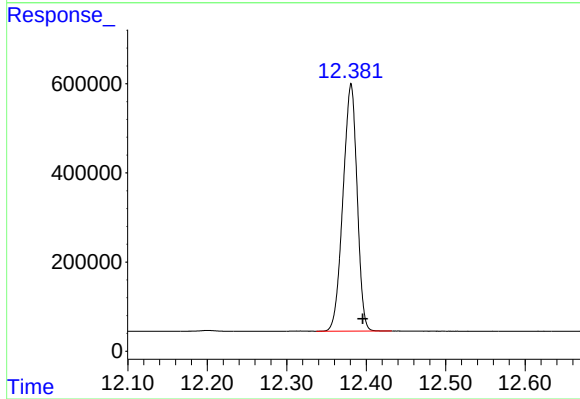


#7 N-EICOSANE

R.T.: 12.381 min
Delta R.T.: -0.015 min
Response: 6842075
Conc: 51.07 ug/ml

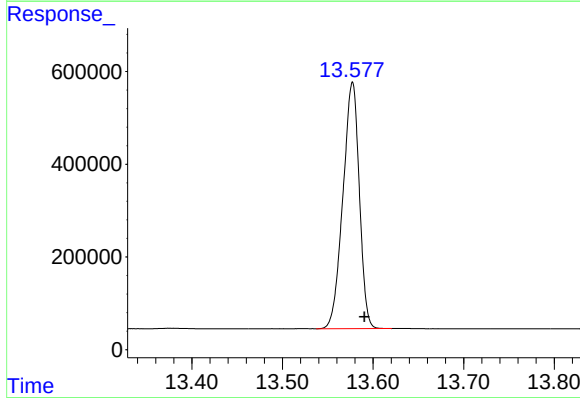


#8 N-DOCOSANE

R.T.: 13.577 min
Delta R.T.: -0.013 min
Response: 6691848
Conc: 50.61 ug/ml

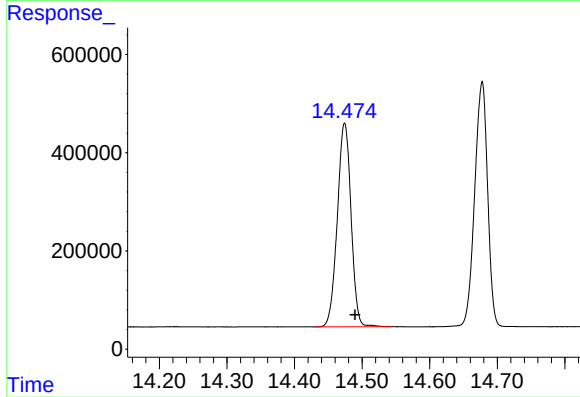

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.474 min
Delta R.T.: -0.016 min
Response: 5850003
Conc: 50.73 ug/ml

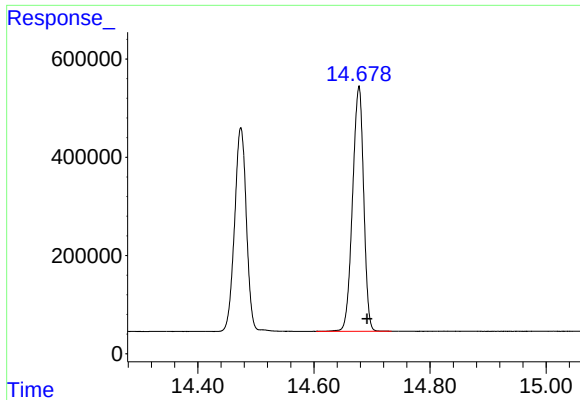

#10 N-TETRACOSANE


R.T.: 14.678 min
Delta R.T.: -0.014 min
Response: 6626684
Conc: 51.09 ug/ml

Instrument :
FID_F
ClientSampleId :

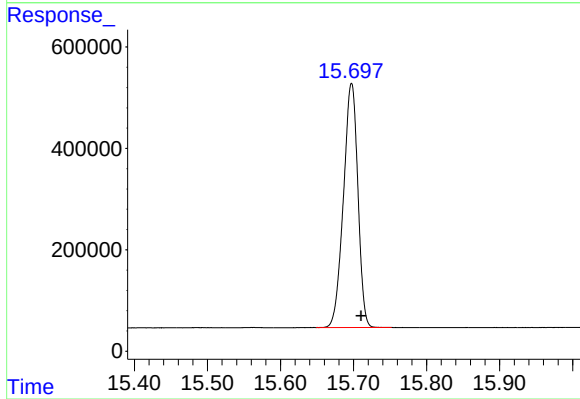

#11 N-HEXACOSANE

R.T.: 15.697 min
Delta R.T.: -0.013 min
Response: 6611746
Conc: 51.48 ug/ml

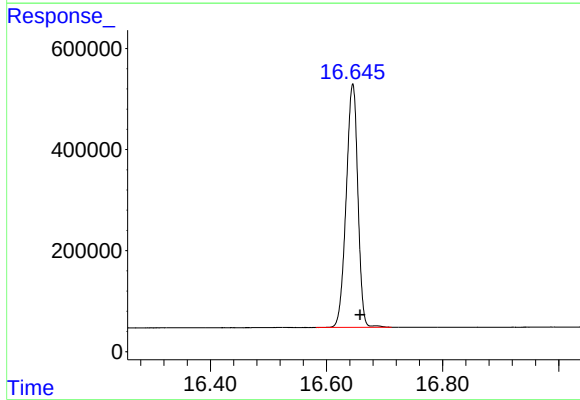

#12 N-OCTACOSANE

R.T.: 16.645 min
Delta R.T.: -0.012 min
Response: 6731867
Conc: 52.94 ug/ml