

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062718\
 Data File : FF001114.D
 Signal(s) : FID2B.ch
 Acq On : 27 Jun 2018 15:46
 Operator : UA\AJ
 Sample : PB110656BS
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB110656BS

Integration File: autoint1.e
 Quant Time: Jun 28 02:18:46 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.467	1839546	15.951 ug/ml
Target Compounds			
2) N-DECANE	4.217	2788214	19.899 ug/ml
3) N-DODECANE	6.233	2679652	19.120 ug/ml
4) N-TETRADECANE	8.025	2585738	18.572 ug/ml
5) N-HEXADECANE	9.623	2485660	18.028 ug/ml
6) N-OCTADECANE	11.063	2460459	18.018 ug/ml
7) N-EICOSANE	12.370	2380688	17.769 ug/ml
8) N-DOCOSANE	13.568	2331939	17.636 ug/ml
10) N-TETRACOSANE	14.669	2334128	17.995 ug/ml
11) N-HEXACOSANE	15.689	2286832	17.804 ug/ml
12) N-OCTACOSANE	16.638	2324137	18.277 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062718\
Data File : FF001114.D
Signal(s) : FID2B.ch
Acq On : 27 Jun 2018 15:46
Operator : UA\AJ
Sample : PB110656BS
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB110656BS

Integration File: autoint1.e
Quant Time: Jun 28 02:18:46 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

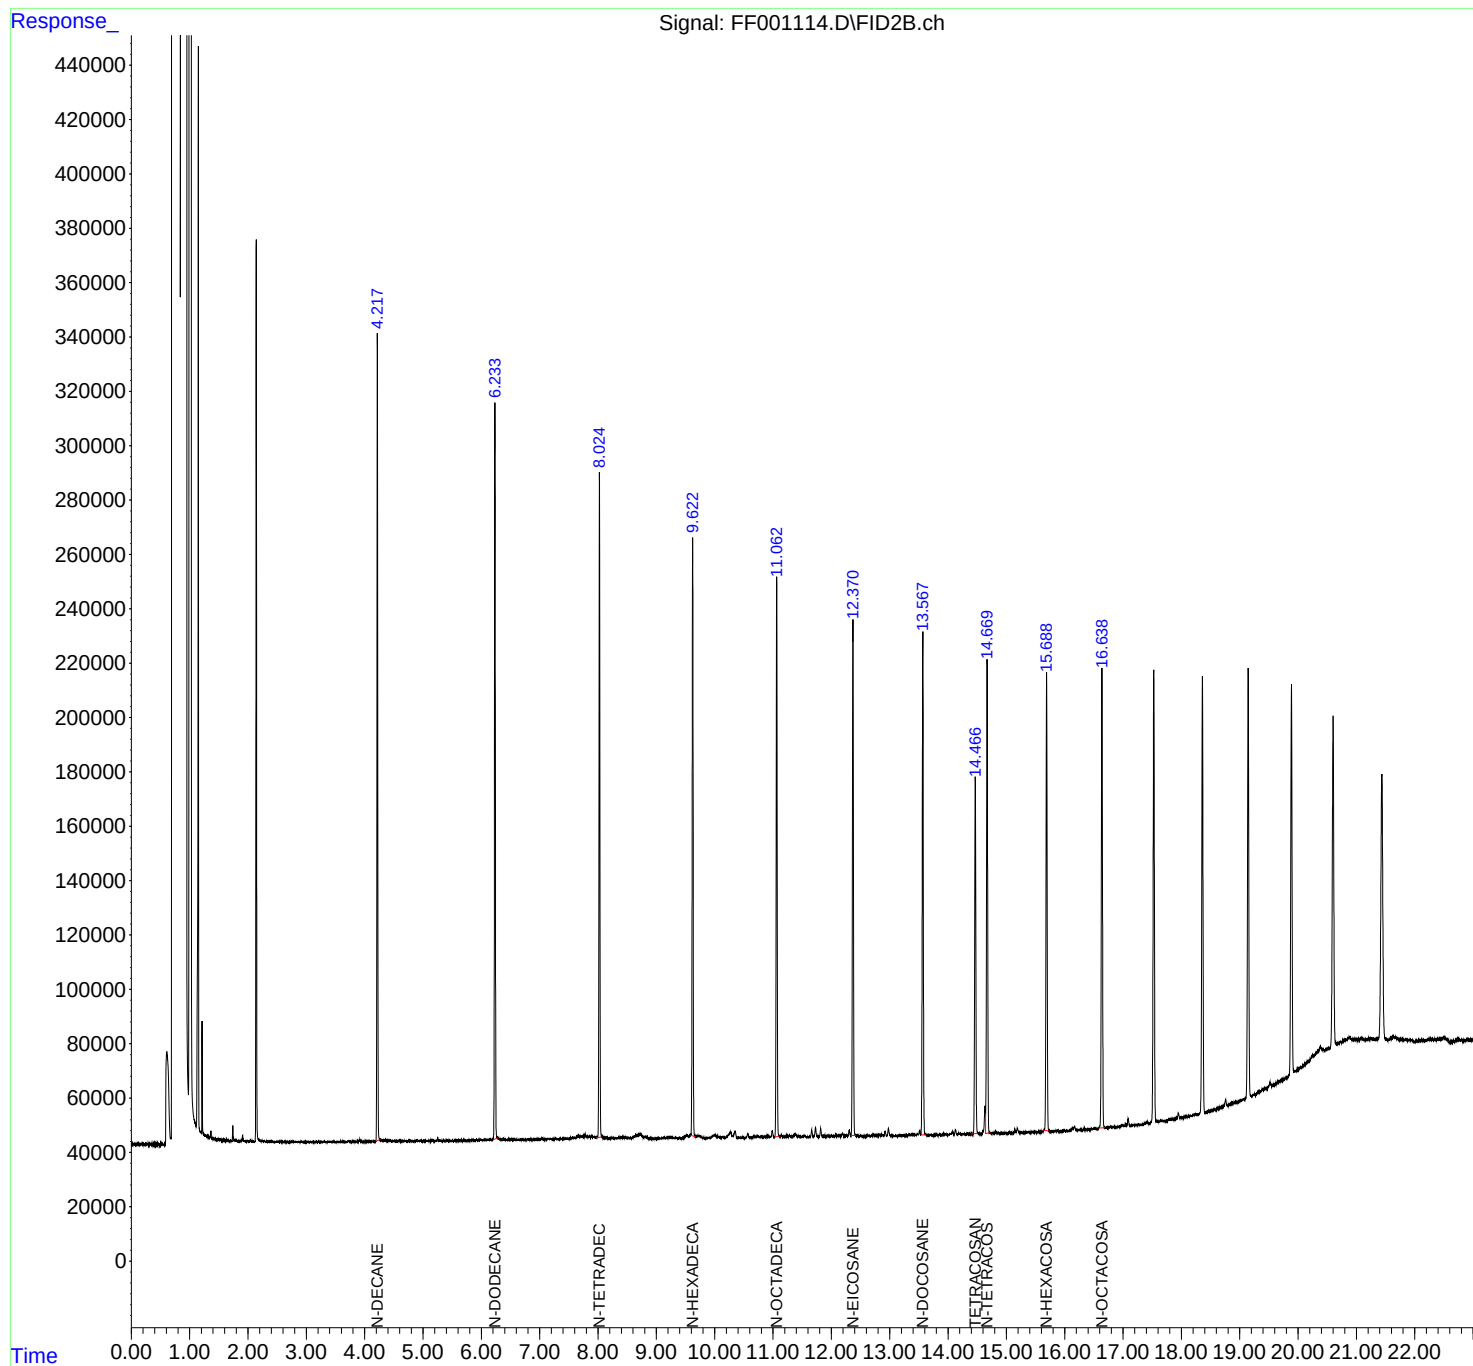


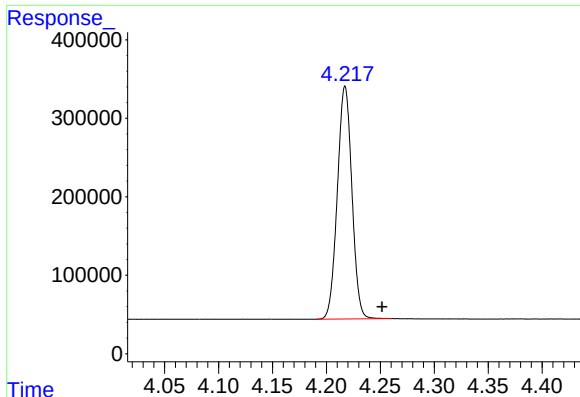

#2 N-DECANE


R.T.: 4.217 min
Delta R.T.: -0.034 min
Response: 2788214
Conc: 19.90 ug/ml

Instrument :
FID_F
ClientSampleId :
PB110656BS

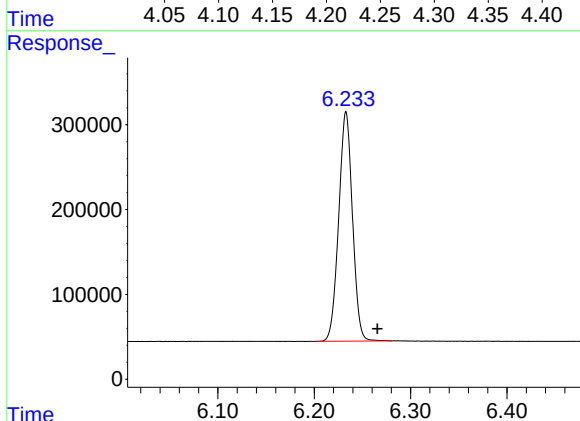


#3 N-DODECANE

R.T.: 6.233 min
Delta R.T.: -0.033 min
Response: 2679652
Conc: 19.12 ug/ml

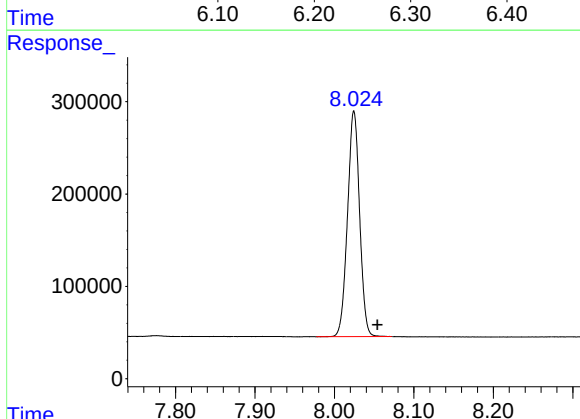


#4 N-TETRADECANE

R.T.: 8.025 min
Delta R.T.: -0.030 min
Response: 2585738
Conc: 18.57 ug/ml

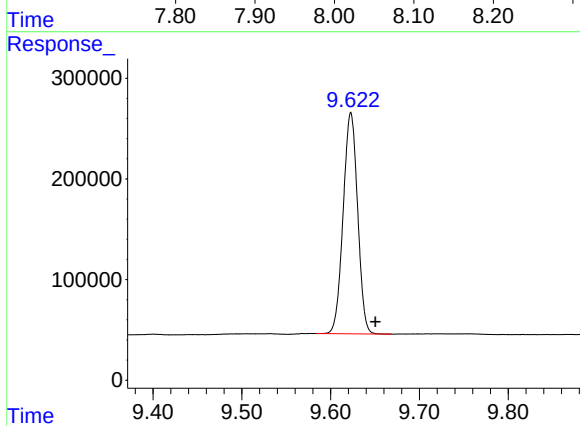

#5 N-HEXADECANE


R.T.: 9.623 min
Delta R.T.: -0.027 min
Response: 2485660
Conc: 18.03 ug/ml

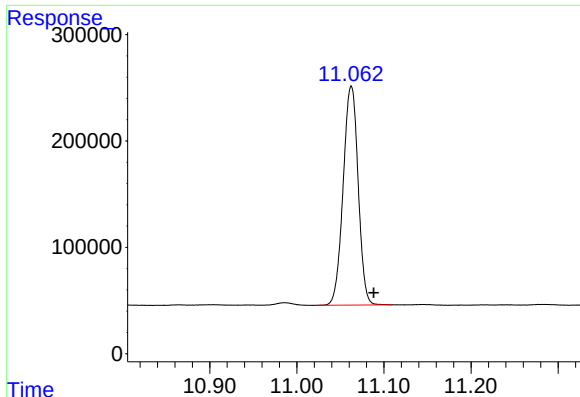

#6 N-OCTADECANE


R.T.: 11.063 min
Delta R.T.: -0.026 min
Response: 2460459
Conc: 18.02 ug/ml

Instrument :
FID_F
ClientSampleId :
PB110656BS

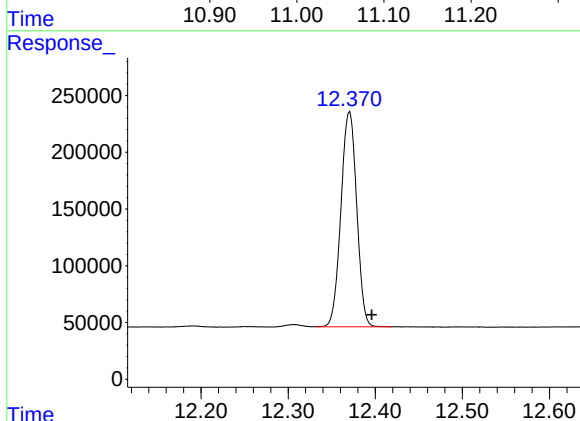


#7 N-EICOSANE

R.T.: 12.370 min
Delta R.T.: -0.026 min
Response: 2380688
Conc: 17.77 ug/ml

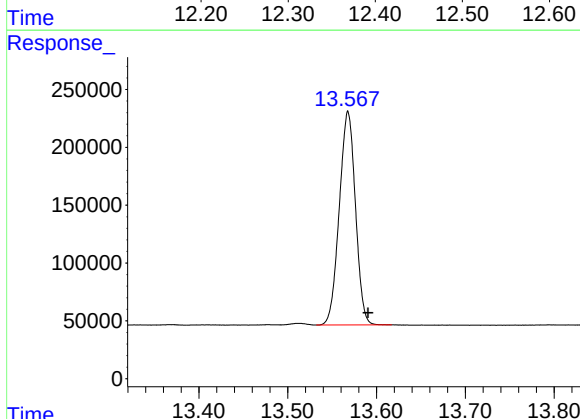


#8 N-DOCOSANE

R.T.: 13.568 min
Delta R.T.: -0.023 min
Response: 2331939
Conc: 17.64 ug/ml

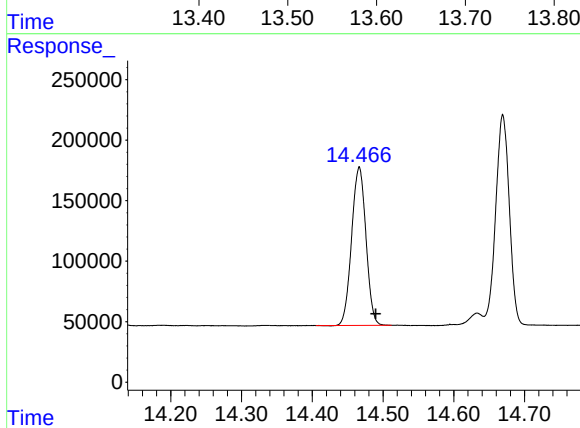

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.467 min
Delta R.T.: -0.023 min
Response: 1839546
Conc: 15.95 ug/ml

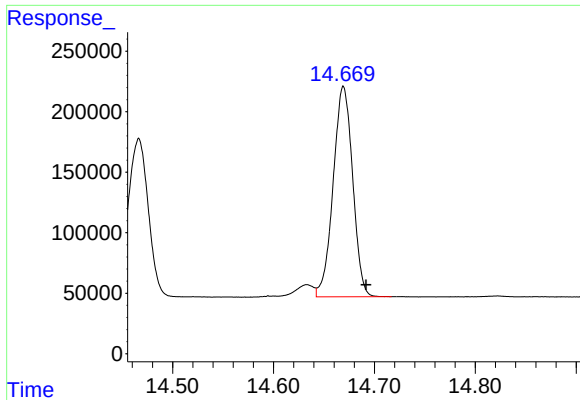

#10 N-TETRACOSANE


R.T.: 14.669 min
Delta R.T.: -0.022 min
Response: 2334128
Conc: 18.00 ug/ml

Instrument :
FID_F
ClientSampleId :
PB110656BS

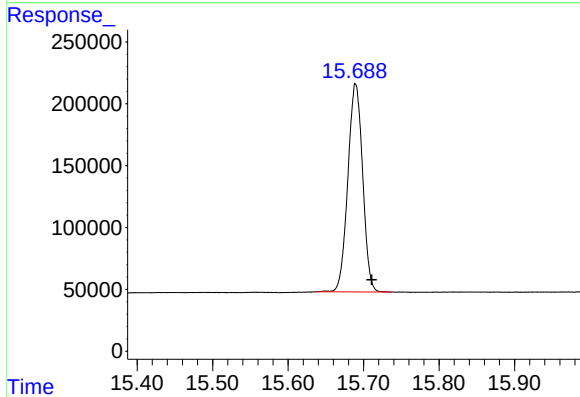

#11 N-HEXACOSANE

R.T.: 15.689 min
Delta R.T.: -0.021 min
Response: 2286832
Conc: 17.80 ug/ml

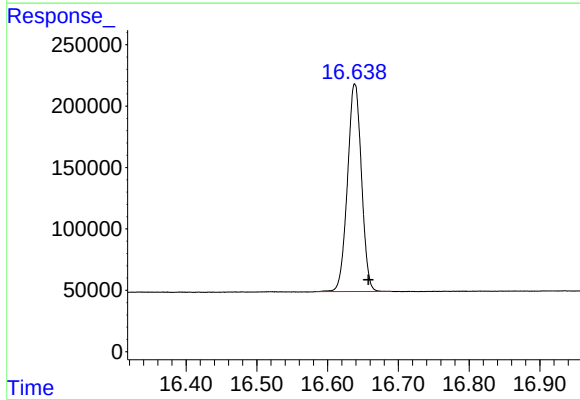

#12 N-OCTACOSANE

R.T.: 16.638 min
Delta R.T.: -0.019 min
Response: 2324137
Conc: 18.28 ug/ml