

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062718\
 Data File : FF001127.D
 Signal(s) : FID2B.ch
 Acq On : 27 Jun 2018 22:14
 Operator : UA\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 28 03:28:33 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.473	5050905	43.797 ug/ml
Target Compounds			
2) N-DECANE	4.237	7668279	54.728 ug/ml
3) N-DODECANE	6.251	7161192	51.096 ug/ml
4) N-TETRADECANE	8.038	6750103	48.482 ug/ml
5) N-HEXADECANE	9.634	6407478	46.472 ug/ml
6) N-OCTADECANE	11.072	6156557	45.085 ug/ml
7) N-EICOSANE	12.379	5919398	44.182 ug/ml
8) N-DOCOSANE	13.575	5778217	43.699 ug/ml
10) N-TETRACOSANE	14.676	5711183	44.031 ug/ml
11) N-HEXACOSANE	15.695	5692674	44.320 ug/ml
12) N-OCTACOSANE	16.644	5806823	45.666 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062718\
Data File : FF001127.D
Signal(s) : FID2B.ch
Acq On : 27 Jun 2018 22:14
Operator : UA\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 28 03:28:33 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

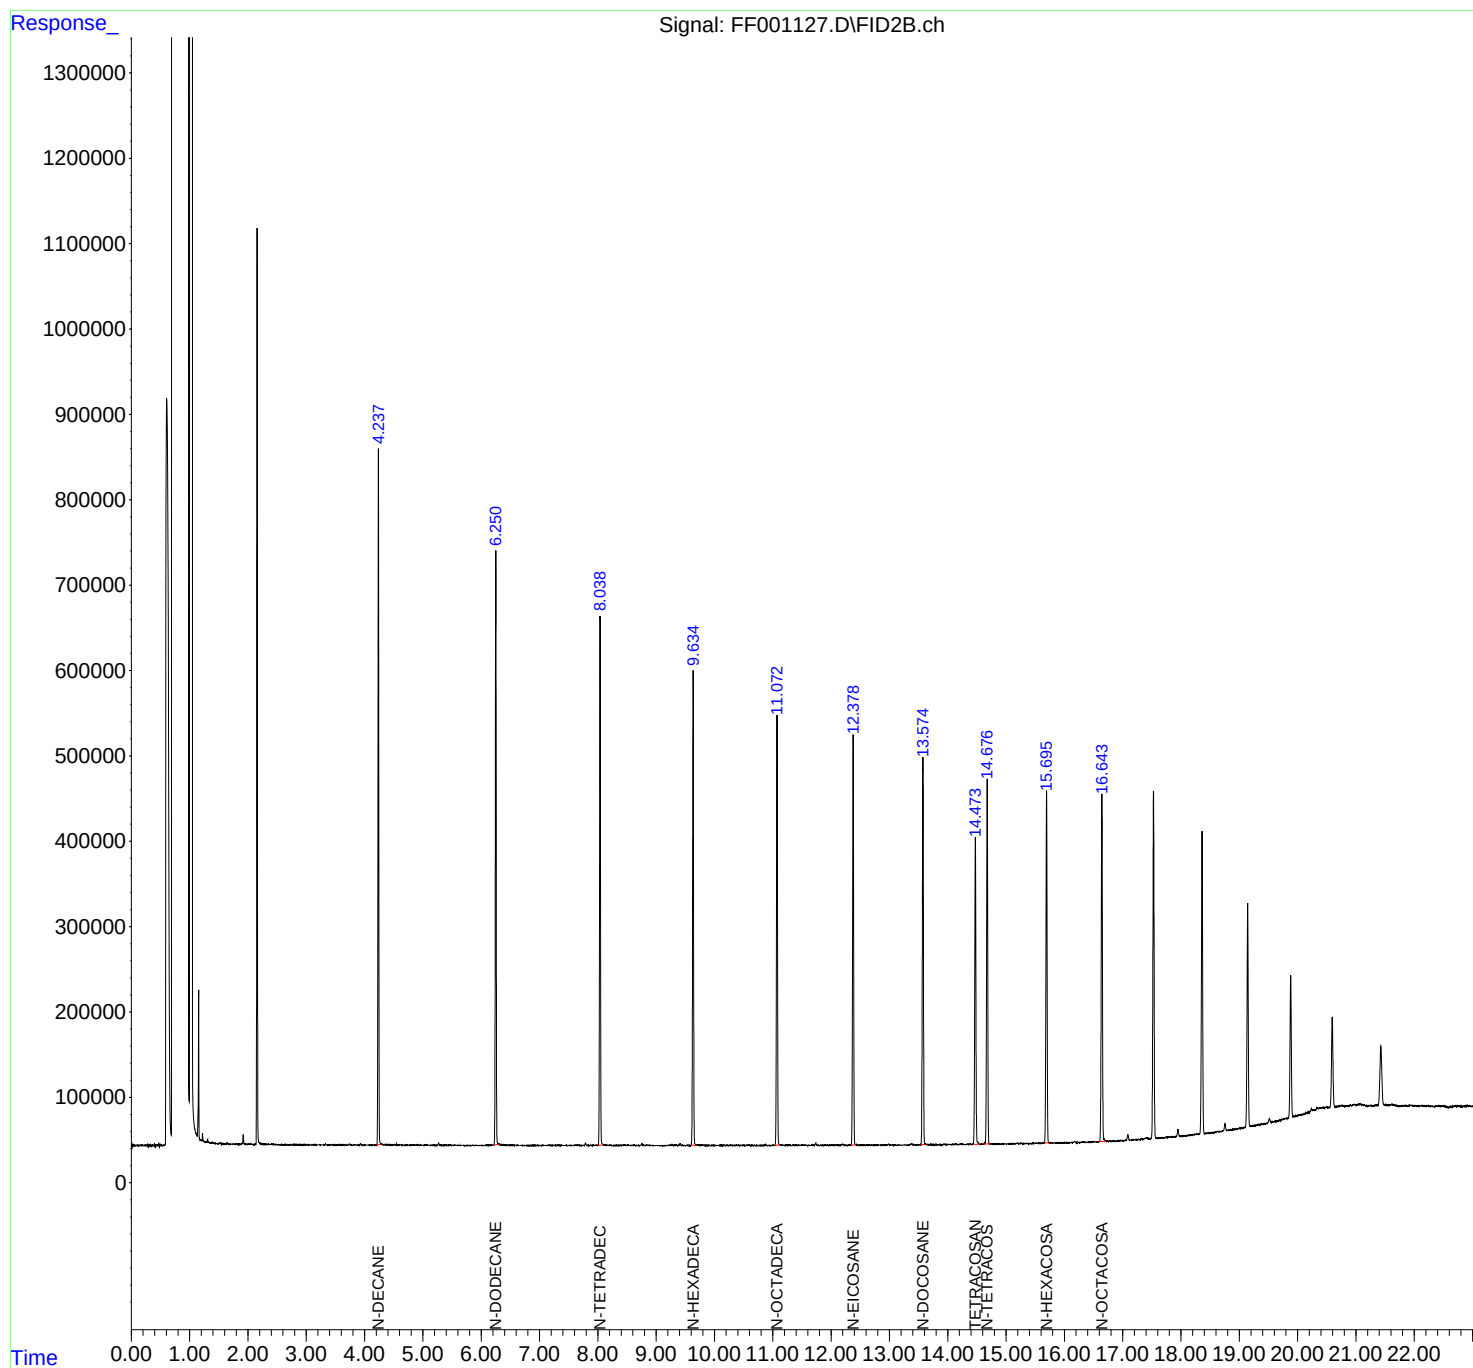


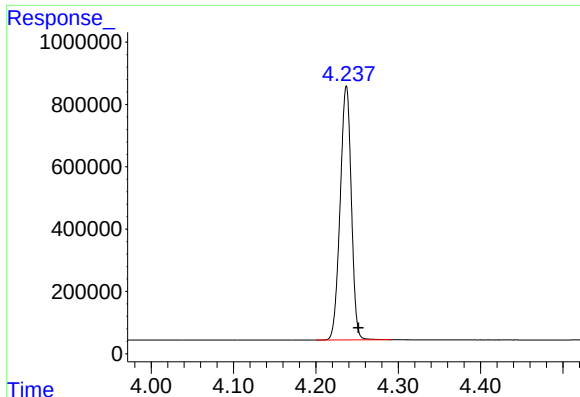

#2 N-DECANE


R.T.: 4.237 min
Delta R.T.: -0.015 min
Response: 7668279
Conc: 54.73 ug/ml

Instrument :
FID_F
ClientSampleId :

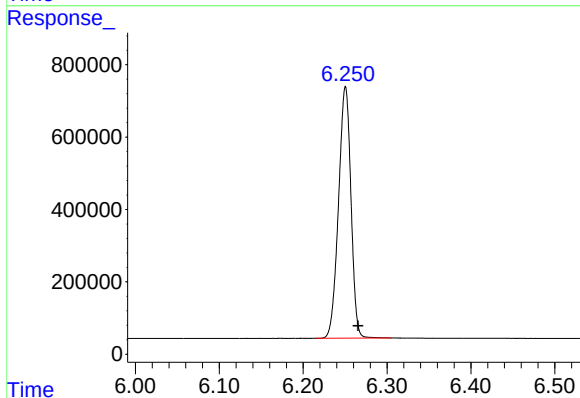


#3 N-DODECANE

R.T.: 6.251 min
Delta R.T.: -0.015 min
Response: 7161192
Conc: 51.10 ug/ml

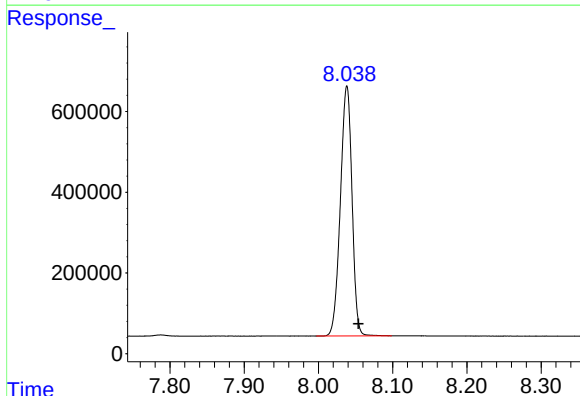


#4 N-TETRADECANE

R.T.: 8.038 min
Delta R.T.: -0.016 min
Response: 6750103
Conc: 48.48 ug/ml

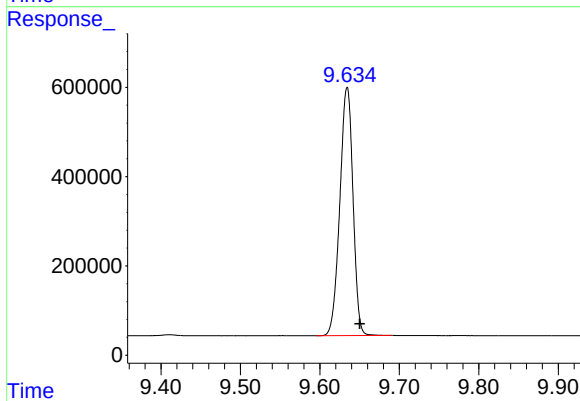

#5 N-HEXADECANE


R.T.: 9.634 min
Delta R.T.: -0.016 min
Response: 6407478
Conc: 46.47 ug/ml

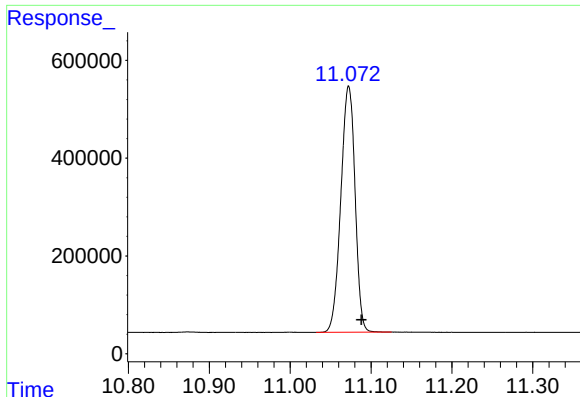

#6 N-OCTADECANE


R.T.: 11.072 min
Delta R.T.: -0.016 min
Response: 6156557
Conc: 45.09 ug/ml

Instrument :
FID_F
ClientSampleId :

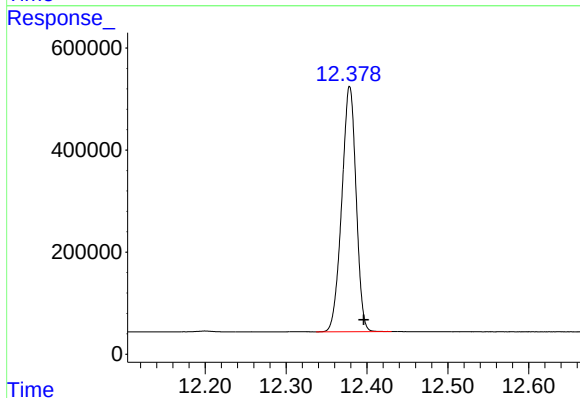


#7 N-EICOSANE

R.T.: 12.379 min
Delta R.T.: -0.017 min
Response: 5919398
Conc: 44.18 ug/ml

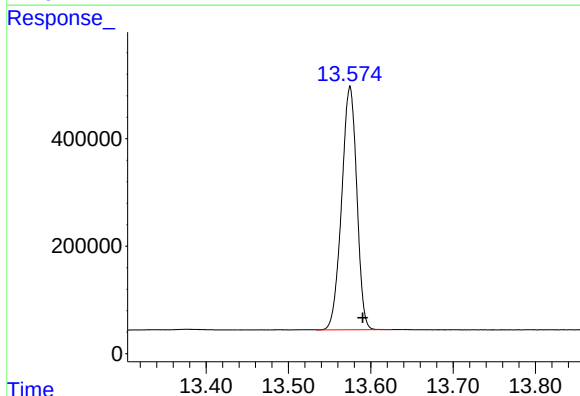


#8 N-DOCOSANE

R.T.: 13.575 min
Delta R.T.: -0.016 min
Response: 5778217
Conc: 43.70 ug/ml

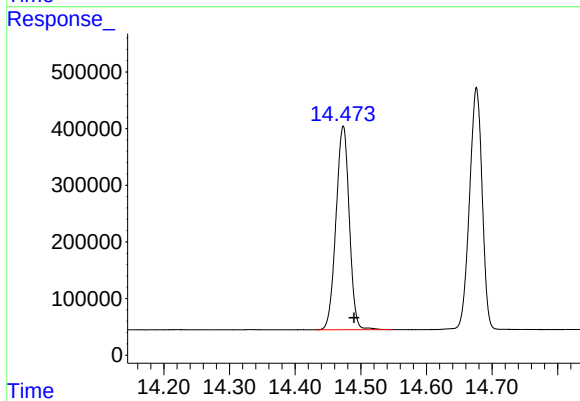

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.473 min
Delta R.T.: -0.016 min
Response: 5050905
Conc: 43.80 ug/ml

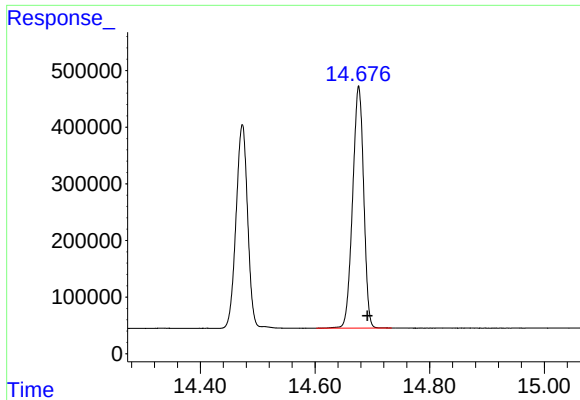

#10 N-TETRACOSANE


R.T.: 14.676 min
Delta R.T.: -0.015 min
Response: 5711183
Conc: 44.03 ug/ml

Instrument :
FID_F
ClientSampleId :

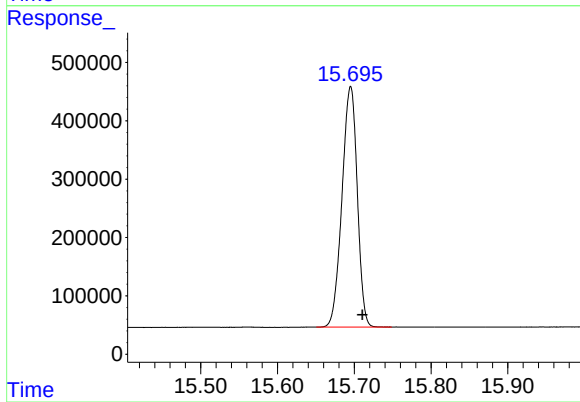

#11 N-HEXACOSANE

R.T.: 15.695 min
Delta R.T.: -0.015 min
Response: 5692674
Conc: 44.32 ug/ml

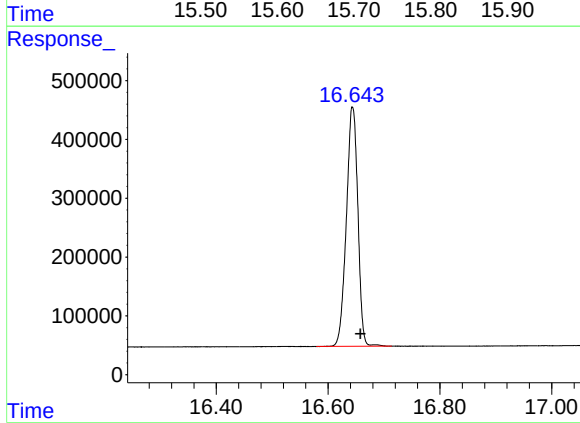

#12 N-OCTACOSANE

R.T.: 16.644 min
Delta R.T.: -0.014 min
Response: 5806823
Conc: 45.67 ug/ml