

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062719\
Data File : FF004866.D
Signal(s) : FID2B.ch
Acq On : 27 Jun 2019 09:11
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 28 01:09:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.622	131003	1.150 ug/ml
16)	N-HEXATRIACONTANE	20.187	190813	1.843 ug/ml
18)	N-TETRACONTANE	21.865	244351	2.102 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062719\
Data File : FF004866.D
Signal(s) : FID2B.ch
Acq On : 27 Jun 2019 09:11
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 28 01:09:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

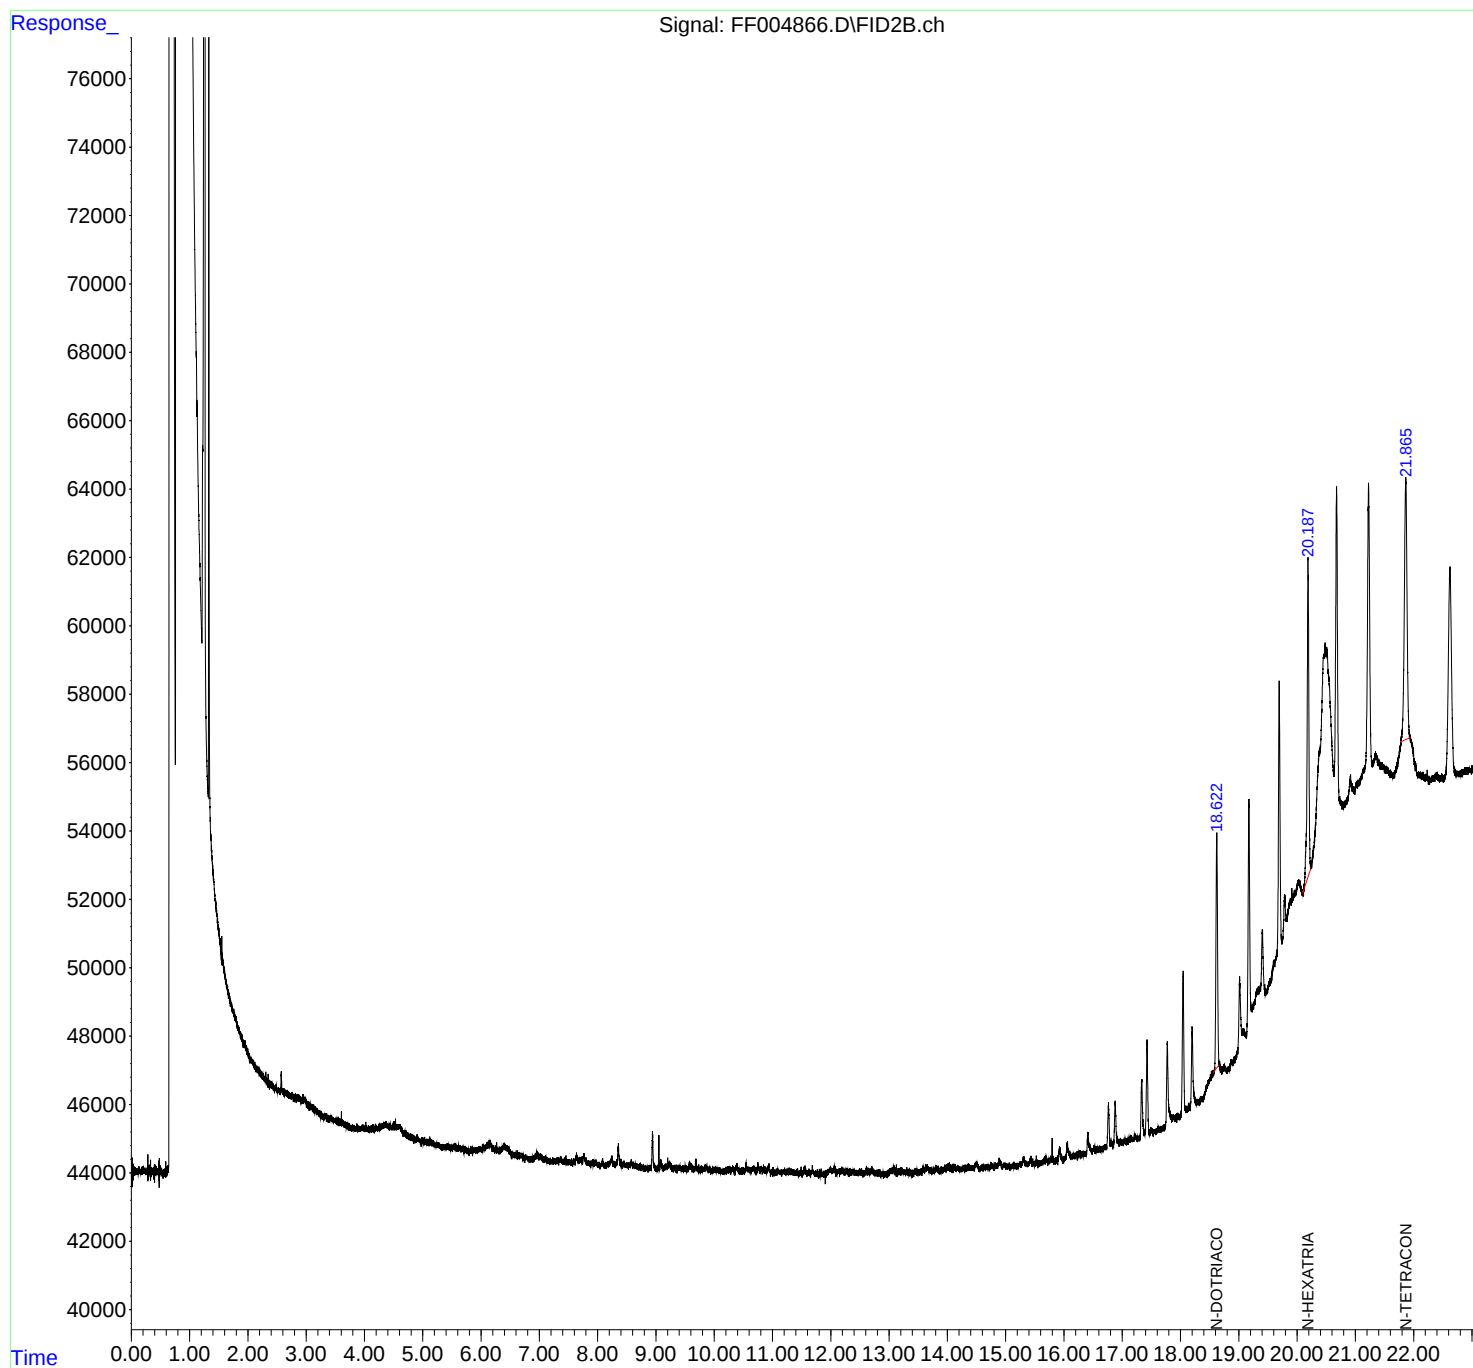


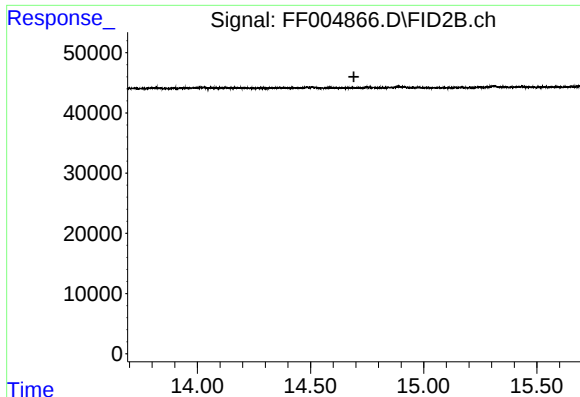

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.692 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

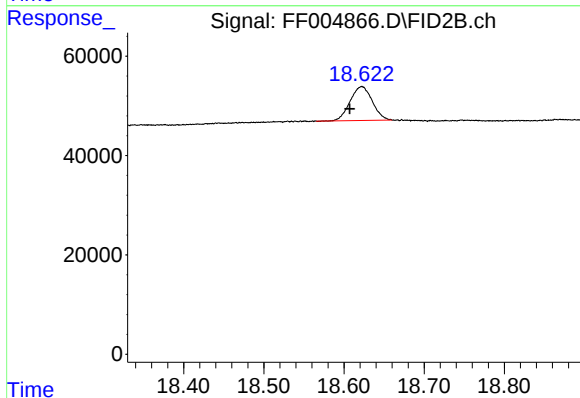


#14 N-DOTRIACONTANE

R.T.: 18.622 min
Delta R.T.: 0.015 min
Response: 131003
Conc: 1.15 ug/ml

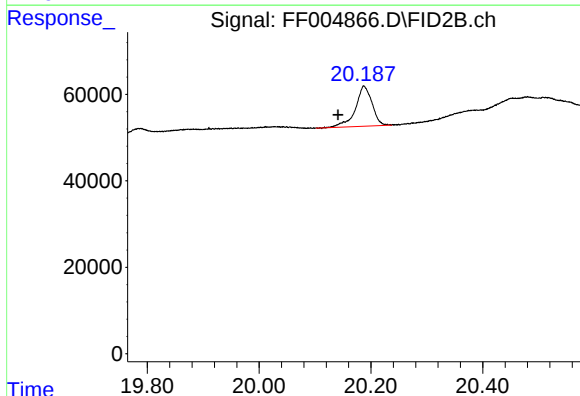

#16 N-HEXATRIACONTANE

R.T.: 20.187 min
Delta R.T.: 0.046 min
Response: 190813
Conc: 1.84 ug/ml

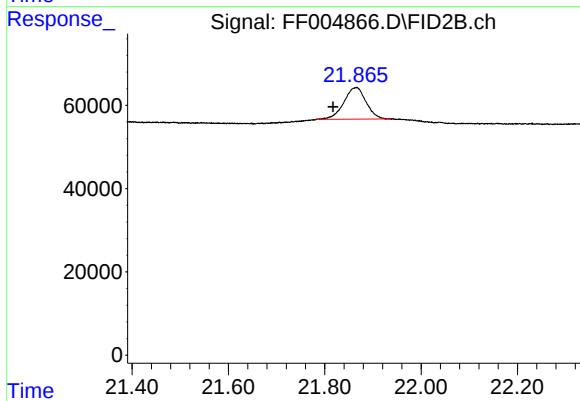

#18 N-TETRACONTANE

R.T.: 21.865 min
Delta R.T.: 0.048 min
Response: 244351
Conc: 2.10 ug/ml