

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062719\
 Data File : FF004869.D
 Signal(s) : FID2B.ch
 Acq On : 27 Jun 2019 11:56
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Jun 28 01:09:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
 Quant Title :
 QLast Update : Wed Jun 26 14:27:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.418	5221873	41.155 ug/ml
12) N-OCTACOSANE	16.877	4682763	41.983 ug/ml
13) N-TRIACONTANE	17.770	112295	1.000 ug/ml
14) N-DOTRIACONTANE	18.616	176803	1.552 ug/ml
16) N-HEXATRIACONTANE	20.195f	171351	1.655 ug/ml
18) N-TETRACONTANE	21.875f	293346	2.523 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062719\
Data File : FF004869.D
Signal(s) : FID2B.ch
Acq On : 27 Jun 2019 11:56
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Jun 28 01:09:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

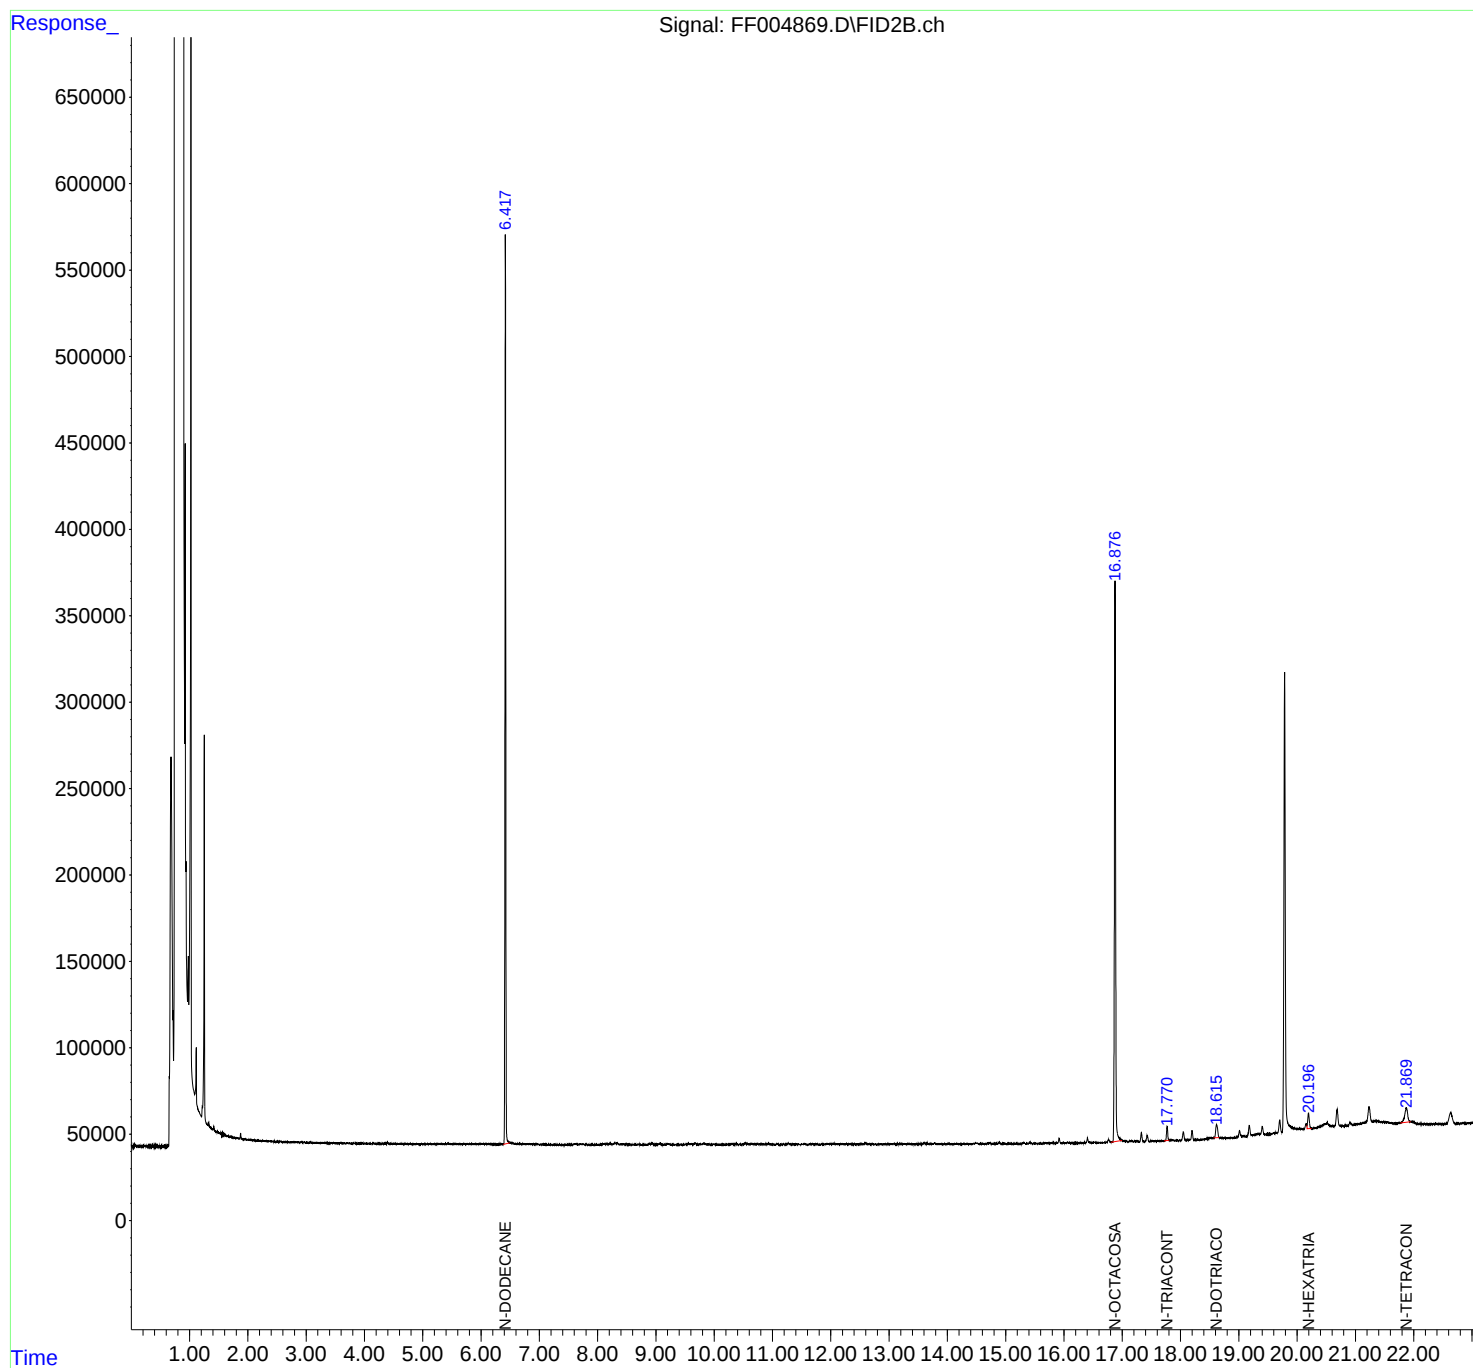


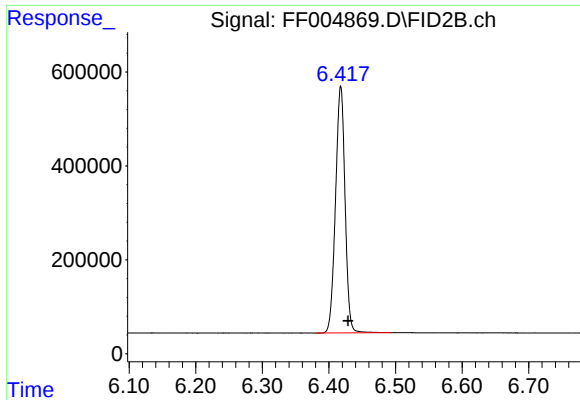

#3 N-DODECANE


R.T.: 6.418 min
Delta R.T.: -0.011 min
Response: 5221873
Conc: 41.16 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

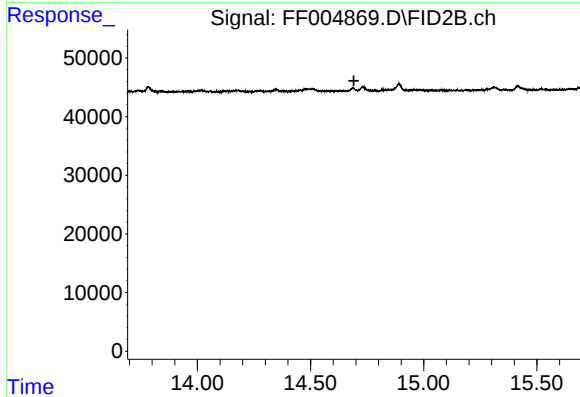


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.692 min
Response: 0
Conc: N.D.

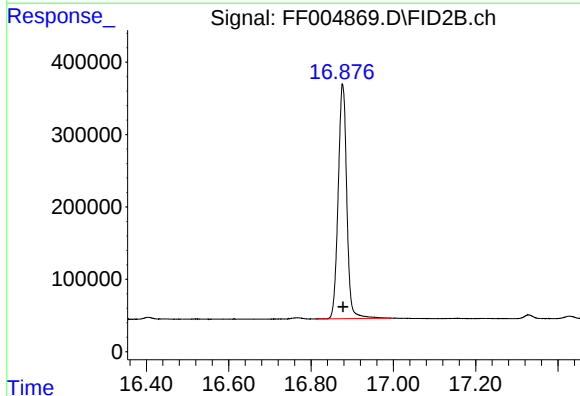


#12 N-OCTACOSANE

R.T.: 16.877 min
Delta R.T.: 0.000 min
Response: 4682763
Conc: 41.98 ug/ml

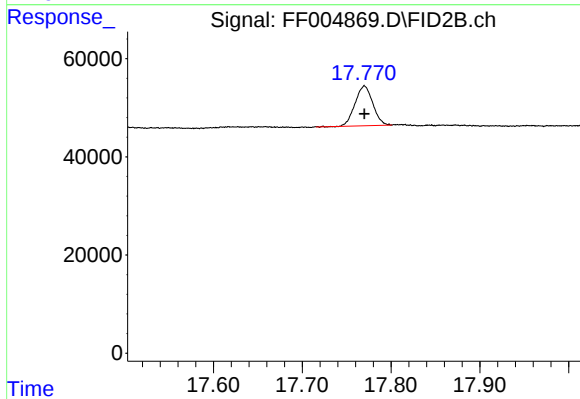

#13 N-TRIACONTANE


R.T.: 17.770 min
Delta R.T.: 0.000 min
Response: 112295
Conc: 1.00 ug/ml

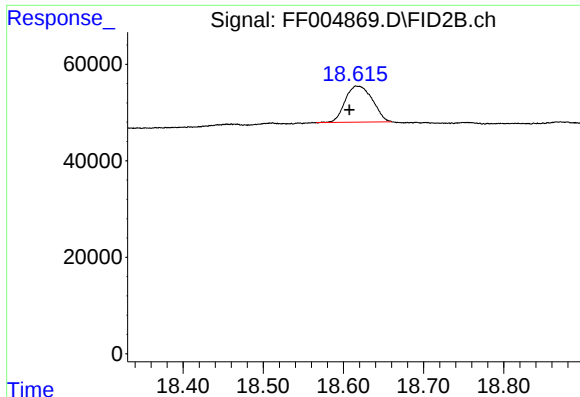

#14 N-DOTRIACONTANE


R.T.: 18.616 min
Delta R.T.: 0.009 min
Response: 176803
Conc: 1.55 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

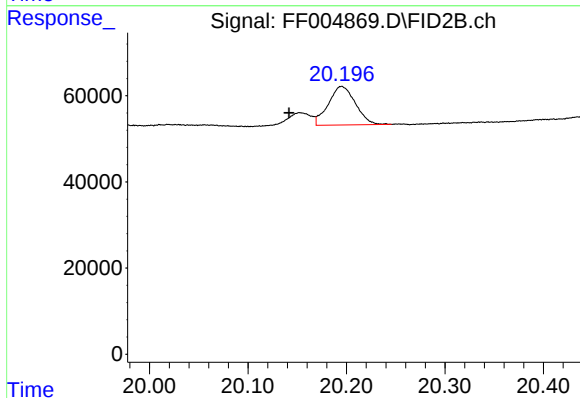

#16 N-HEXATRIACONTANE

R.T.: 20.195 min
Delta R.T.: 0.053 min
Response: 171351
Conc: 1.65 ug/ml

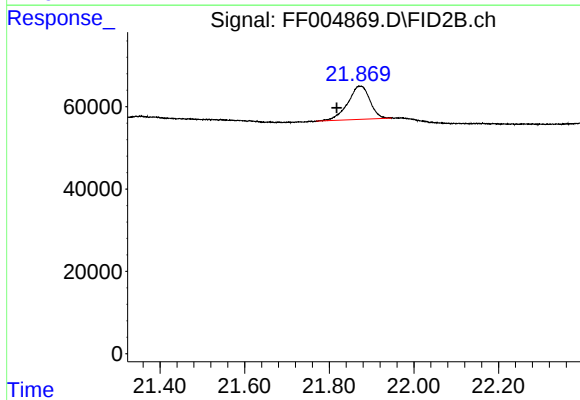

#18 N-TETRACONTANE

R.T.: 21.875 min
Delta R.T.: 0.058 min
Response: 293346
Conc: 2.52 ug/ml