

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062719\
 Data File : FF004872.D
 Signal(s) : FID2B.ch
 Acq On : 27 Jun 2019 15:39
 Operator : DD\AJ
 Sample : K3551-01
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SIMW-02-20190625

Integration File: autoint1.e
 Quant Time: Jun 28 01:10:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
 Quant Title :
 QLast Update : Wed Jun 26 14:27:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.688	2474273	25.440 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.871	131687	1.181 ug/ml
13) N-TRIACONTANE	17.765	166505	1.482 ug/ml
14) N-DOTRIACONTANE	18.617	306384	2.690 ug/ml
16) N-HEXATRIACONTANE	20.185	337611	3.260 ug/ml
18) N-TETRACONTANE	21.860	631005	5.428 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062719\
Data File : FF004872.D
Signal(s) : FID2B.ch
Acq On : 27 Jun 2019 15:39
Operator : DD\AJ
Sample : K3551-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SIMW-02-20190625

Integration File: autoint1.e
Quant Time: Jun 28 01:10:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

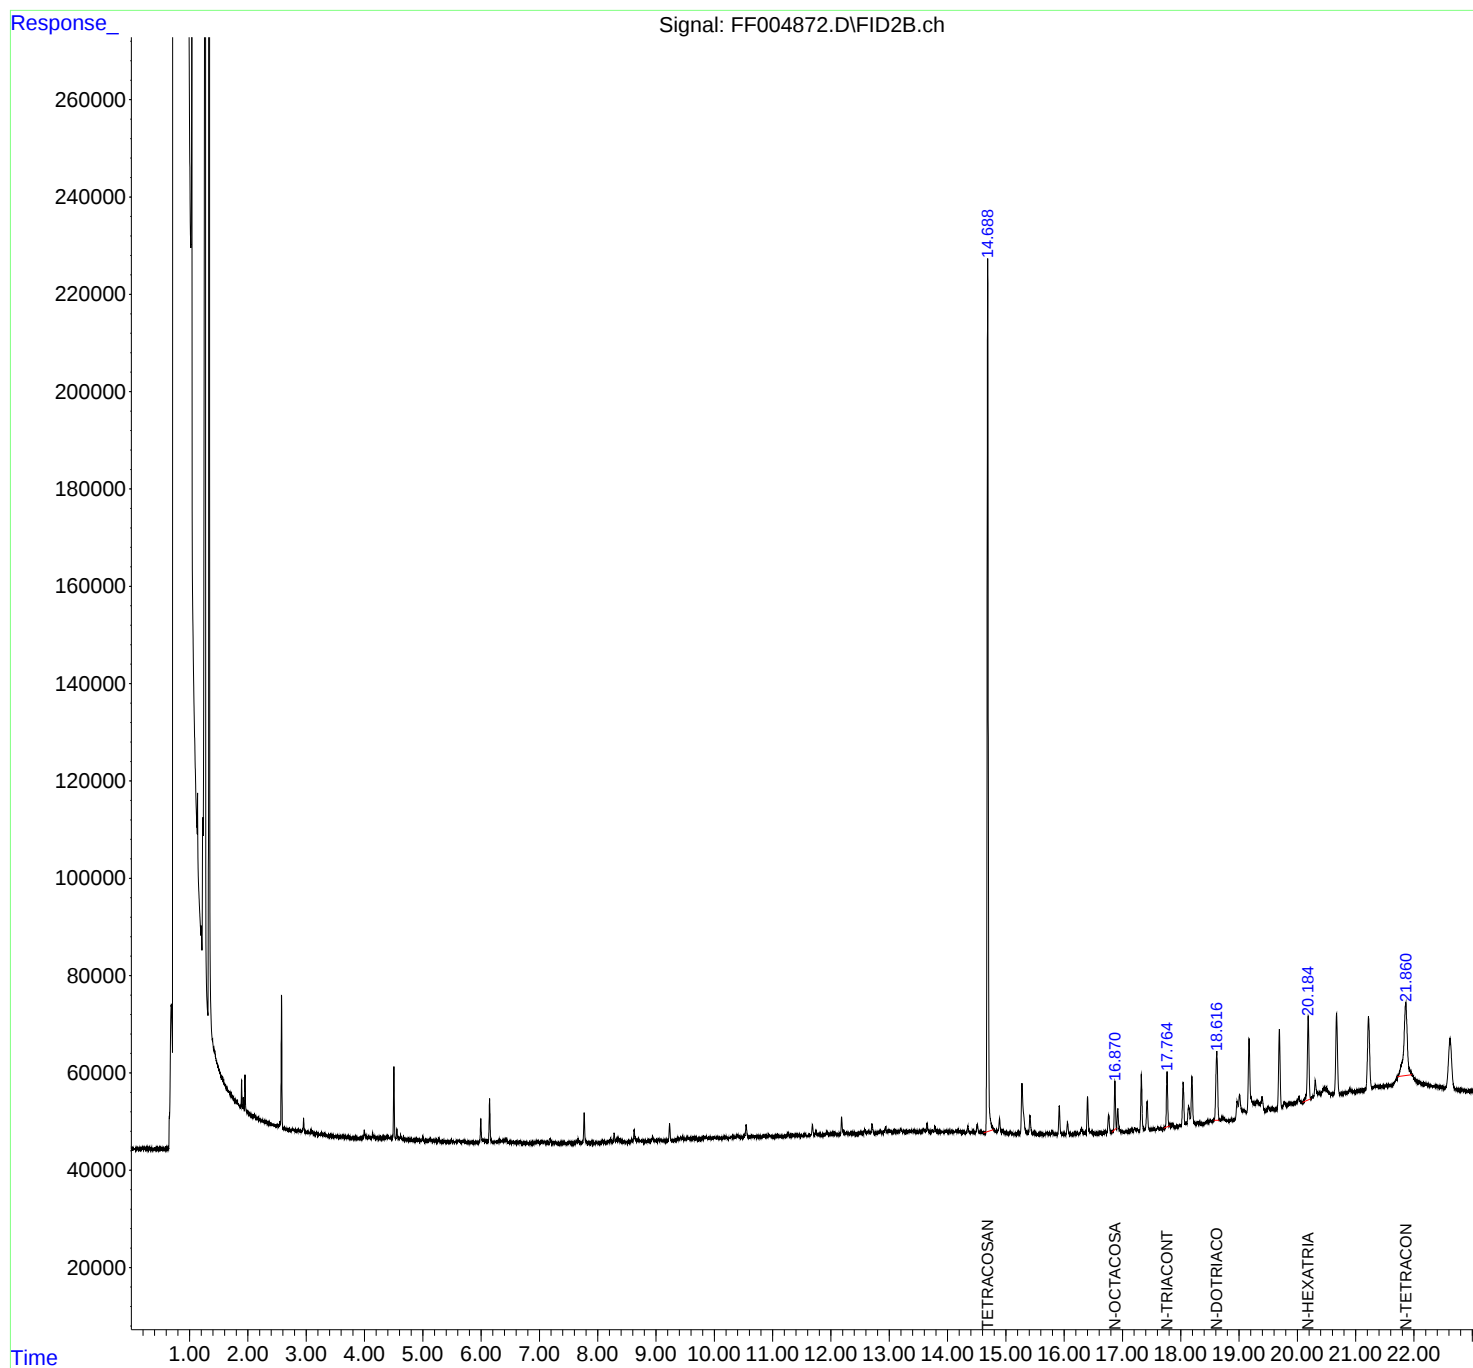


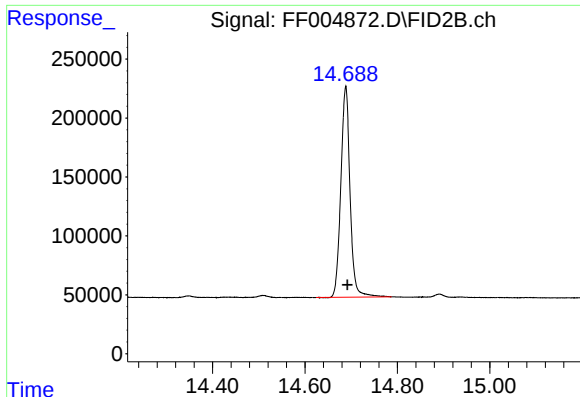

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.688 min
Delta R.T.: -0.003 min
Response: 2474273
Conc: 25.44 ug/ml

Instrument :
FID_F
ClientSampleId :
SIMW-02-20190625

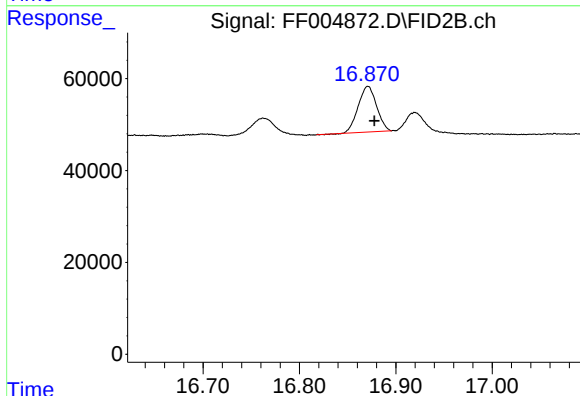


#12 N-OCTACOSANE

R.T.: 16.871 min
Delta R.T.: -0.007 min
Response: 131687
Conc: 1.18 ug/ml

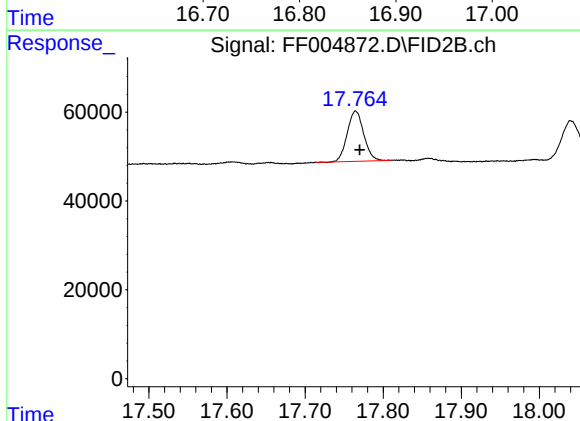


#13 N-TRIACONTANE

R.T.: 17.765 min
Delta R.T.: -0.005 min
Response: 166505
Conc: 1.48 ug/ml

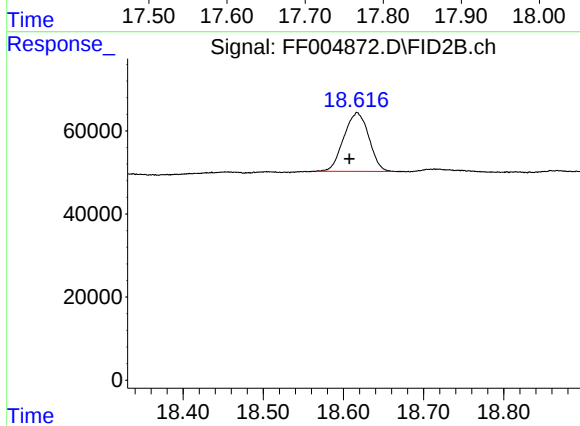

#14 N-DOTRIACONTANE


R.T.: 18.617 min
Delta R.T.: 0.010 min
Response: 306384
Conc: 2.69 ug/ml

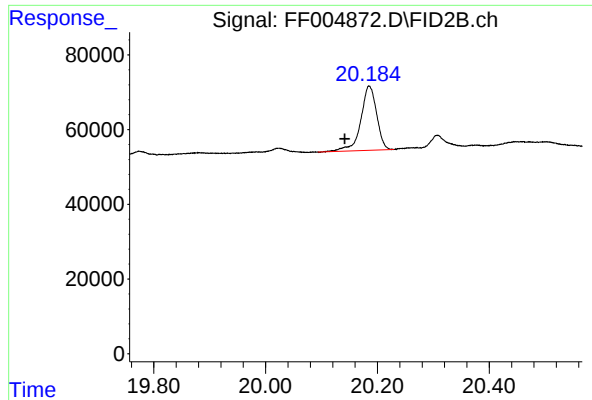

#16 N-HEXATRIACONTANE

R.T.: 20.185 min
Delta R.T.: 0.044 min
Response: 337611
Conc: 3.26 ug/ml

Instrument :
FID_F
ClientSampleId :
SIMW-02-20190625

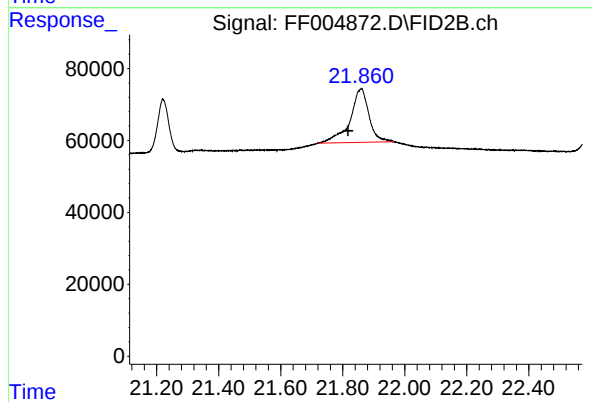

#18 N-TETRACONTANE

R.T.: 21.860 min
Delta R.T.: 0.043 min
Response: 631005
Conc: 5.43 ug/ml