

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062719\
Data File : FF004877.D
Signal(s) : FID2B.ch
Acq On : 27 Jun 2019 18:06
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 28 01:11:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.688	2151215	22.119 ug/ml
Target Compounds				
13)	N-TRIACONTANE	17.766	121354	1.080 ug/ml
14)	N-DOTRIACONTANE	18.608	209759	1.842 ug/ml
16)	N-HEXATRIACONTANE	20.186	174155	1.682 ug/ml
18)	N-TETRACONTANE	21.859	240411	2.068 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062719\
Data File : FF004877.D
Signal(s) : FID2B.ch
Acq On : 27 Jun 2019 18:06
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 28 01:11:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

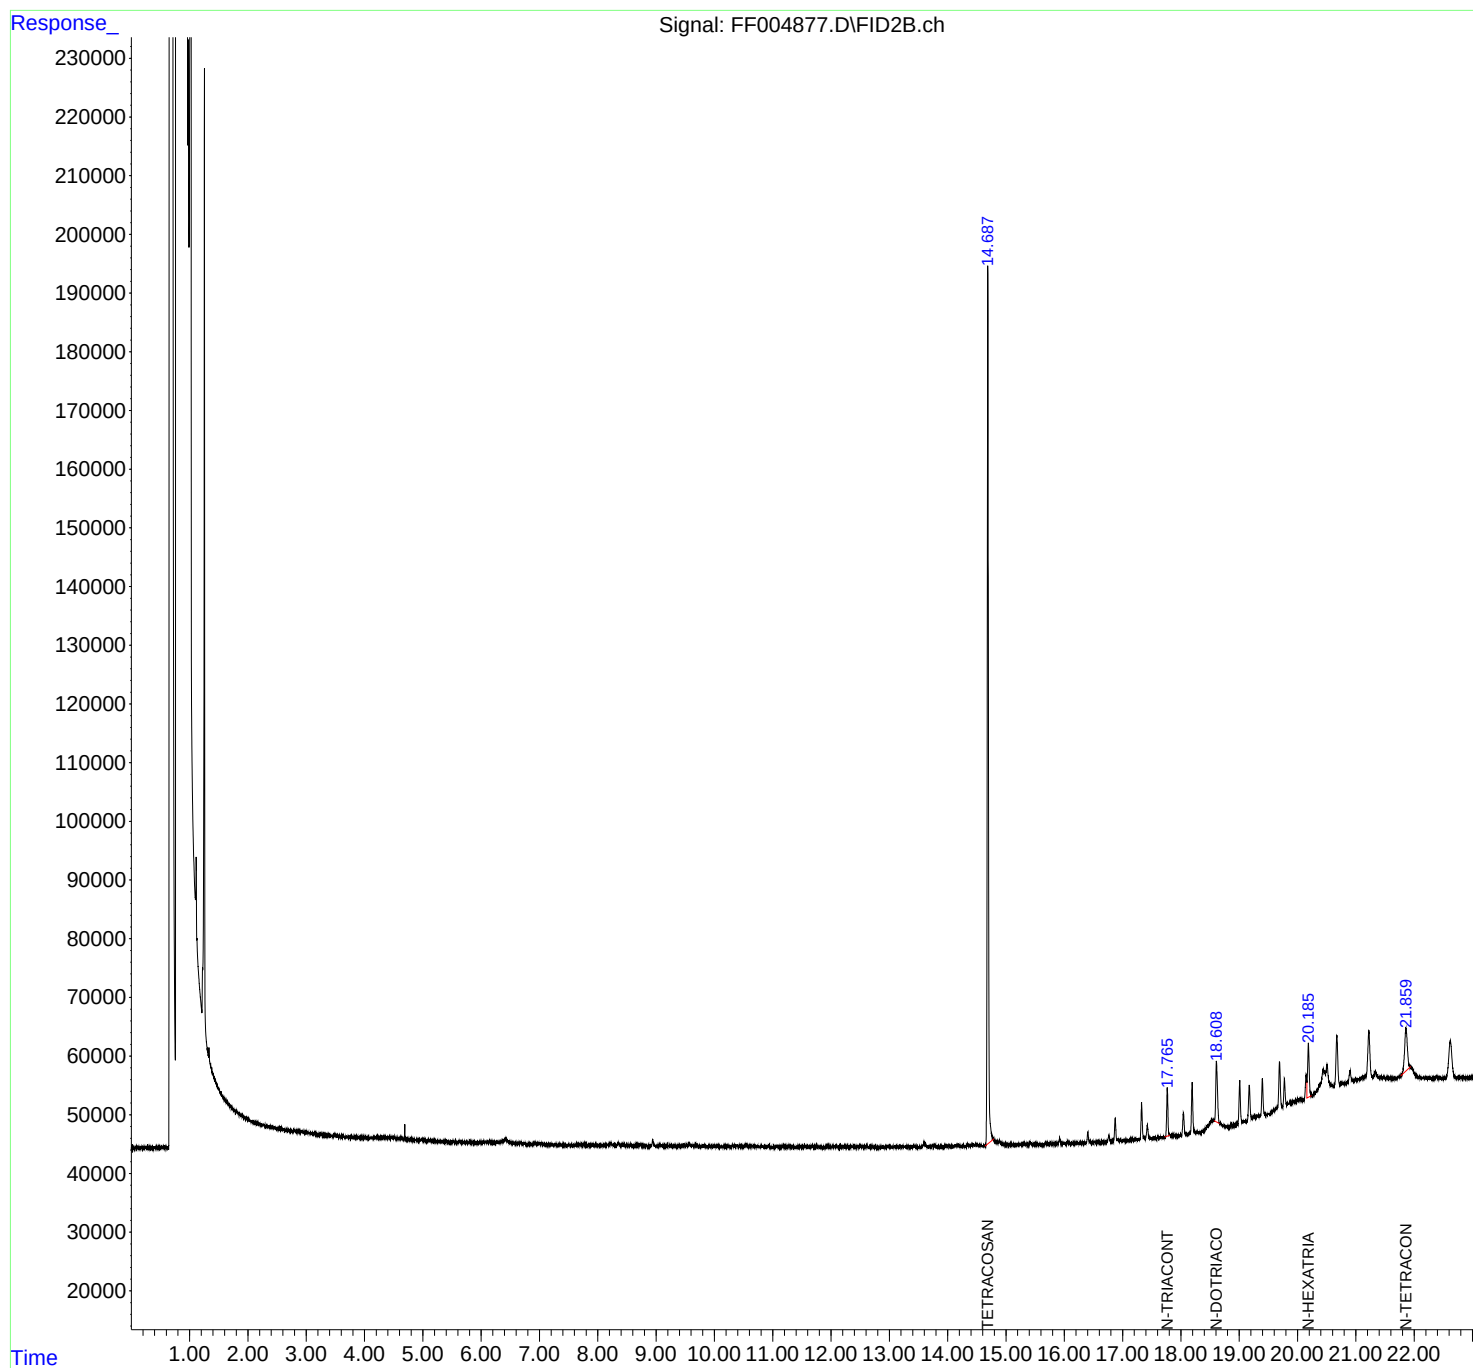


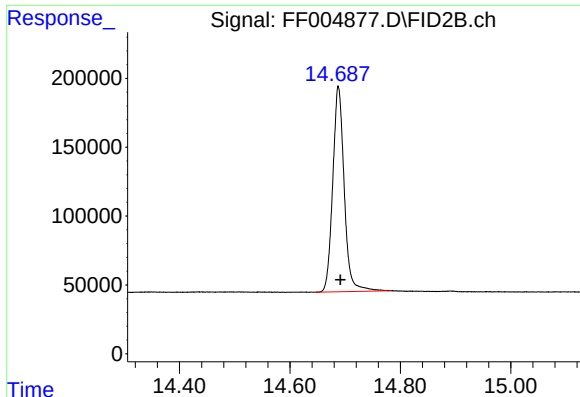

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.688 min
Delta R.T.: -0.004 min
Response: 2151215
Conc: 22.12 ug/ml

Instrument :
FID_F
ClientSampleId :

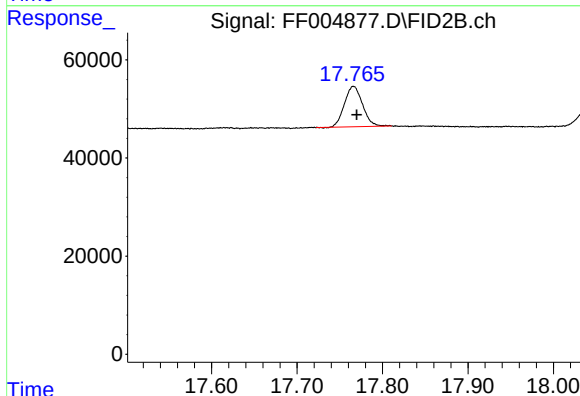


#13 N-TRIACONTANE

R.T.: 17.766 min
Delta R.T.: -0.004 min
Response: 121354
Conc: 1.08 ug/ml

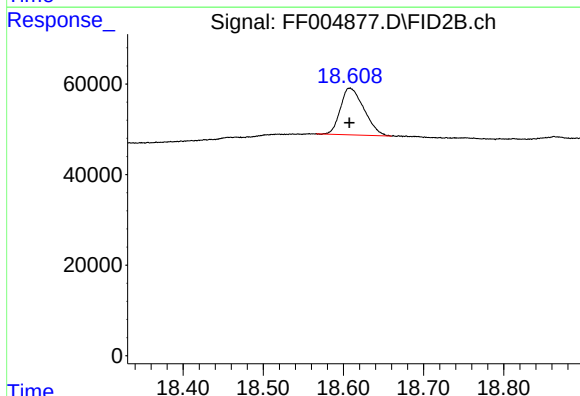


#14 N-DOTRIACONTANE

R.T.: 18.608 min
Delta R.T.: 0.000 min
Response: 209759
Conc: 1.84 ug/ml

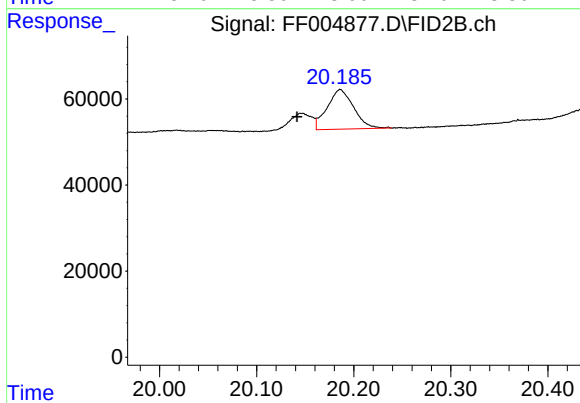

#16 N-HEXATRIACONTANE

R.T.: 20.186 min
Delta R.T.: 0.045 min
Response: 174155
Conc: 1.68 ug/ml

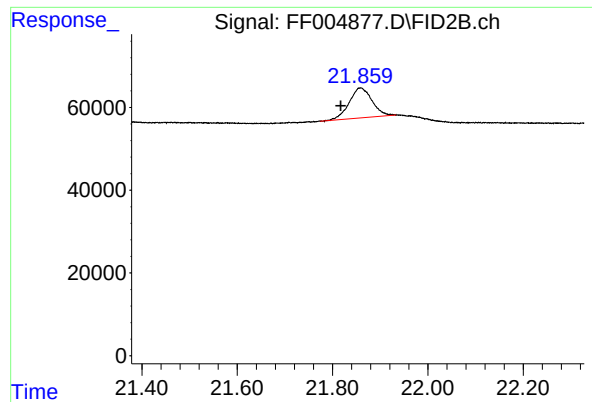

#18 N-TETRACONTANE

R.T.: 21.859 min
Delta R.T.: 0.042 min
Response: 240411
Conc: 2.07 ug/ml

Instrument :
FID_F
ClientSampleId :