

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062722\
 Data File : FF010885.D
 Signal(s) : FID2B.ch
 Acq On : 27 Jun 2022 19:44
 Operator : AJ\MA
 Sample : N3494-04 10X
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 28 01:57:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
 Quant Title :
 QLast Update : Tue Jun 07 09:12:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.824	112257	0.993 ug/ml
Target Compounds			
7) N-EICOSANE	12.768	146642	1.160 ug/ml
8) N-DOCOSANE	13.928	189231	1.498 ug/ml
11) N-HEXACOSANE	16.055	146672	1.158 ug/ml
12) N-OCTACOSANE	17.010	311445	2.552 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062722\
Data File : FF010885.D
Signal(s) : FID2B.ch
Acq On : 27 Jun 2022 19:44
Operator : AJ\MA
Sample : N3494-04 10X
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 28 01:57:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

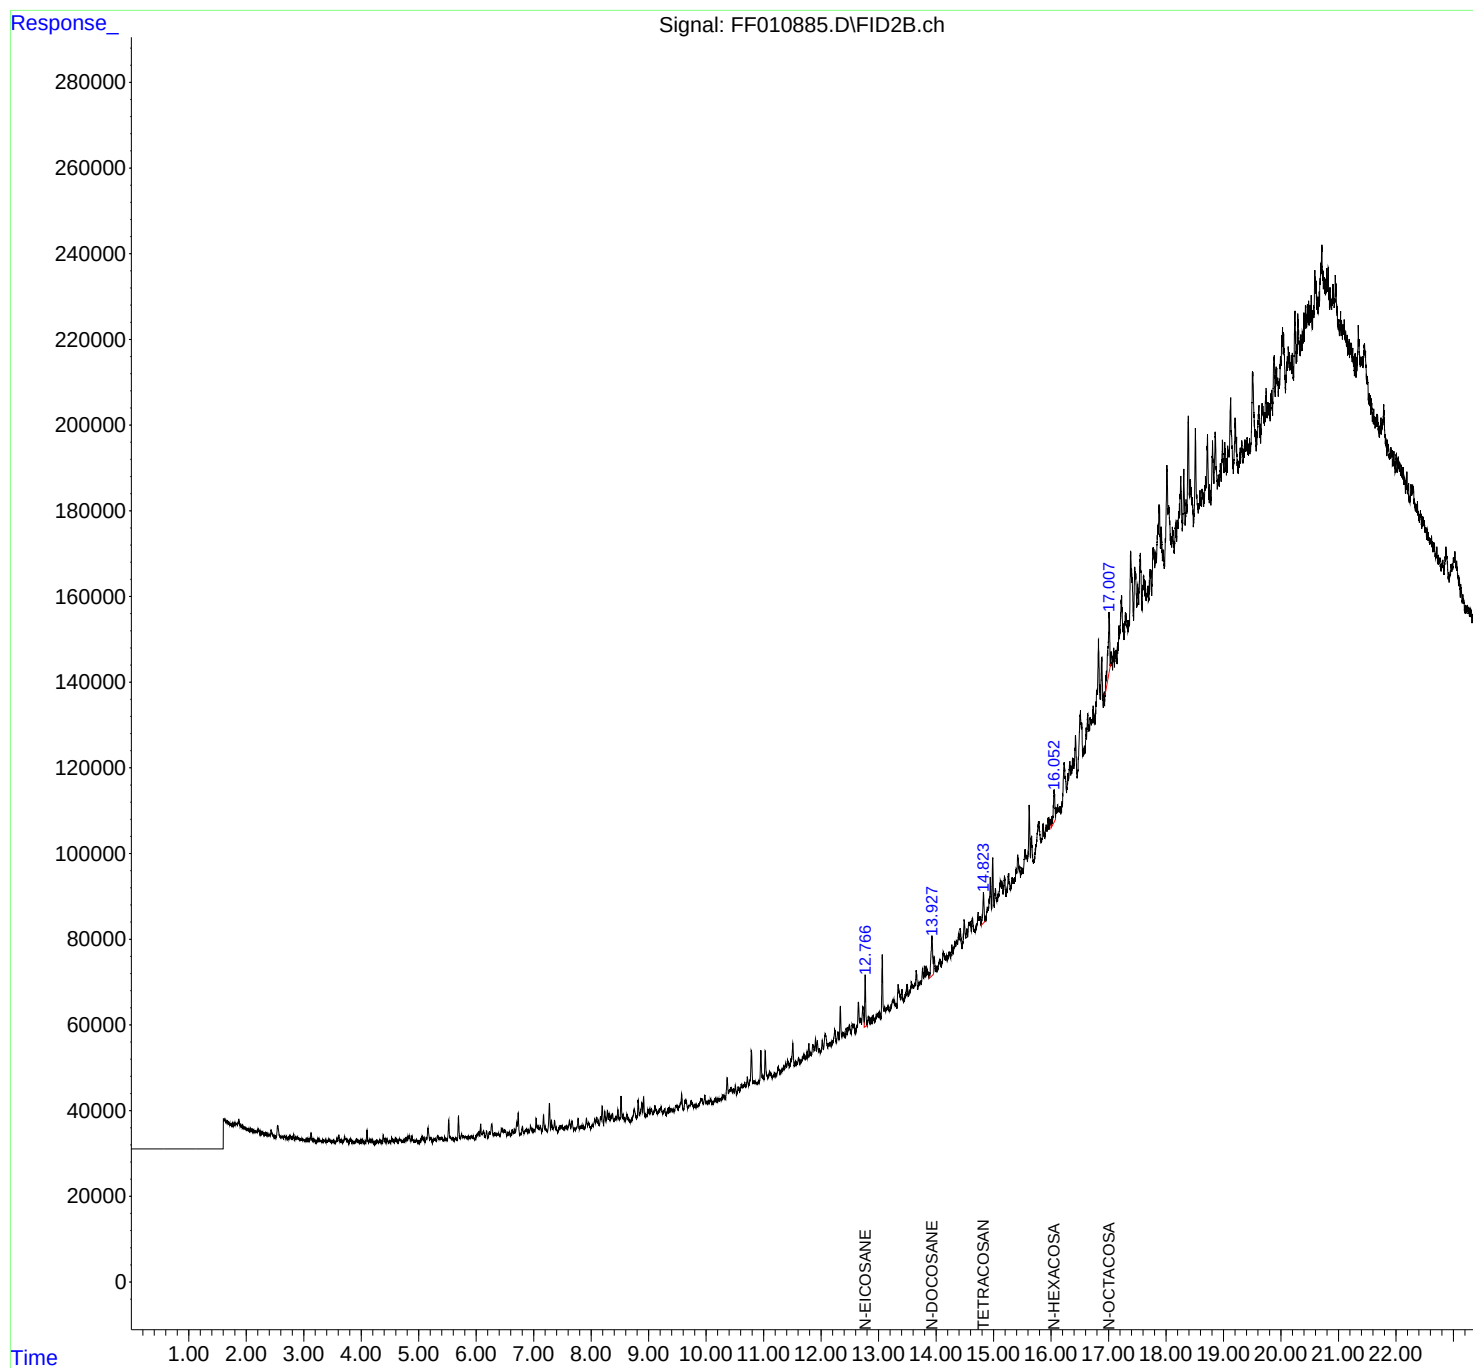


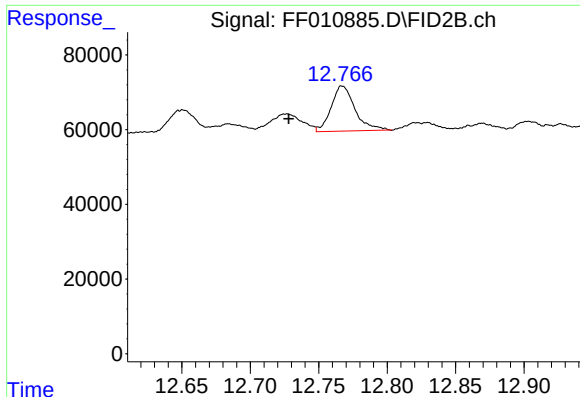

#7 N-EICOSANE


R.T.: 12.768 min
Delta R.T.: 0.039 min
Response: 146642
Conc: 1.16 ug/ml

Instrument :
FID_F
ClientSampleId :

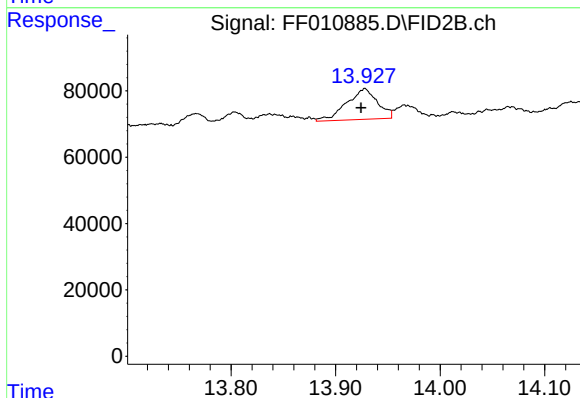


#8 N-DOCOSANE

R.T.: 13.928 min
Delta R.T.: 0.003 min
Response: 189231
Conc: 1.50 ug/ml

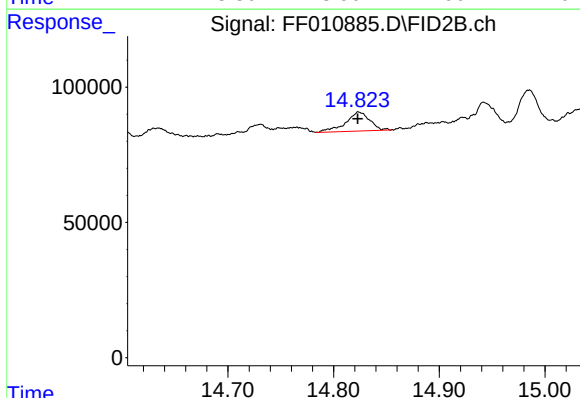


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.824 min
Delta R.T.: 0.002 min
Response: 112257
Conc: 0.99 ug/ml

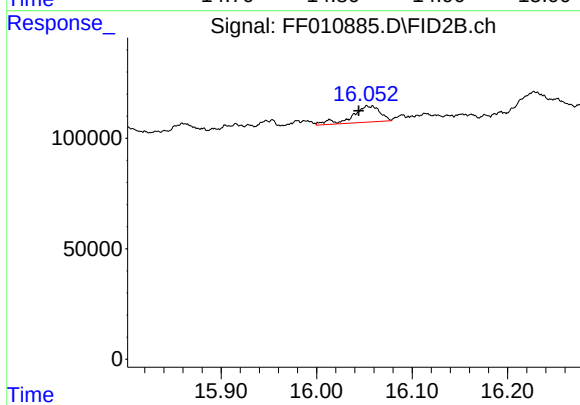

#11 N-HEXACOSANE

R.T.: 16.055 min
Delta R.T.: 0.011 min
Response: 146672
Conc: 1.16 ug/ml

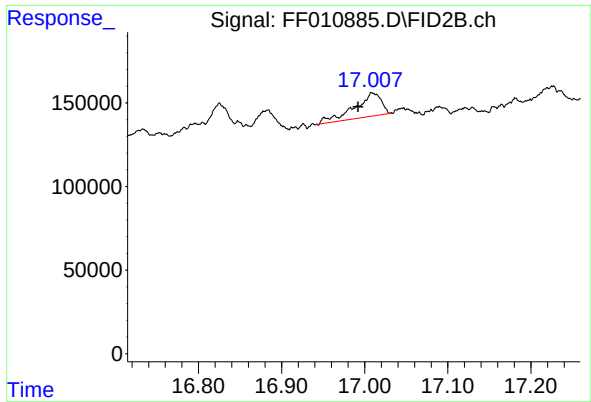

#12 N-OCTACOSANE

R.T.: 17.010 min
Delta R.T.: 0.018 min
Response: 311445
Conc: 2.55 ug/ml

Instrument :
FID_F
ClientSampleId :