

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062722\
 Data File : FF010897.D
 Signal(s) : FID2B.ch
 Acq On : 28 Jun 2022 02:05
 Operator : AJ\MA
 Sample : N3494-34 10X
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 28 02:45:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
 Quant Title :
 QLast Update : Tue Jun 07 09:12:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.827	192666	1.704 ug/ml
Target Compounds			
3) N-DODECANE	6.626f	112467	0.925 ug/ml
7) N-EICOSANE	12.773	201036	1.590 ug/ml
11) N-HEXACOSANE	16.054	74153	0.585 ug/ml
12) N-OCTACOSANE	17.006	93697	0.768 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062722\
Data File : FF010897.D
Signal(s) : FID2B.ch
Acq On : 28 Jun 2022 02:05
Operator : AJ\MA
Sample : N3494-34 10X
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 28 02:45:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

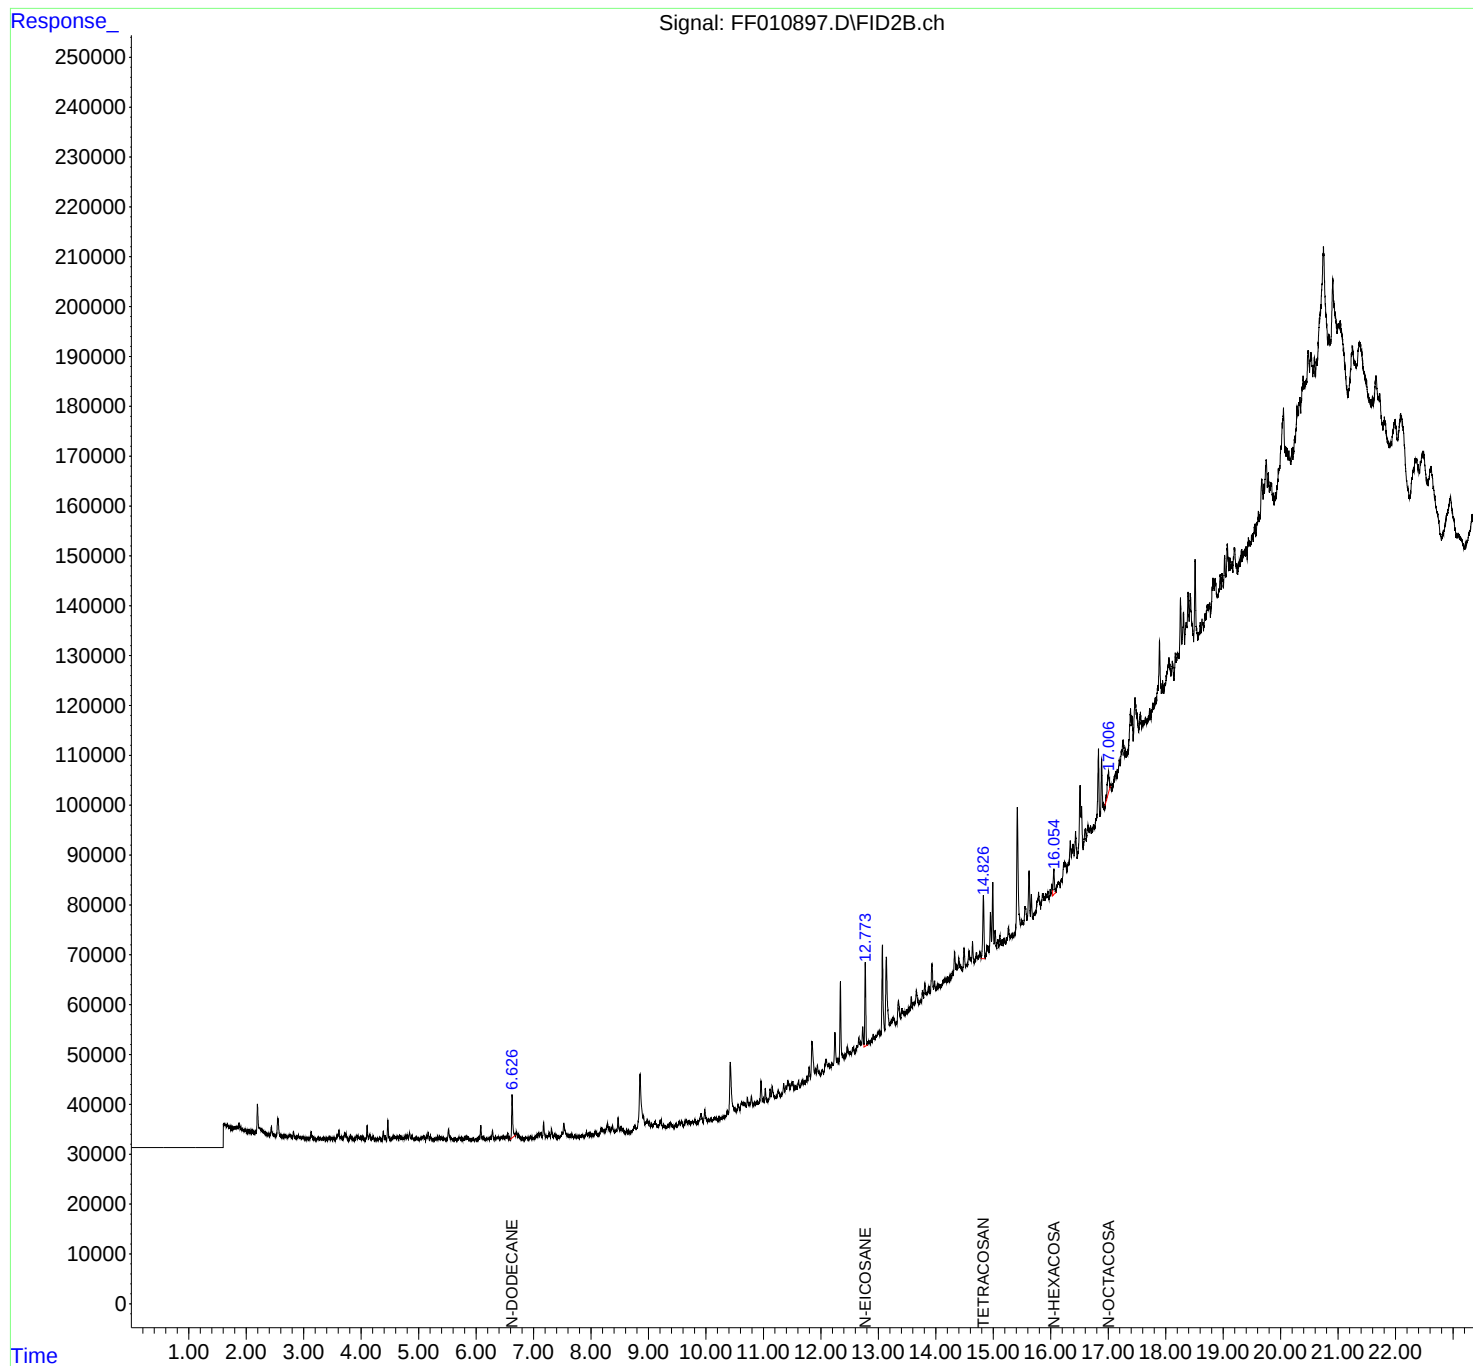


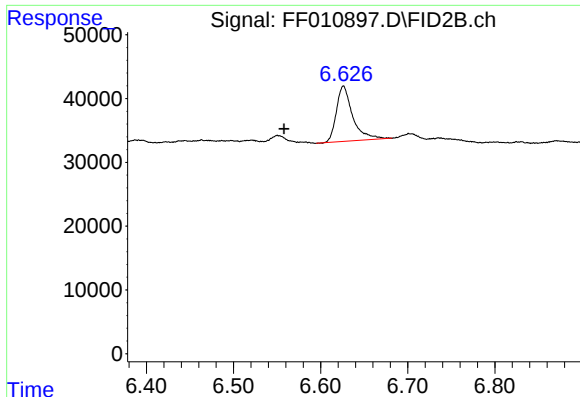

#3 N-DODECANE


R.T.: 6.626 min
Delta R.T.: 0.068 min
Response: 112467
Conc: 0.93 ug/ml

Instrument :
FID_F
ClientSampleId :

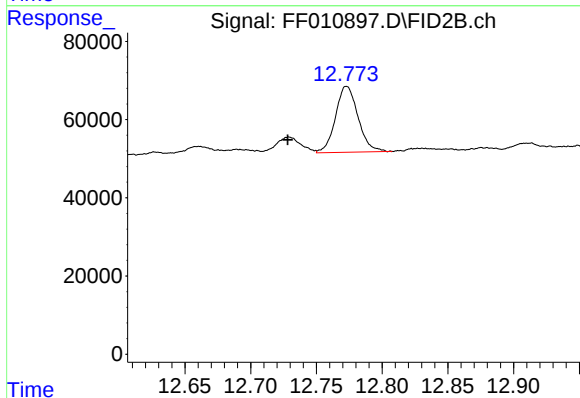


#7 N-EICOSANE

R.T.: 12.773 min
Delta R.T.: 0.045 min
Response: 201036
Conc: 1.59 ug/ml

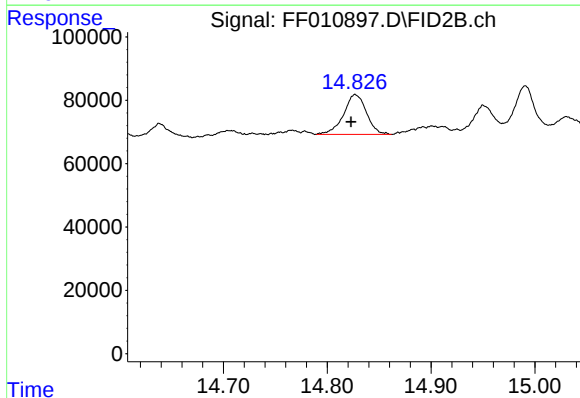


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.827 min
Delta R.T.: 0.005 min
Response: 192666
Conc: 1.70 ug/ml

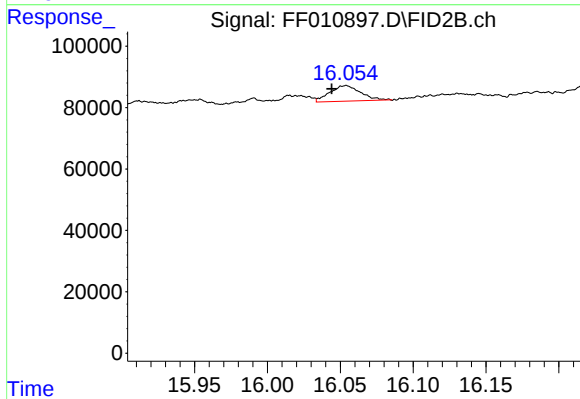

#11 N-HEXACOSANE

R.T.: 16.054 min
Delta R.T.: 0.010 min
Response: 74153
Conc: 0.59 ug/ml

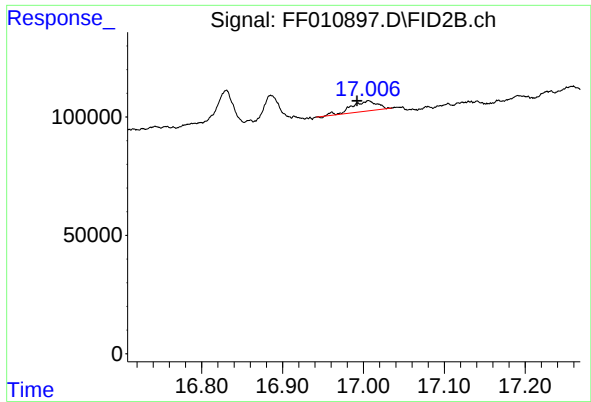

#12 N-OCTACOSANE

R.T.: 17.006 min
Delta R.T.: 0.014 min
Response: 93697
Conc: 0.77 ug/ml

Instrument :

FID_F

ClientSampleId :