

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062722\
 Data File : FF010893.D
 Signal(s) : FID2B.ch
 Acq On : 28 Jun 2022 00:08
 Operator : AJ\MA
 Sample : N3494-24 10X
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SP-EXC-1-3-GR

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/28/2022
 Supervised By :Ankita Jodhani 06/28/2022

Integration File: autoint1.e
 Quant Time: Jun 28 01:59:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
 Quant Title :
 QLast Update : Tue Jun 07 09:12:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.831	155783	1.378 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062722\
Data File : FF010893.D
Signal(s) : FID2B.ch
Acq On : 28 Jun 2022 00:08
Operator : AJ\MA
Sample : N3494-24 10X
Misc :
ALS Vial : 75 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
SP-EXC-1-3-GR


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/28/2022
Supervised By :Ankita Jodhani 06/28/2022

Integration File: autoint1.e
Quant Time: Jun 28 01:59:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

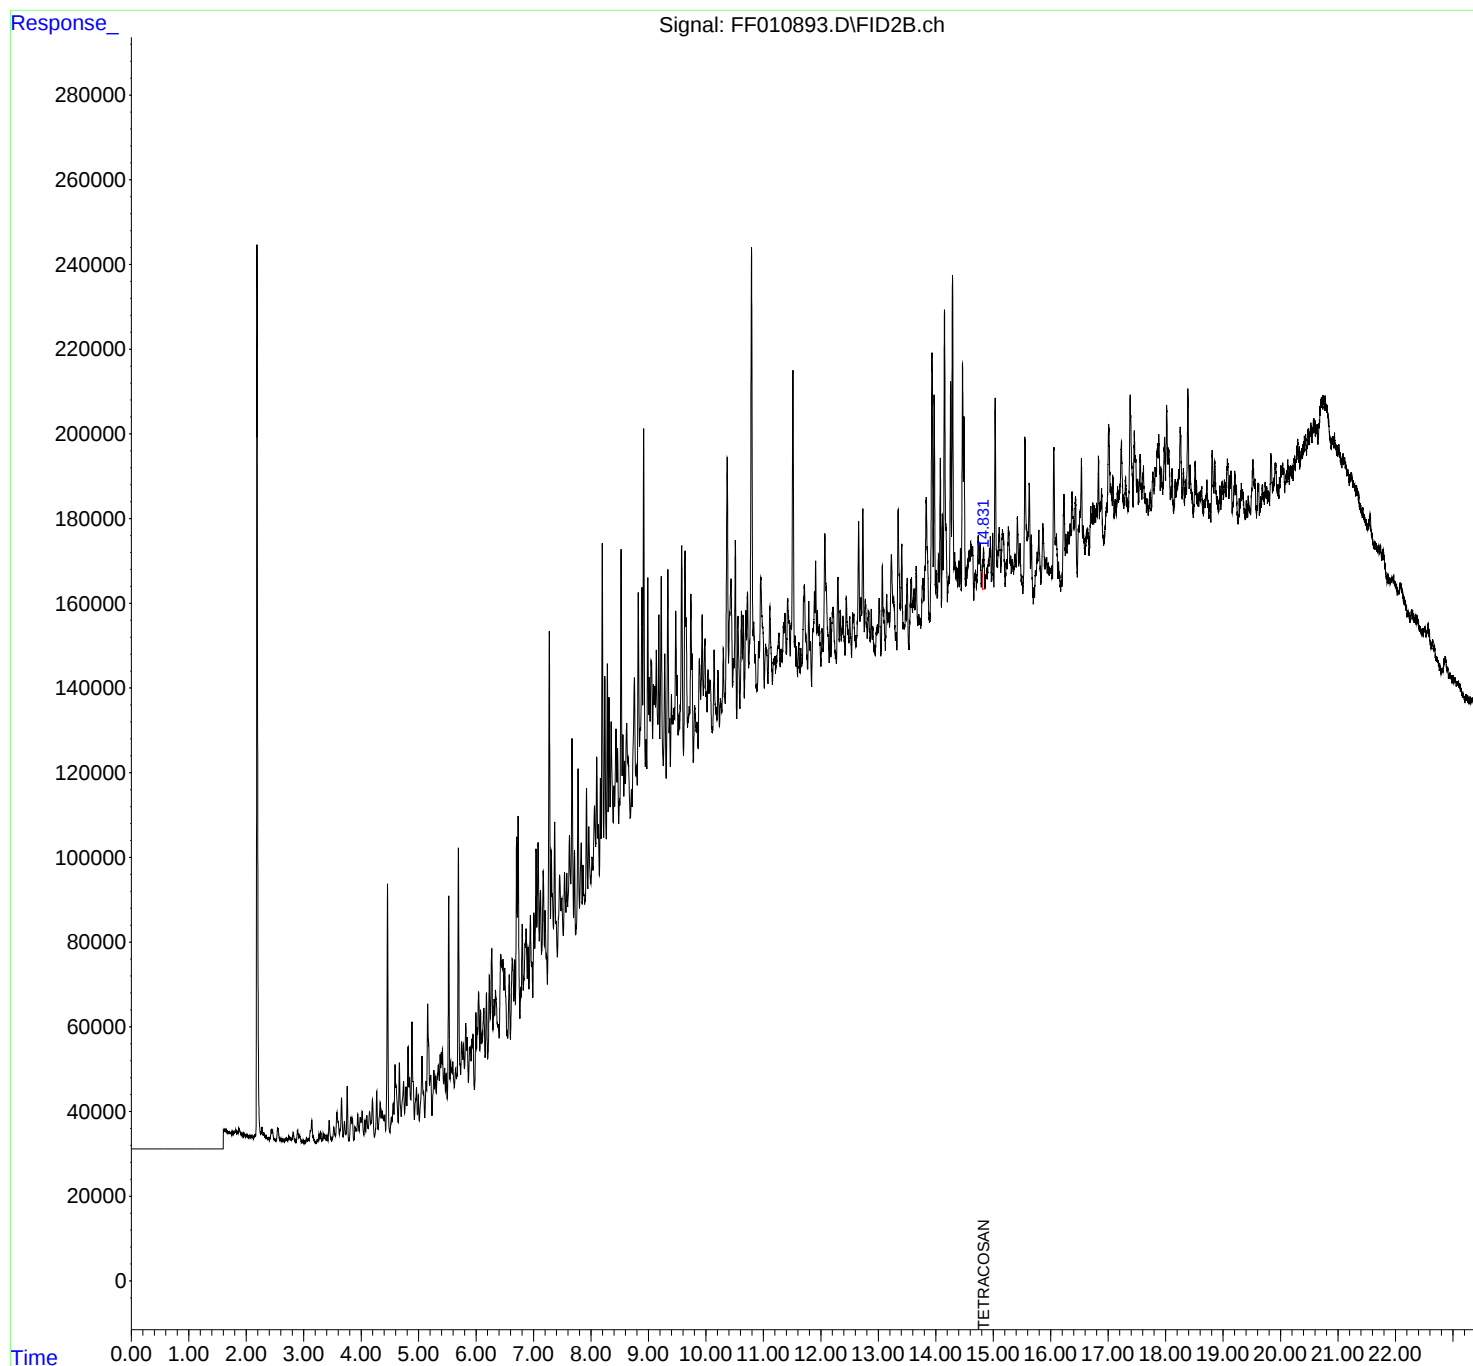

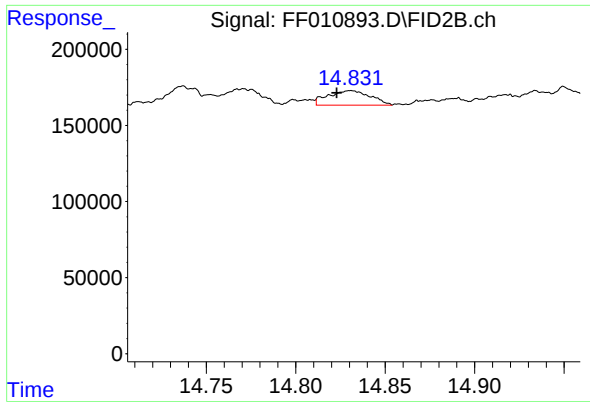

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.831 min
Delta R.T.: 0.008 min
Response: 155783
Conc: 1.38 ug/ml

Instrument :
FID_F
ClientSampleId :
SP-EXC-1-3-GR

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/28/2022
Supervised By :Ankita Jodhani 06/28/2022