

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062722\
Data File : FF010897.D
Signal(s) : FID2B.ch
Acq On : 28 Jun 2022 02:05
Operator : AJ\MA
Sample : N3494-34 10X
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SP-EXC-1-1-GR

Integration File: autoint1.e
Quant Time: Jun 28 02:45:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.827	192666	1.704 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062722\
Data File : FF010897.D
Signal(s) : FID2B.ch
Acq On : 28 Jun 2022 02:05
Operator : AJ\MA
Sample : N3494-34 10X
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SP-EXC-1-1-GR

Integration File: autoint1.e
Quant Time: Jun 28 02:45:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

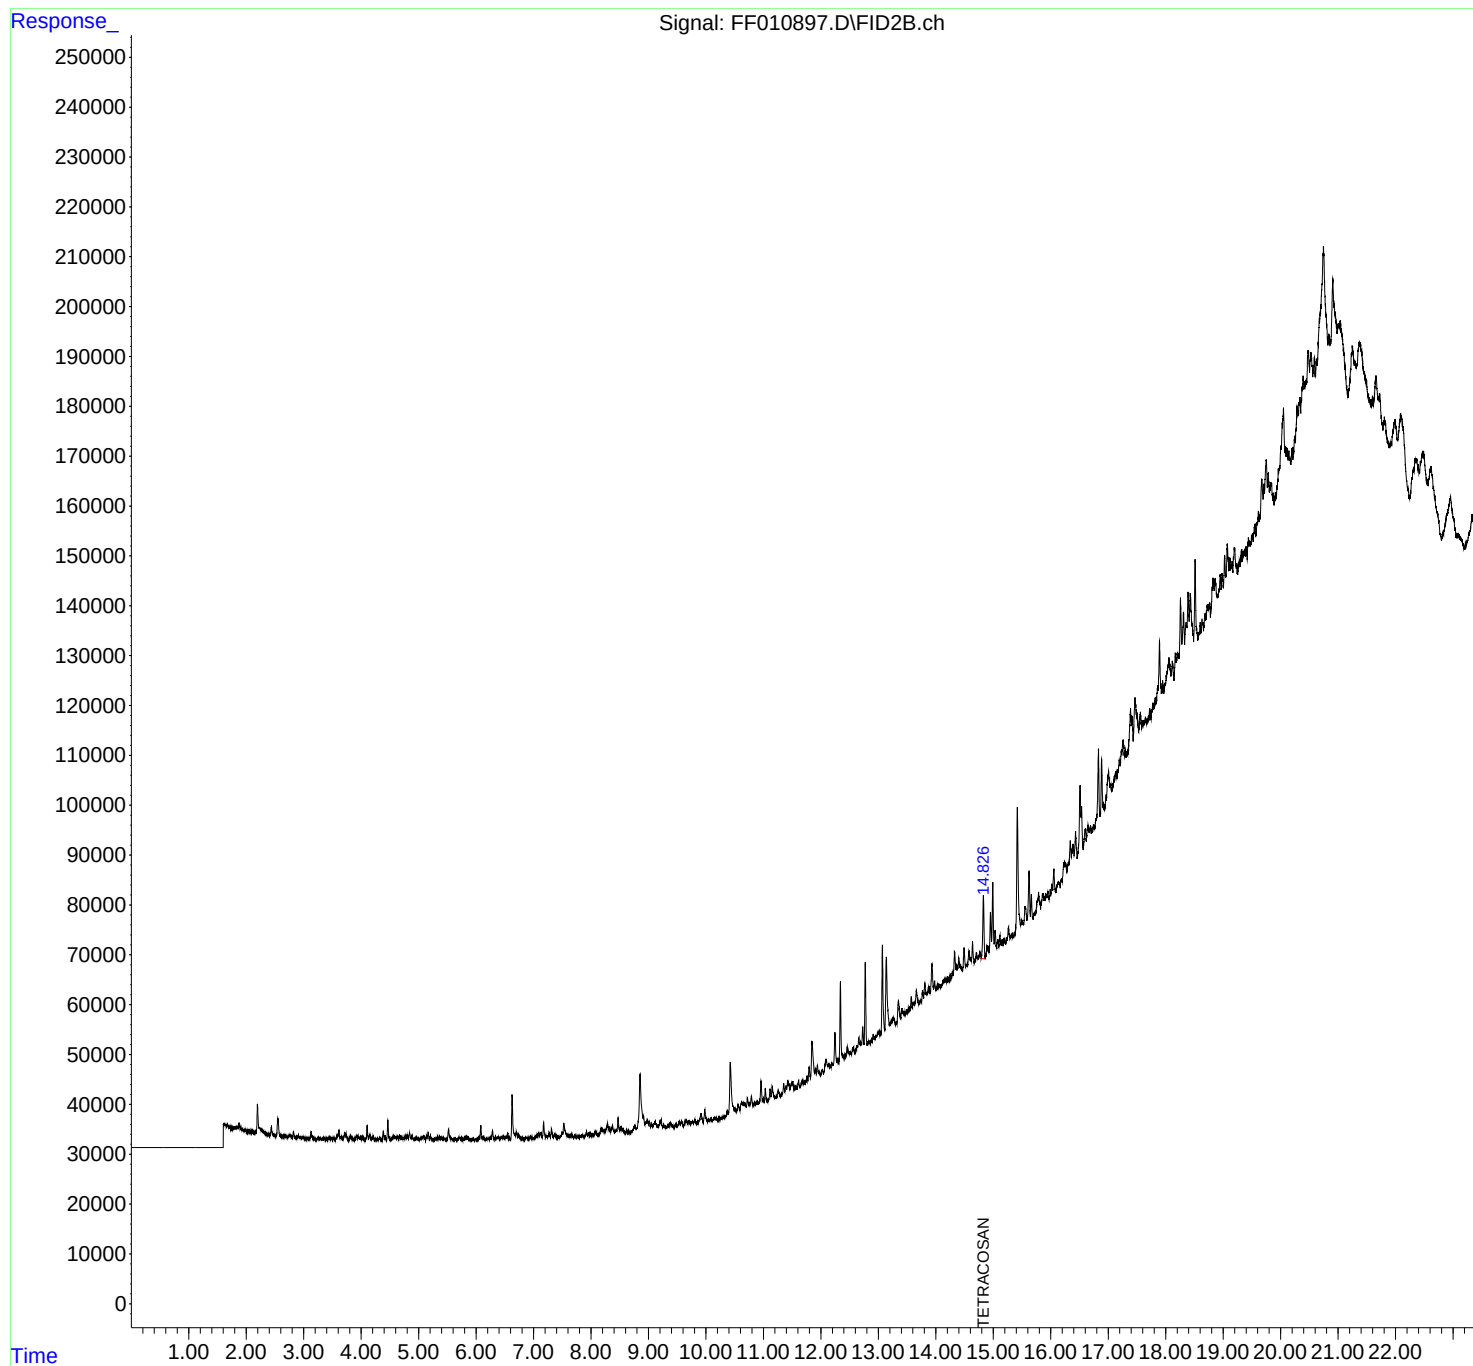

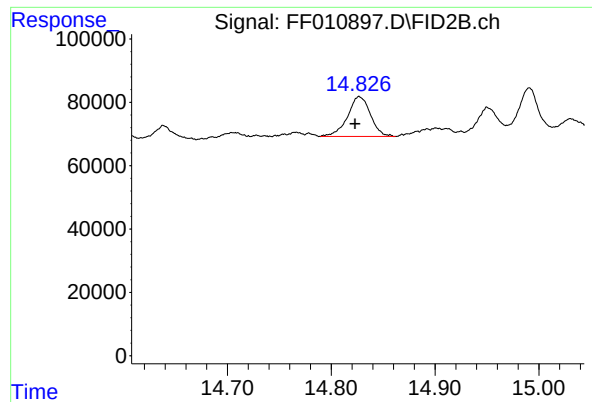

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.827 min
Delta R.T.: 0.005 min
Response: 192666
Conc: 1.70 ug/ml

Instrument :
FID_F
ClientSampleId :
SP-EXC-1-1-GR