

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062723AL\
 Data File : FF013031.D
 Signal(s) : FID2B.ch
 Acq On : 27 Jun 2023 11:41
 Operator : YP\AJ
 Sample : 03357-26DL2 100X
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 27 13:13:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 062023.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 20 13:45:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.306	53061	0.501 ug/ml
Spiked Amount 50.000		Recovery =	1.00%
Target Compounds			
13) T n-Docosane (C22)	13.052	18691	0.153 ug/ml
14) T n-Tetracosane (C24)	14.213f	153821	1.253 ug/ml
15) T n-Hexacosane (C26)	15.206	93983	0.781 ug/ml
16) T n-Octacosane (C28)	16.139	162518	1.382 ug/ml
17) T n-Tricontane (C30)	16.999	87383	0.734 ug/ml
18) T n-Dotriacontane (C32)	17.831	54557	0.467 ug/ml
19) T n-Tetratriacontane (C34)	18.641	120008	1.081 ug/ml
20) T n-Hexatriacontane (C36)	19.361	21329	0.201 ug/ml
21) T n-Octatriacontane (C38)	20.077	205233	1.964 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062723AL\
Data File : FF013031.D
Signal(s) : FID2B.ch
Acq On : 27 Jun 2023 11:41
Operator : YP\AJ
Sample : 03357-26DL2 100X
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 27 13:13:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 062023.M
Quant Title : GC Extractables
QLast Update : Tue Jun 20 13:45:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

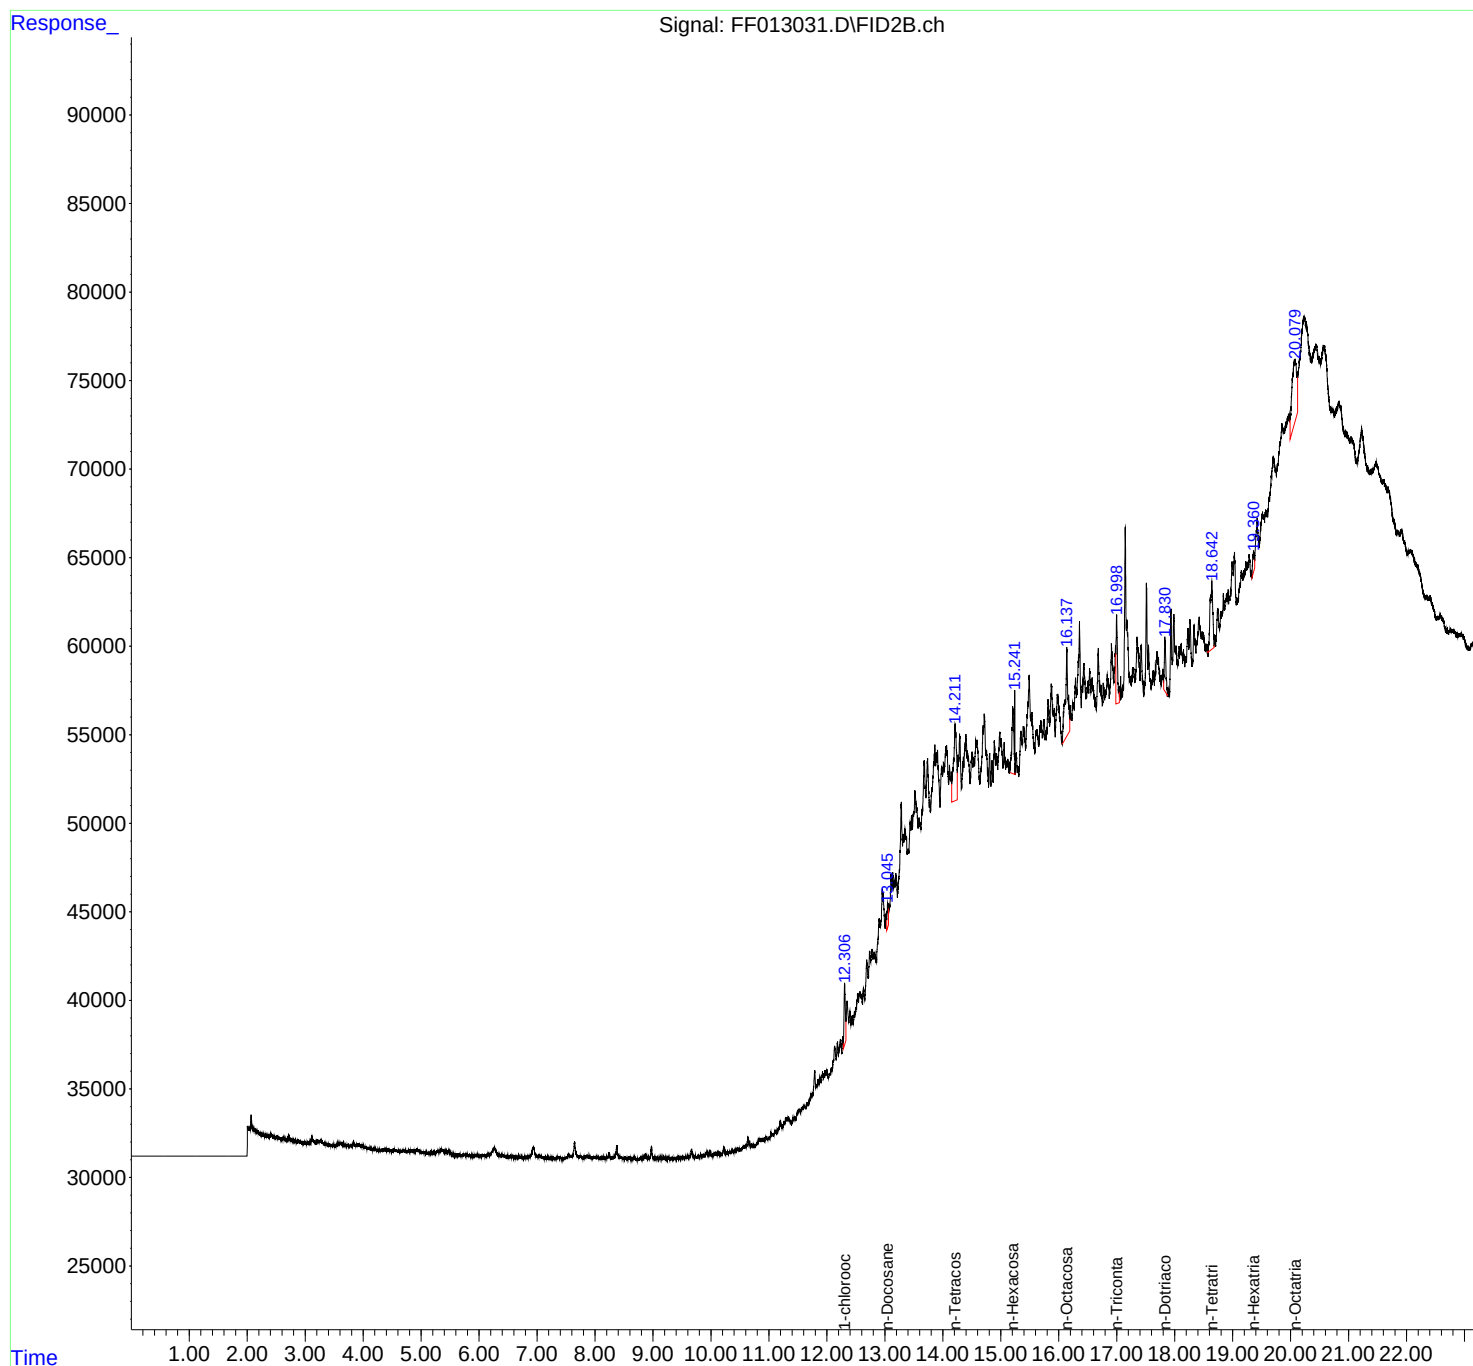


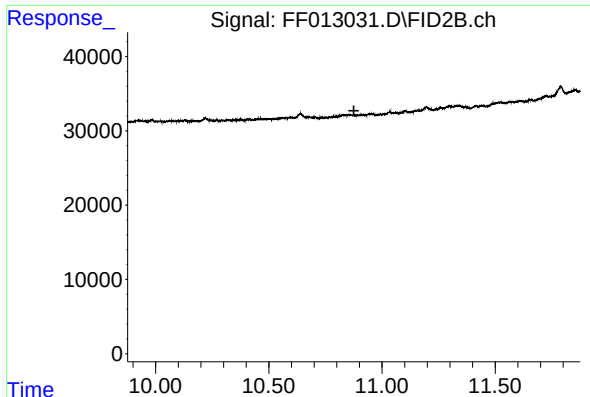

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 10.876 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

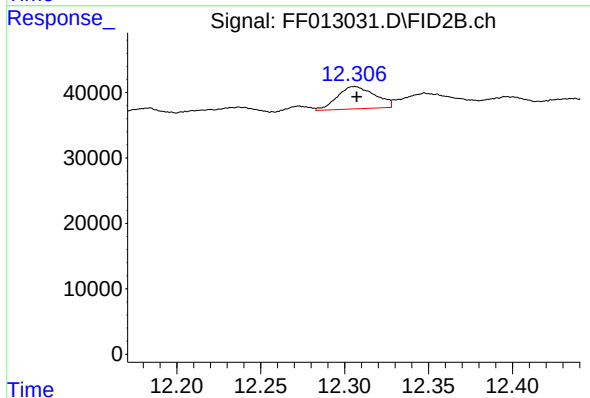


#12 1-chlorooctadecane (SURR)

R.T.: 12.306 min
Delta R.T.: -0.001 min
Response: 53061
Conc: 0.50 ug/ml

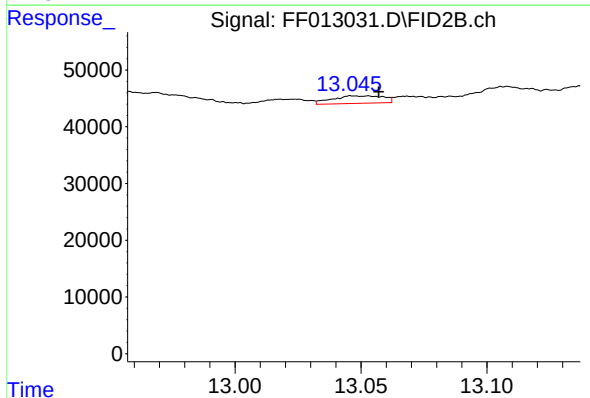


#13 n-Docosane (C22)

R.T.: 13.052 min
Delta R.T.: -0.005 min
Response: 18691
Conc: 0.15 ug/ml

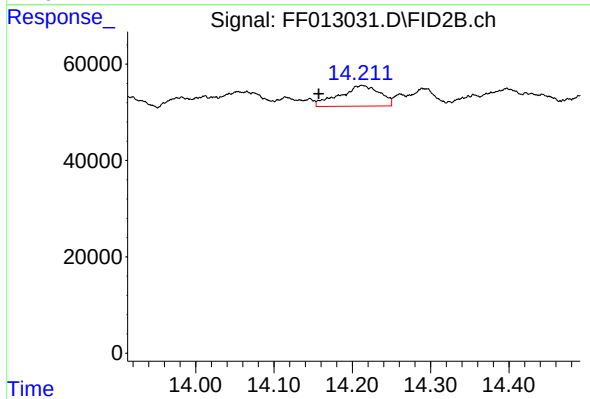

#14 n-Tetracosane (C24)


R.T.: 14.213 min
Delta R.T.: 0.055 min
Response: 153821
Conc: 1.25 ug/ml

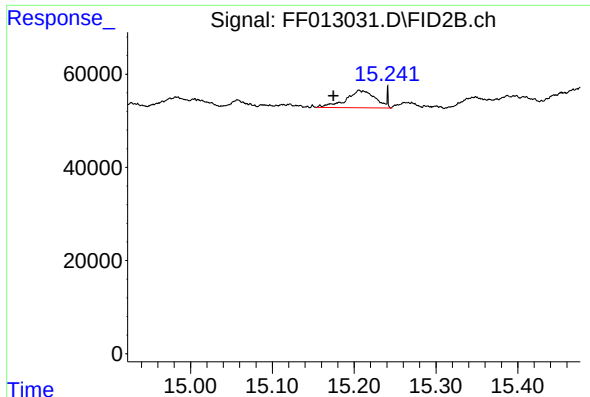

#15 n-Hexacosane (C26)


R.T.: 15.206 min
Delta R.T.: 0.031 min
Response: 93983
Conc: 0.78 ug/ml

Instrument :
FID_F
ClientSampleId :

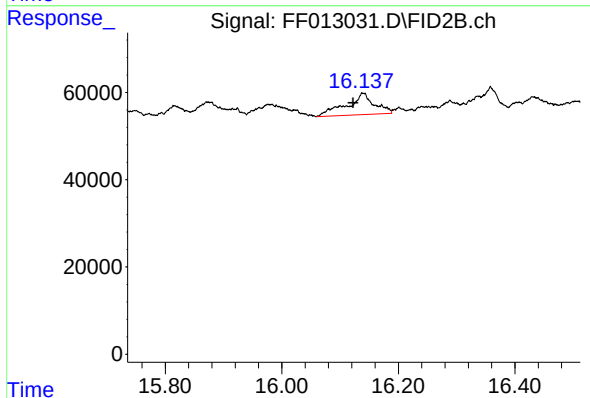


#16 n-Octacosane (C28)

R.T.: 16.139 min
Delta R.T.: 0.017 min
Response: 162518
Conc: 1.38 ug/ml

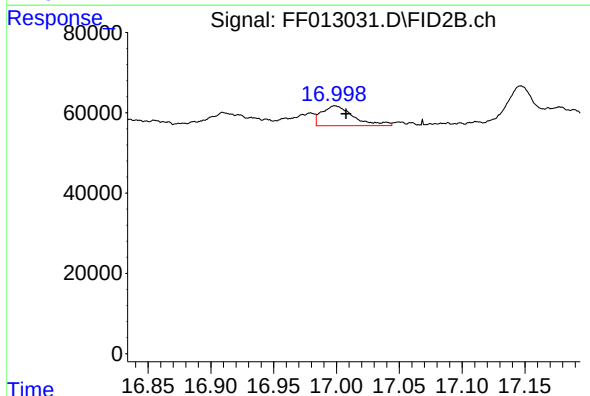


#17 n-Tricontane (C30)

R.T.: 16.999 min
Delta R.T.: -0.009 min
Response: 87383
Conc: 0.73 ug/ml

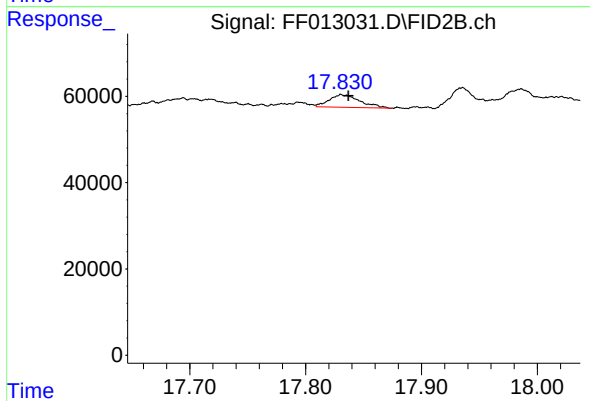

#18 n-Dotriacontane (C32)


R.T.: 17.831 min
Delta R.T.: -0.006 min
Response: 54557
Conc: 0.47 ug/ml

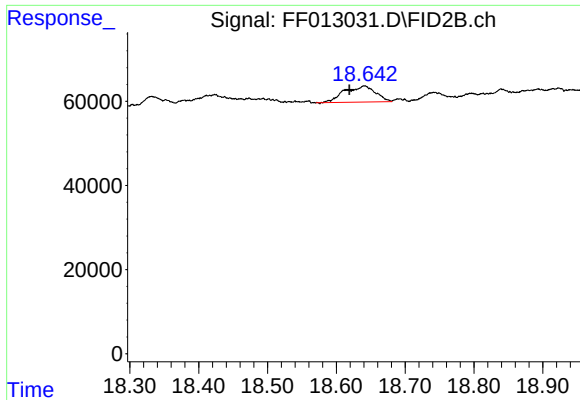

#19 n-Tetratriacontane (C34)


R.T.: 18.641 min
Delta R.T.: 0.022 min
Response: 120008
Conc: 1.08 ug/ml

Instrument :
FID_F
ClientSampleId :

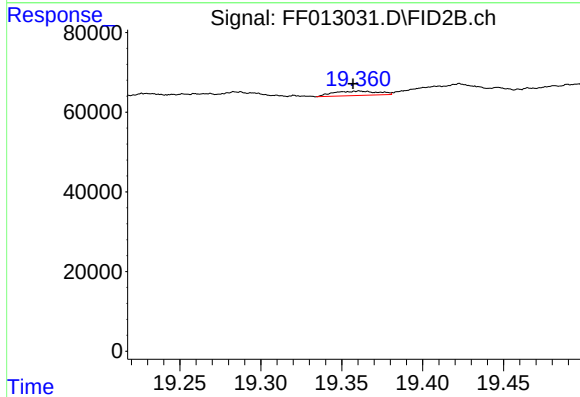

#20 n-Hexatriacontane (C36)

R.T.: 19.361 min
Delta R.T.: 0.004 min
Response: 21329
Conc: 0.20 ug/ml

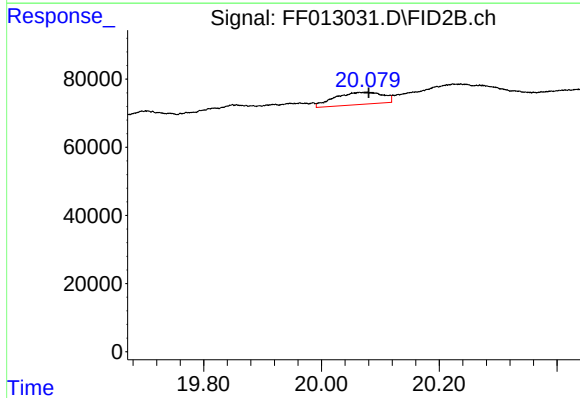

#21 n-Octatriacontane (C38)

R.T.: 20.077 min
Delta R.T.: -0.003 min
Response: 205233
Conc: 1.96 ug/ml