

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062723AL\
 Data File : FF013036.D
 Signal(s) : FID2B.ch
 Acq On : 27 Jun 2023 14:08
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 28 00:22:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 062023.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 20 13:45:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
17) T n-Tricontane (C30)	17.006	37261	0.313 ug/ml
18) T n-Dotriacontane (C32)	17.835	224311	1.918 ug/ml
19) T n-Tetratriacontane (C34)	18.615	177720	1.601 ug/ml
20) T n-Hexatriacontane (C36)	19.353	141154	1.332 ug/ml
21) T n-Octatriacontane (C38)	20.077	172225	1.648 ug/ml
22) T n-Tetracontane (C40)	20.965	140315	1.448 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062723AL\
Data File : FF013036.D
Signal(s) : FID2B.ch
Acq On : 27 Jun 2023 14:08
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 28 00:22:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 062023.M
Quant Title : GC Extractables
QLast Update : Tue Jun 20 13:45:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

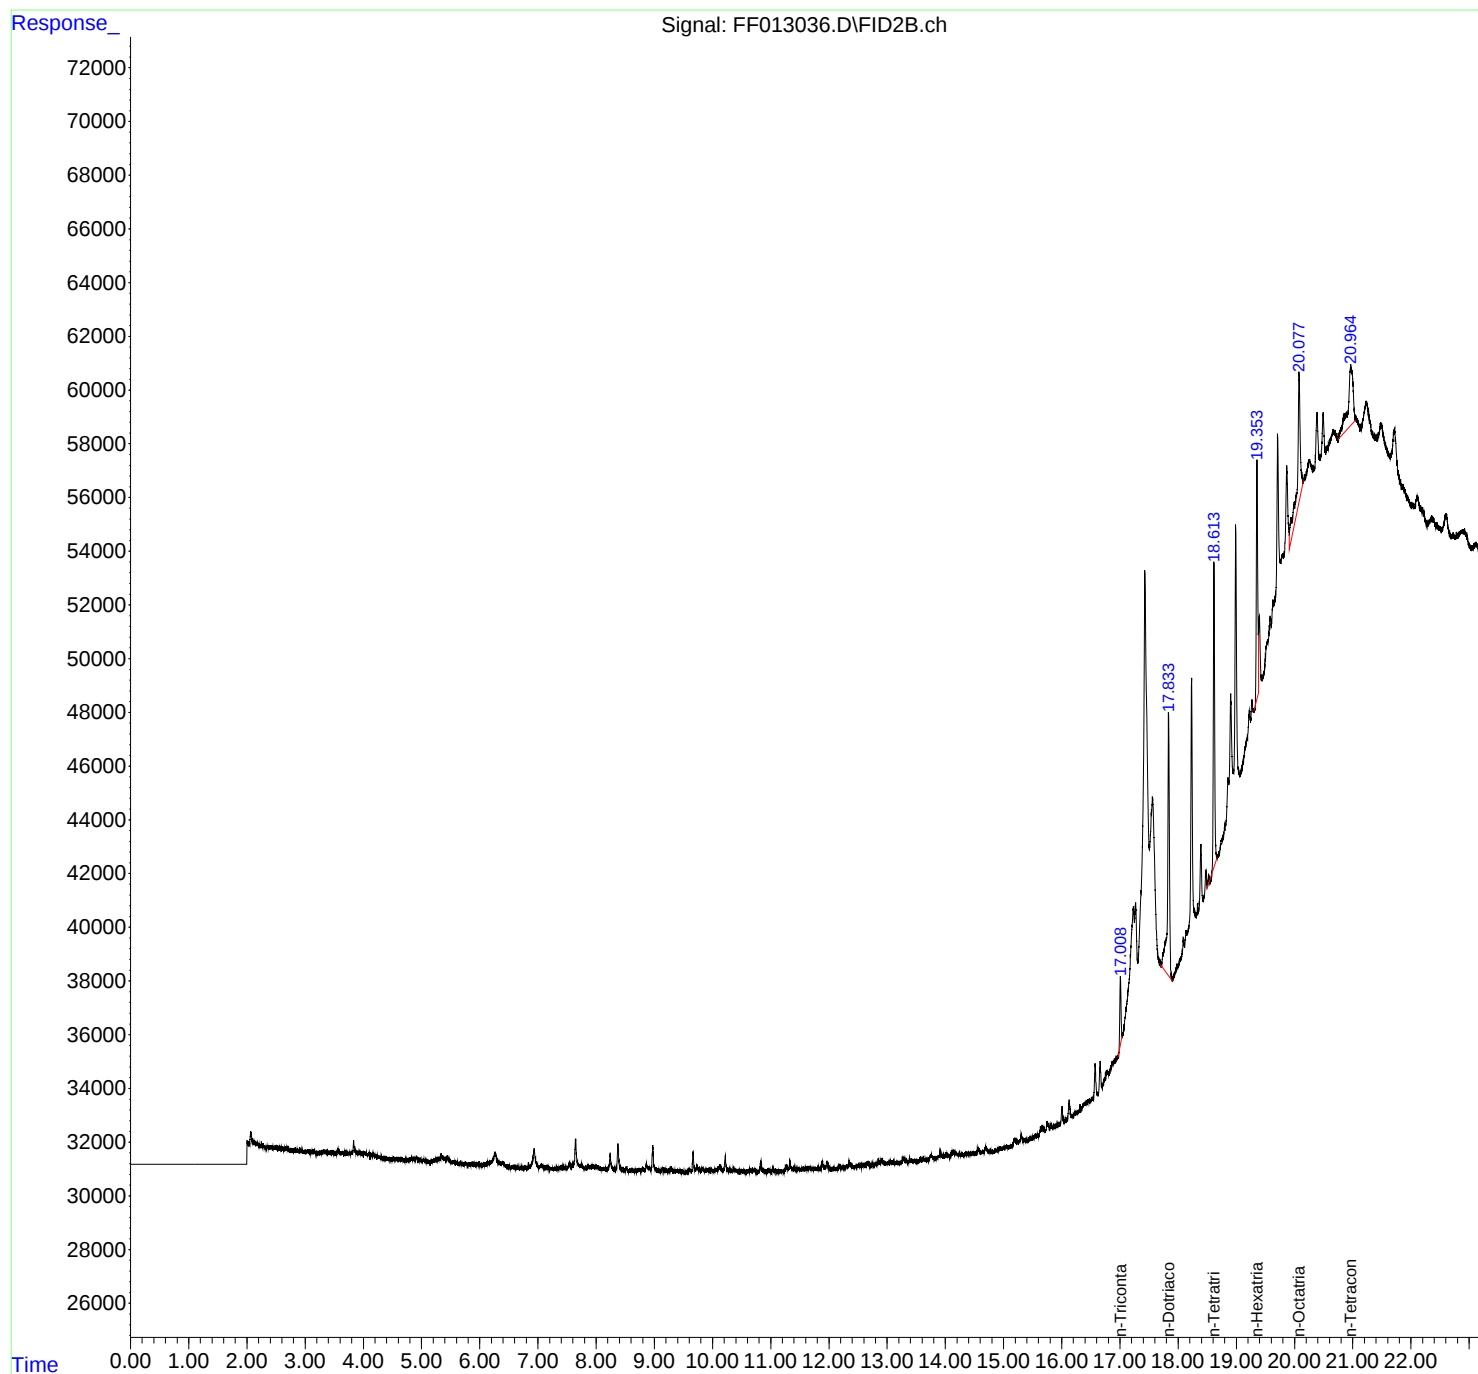


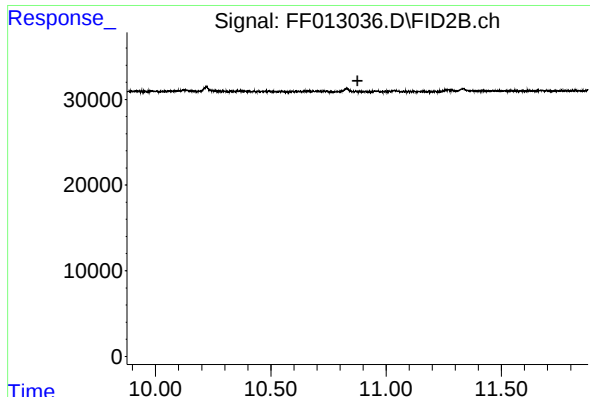

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 10.876 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

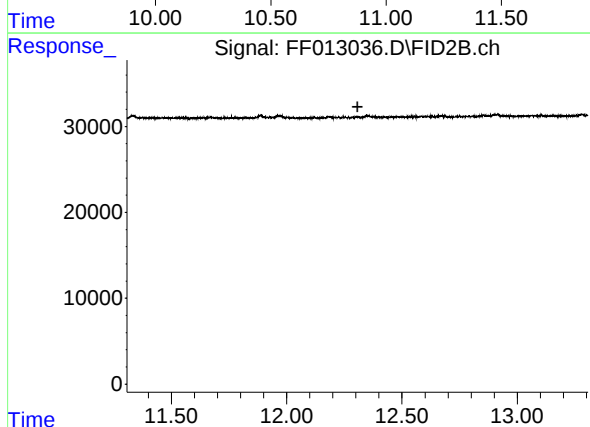


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 12.307 min
Response: 0
Conc: N.D.

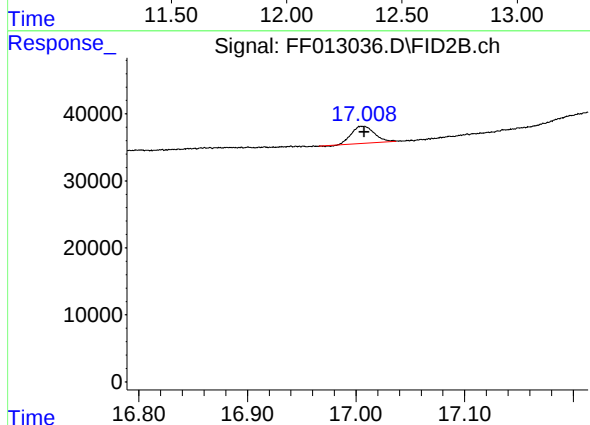


#17 n-Tricontane (C30)

R.T.: 17.006 min
Delta R.T.: -0.001 min
Response: 37261
Conc: 0.31 ug/ml

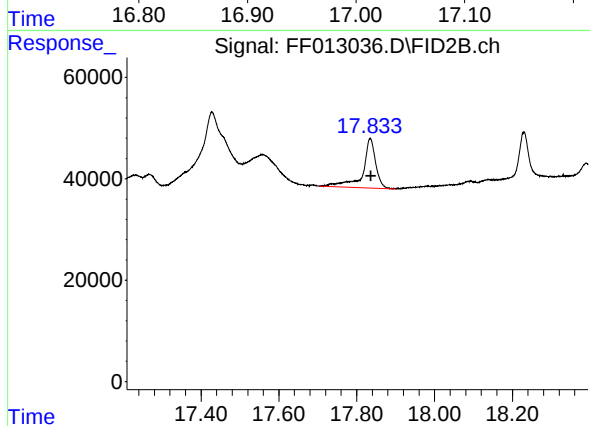

#18 n-Dotriacontane (C32)


R.T.: 17.835 min
Delta R.T.: -0.002 min
Response: 224311
Conc: 1.92 ug/ml

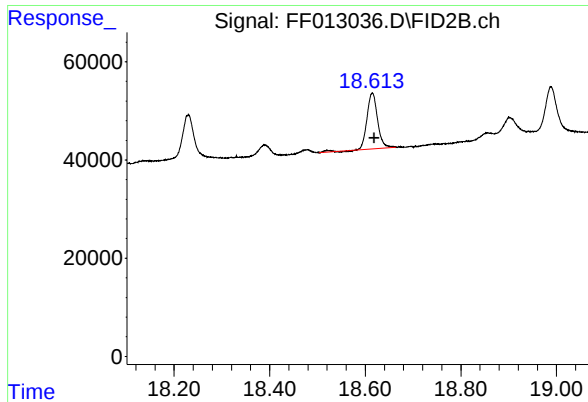

#19 n-Tetratriacontane (C34)


R.T.: 18.615 min
Delta R.T.: -0.005 min
Response: 177720
Conc: 1.60 ug/ml

Instrument :
FID_F
ClientSampleId :

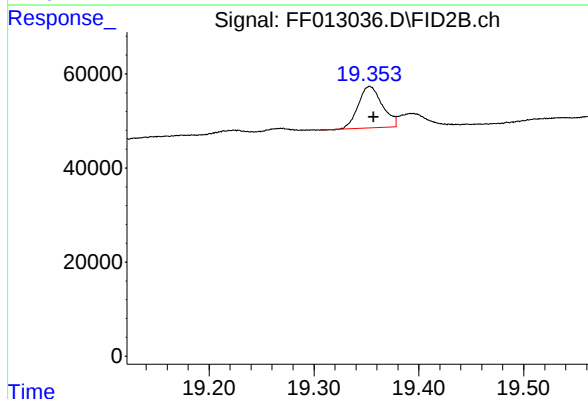


#20 n-Hexatriacontane (C36)

R.T.: 19.353 min
Delta R.T.: -0.004 min
Response: 141154
Conc: 1.33 ug/ml

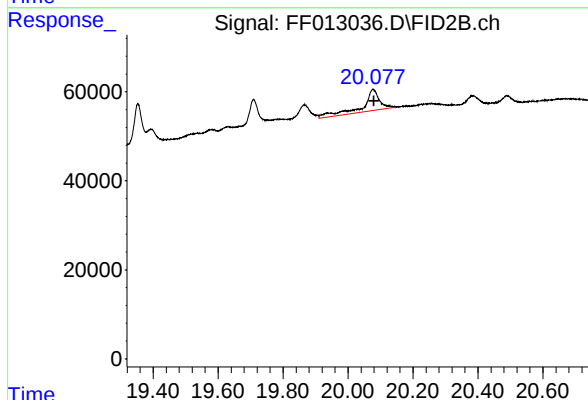

#21 n-Octatriacontane (C38)

R.T.: 20.077 min
Delta R.T.: -0.003 min
Response: 172225
Conc: 1.65 ug/ml

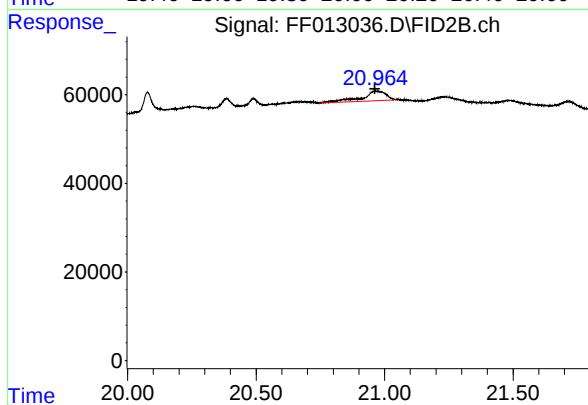

#22 n-Tetracontane (C40)

R.T.: 20.965 min
Delta R.T.: 0.002 min
Response: 140315
Conc: 1.45 ug/ml