

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062818\
 Data File : FF001138.D
 Signal(s) : FID2B.ch
 Acq On : 28 Jun 2018 16:59
 Operator : UA\AJ
 Sample : J3711-01
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 29 01:22:39 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.472	2197761	19.057 ug/ml
Target Compounds			
2) N-DECANE	4.222	1854528	13.236 ug/ml
3) N-DODECANE	6.240	2812901	20.070 ug/ml
4) N-TETRADECANE	8.033	6917650	49.685 ug/ml
5) N-HEXADECANE	9.645	21827268	158.309 ug/ml
6) N-OCTADECANE	11.088	9926994	72.697 ug/ml
7) N-EICOSANE	12.372	3089898	23.063 ug/ml
10) N-TETRACOSANE	14.709	536274	4.134 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062818\
Data File : FF001138.D
Signal(s) : FID2B.ch
Acq On : 28 Jun 2018 16:59
Operator : UA\AJ
Sample : J3711-01
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 29 01:22:39 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

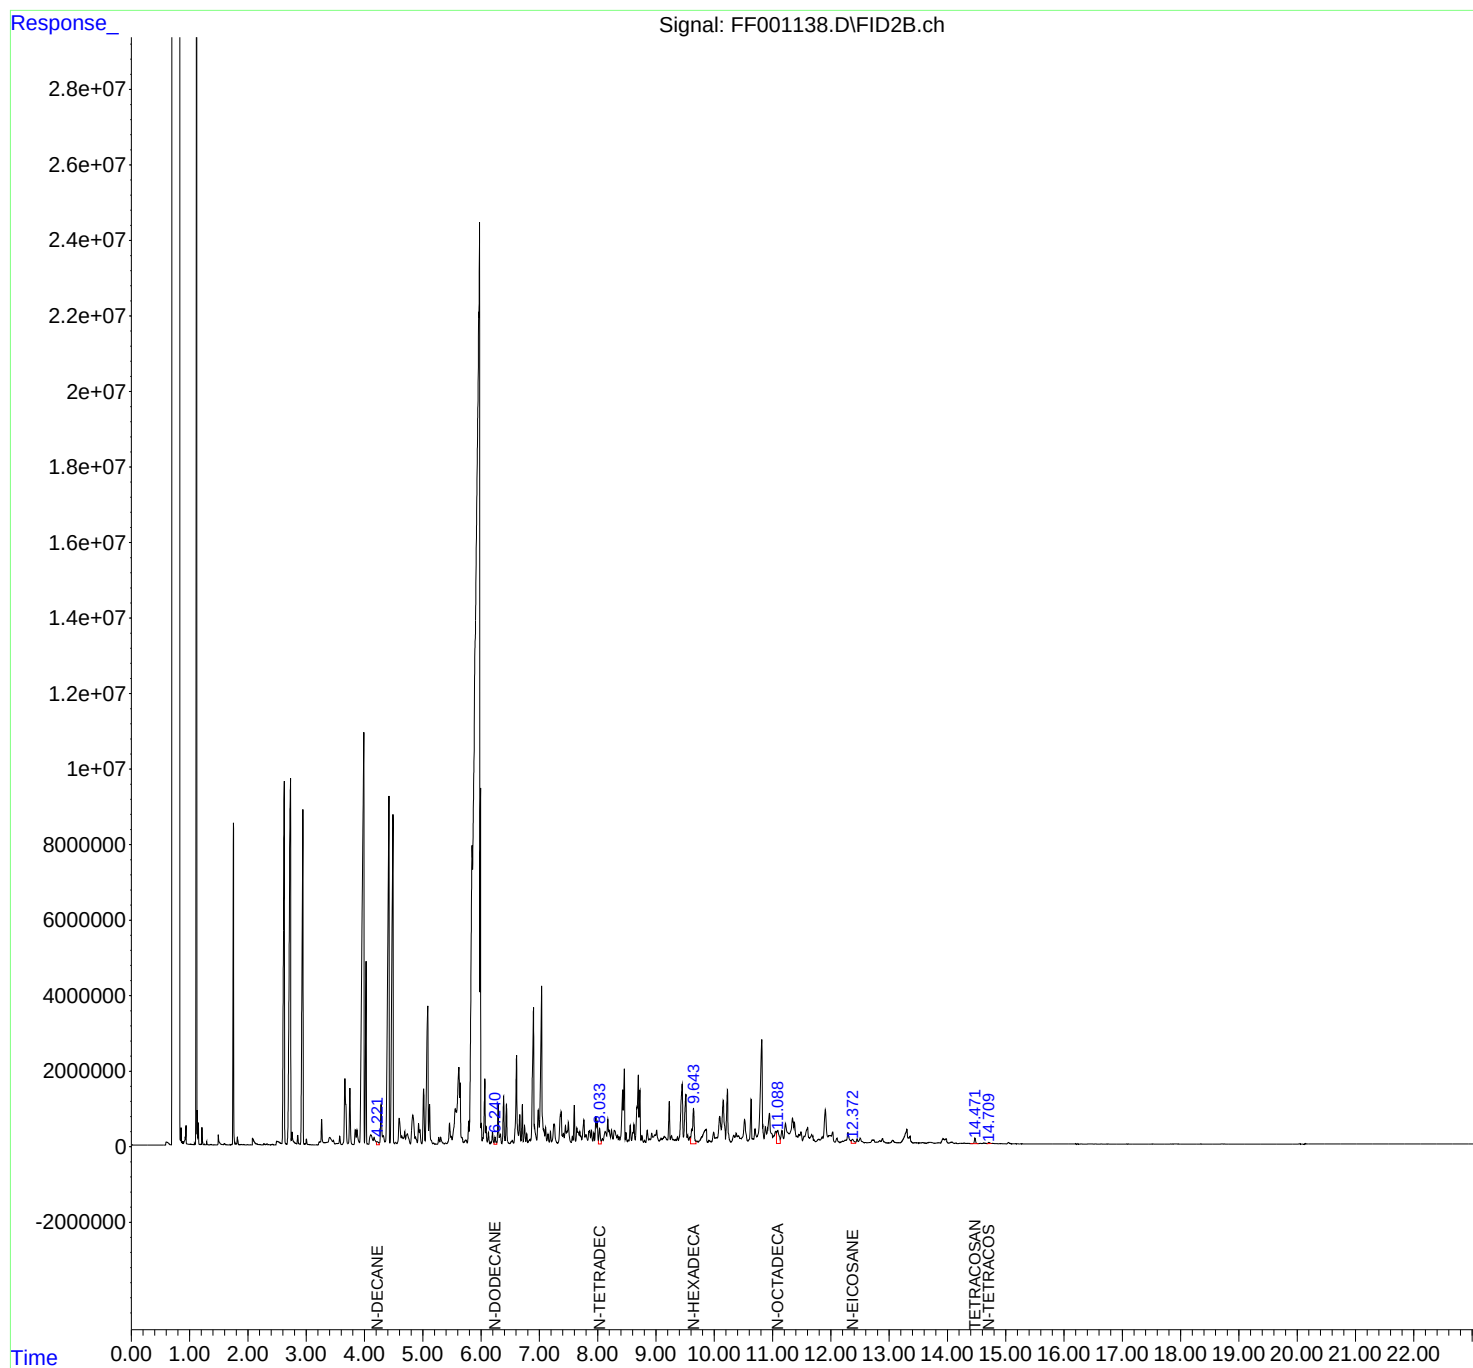


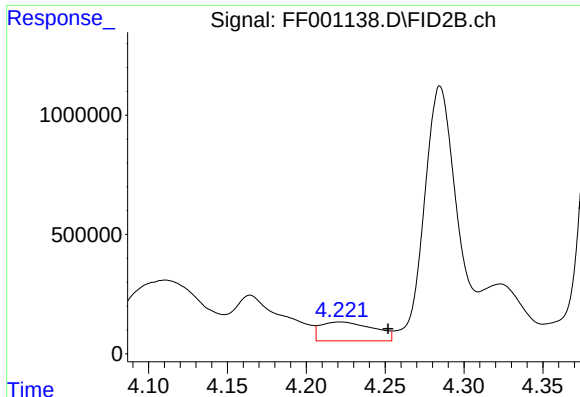

#2 N-DECANE


R.T.: 4.222 min
Delta R.T.: -0.030 min
Response: 1854528
Conc: 13.24 ug/ml

Instrument :
FID_F
ClientSampleId :

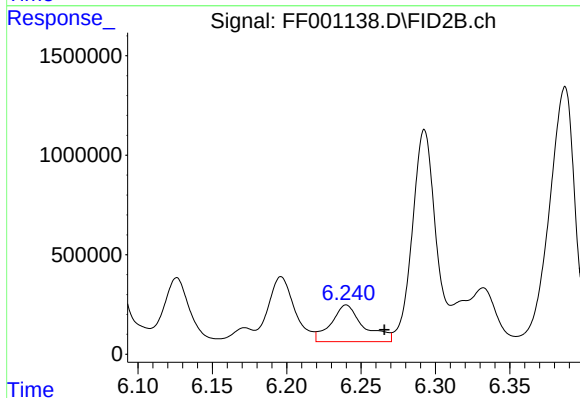


#3 N-DODECANE

R.T.: 6.240 min
Delta R.T.: -0.026 min
Response: 2812901
Conc: 20.07 ug/ml

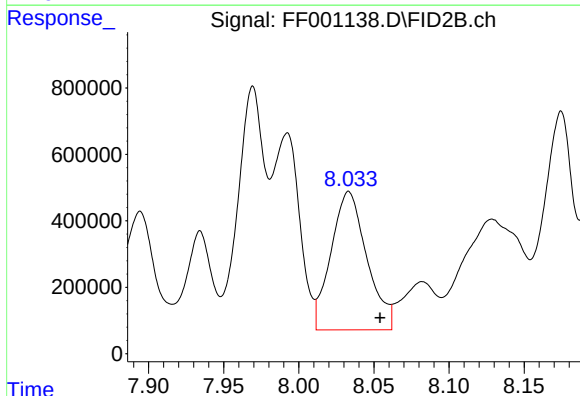


#4 N-TETRADECANE

R.T.: 8.033 min
Delta R.T.: -0.021 min
Response: 6917650
Conc: 49.68 ug/ml

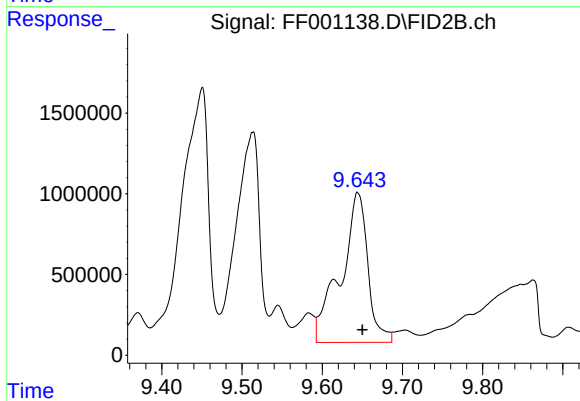

#5 N-HEXADECANE


R.T.: 9.645 min
Delta R.T.: -0.006 min
Response: 21827268
Conc: 158.31 ug/ml

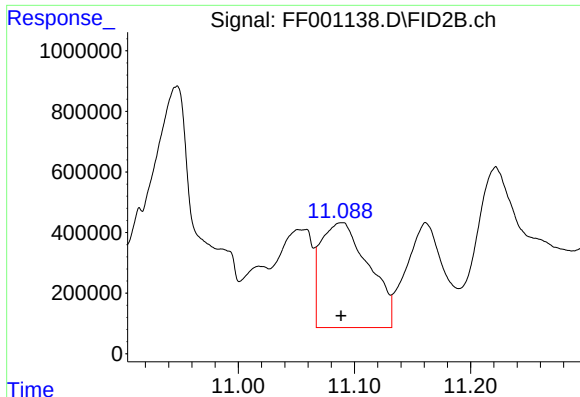

#6 N-OCTADECANE


R.T.: 11.088 min
Delta R.T.: 0.000 min
Response: 9926994
Conc: 72.70 ug/ml

Instrument :
FID_F
ClientSampleId :

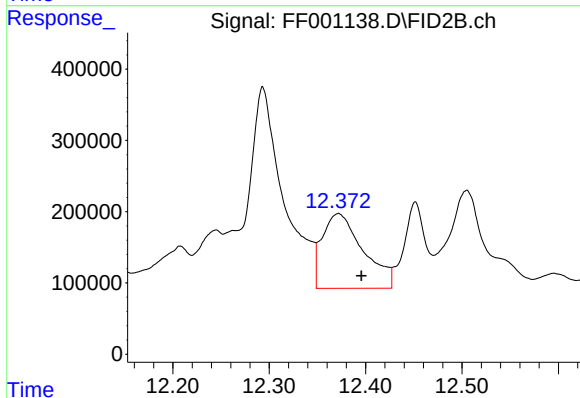


#7 N-EICOSANE

R.T.: 12.372 min
Delta R.T.: -0.024 min
Response: 3089898
Conc: 23.06 ug/ml

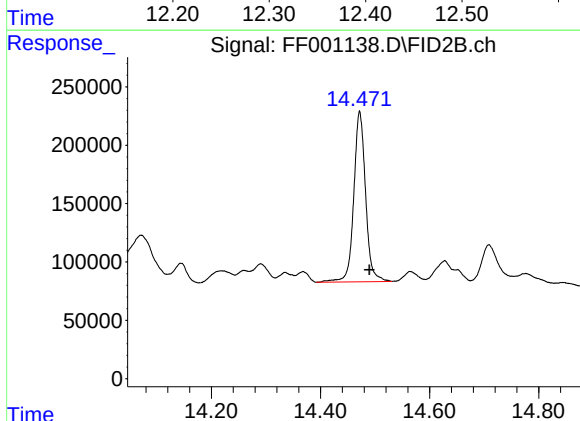

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.472 min
Delta R.T.: -0.018 min
Response: 2197761
Conc: 19.06 ug/ml

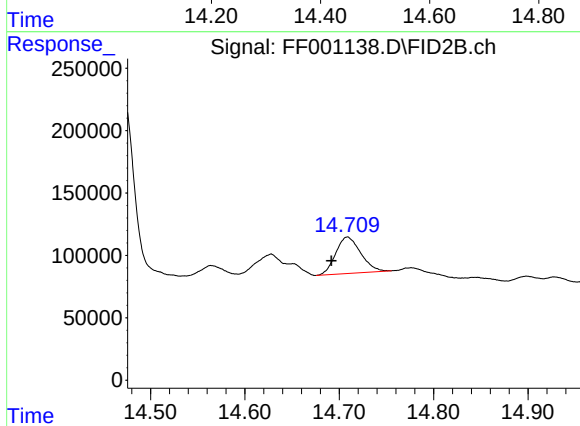

#10 N-TETRACOSANE

R.T.: 14.709 min
Delta R.T.: 0.017 min
Response: 536274
Conc: 4.13 ug/ml