

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062818\
 Data File : FF001139.D
 Signal(s) : FID2B.ch
 Acq On : 28 Jun 2018 17:30
 Operator : UA\AJ
 Sample : J3711-02
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 29 01:22:52 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.469	2192630	19.013 ug/ml
Target Compounds			
3) N-DODECANE	6.268	1242447	8.865 ug/ml
4) N-TETRADECANE	8.015	1231241	8.843 ug/ml
5) N-HEXADECANE	9.657	330287	2.396 ug/ml
6) N-OCTADECANE	11.119	514685	3.769 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062818\
Data File : FF001139.D
Signal(s) : FID2B.ch
Acq On : 28 Jun 2018 17:30
Operator : UA\AJ
Sample : J3711-02
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 29 01:22:52 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

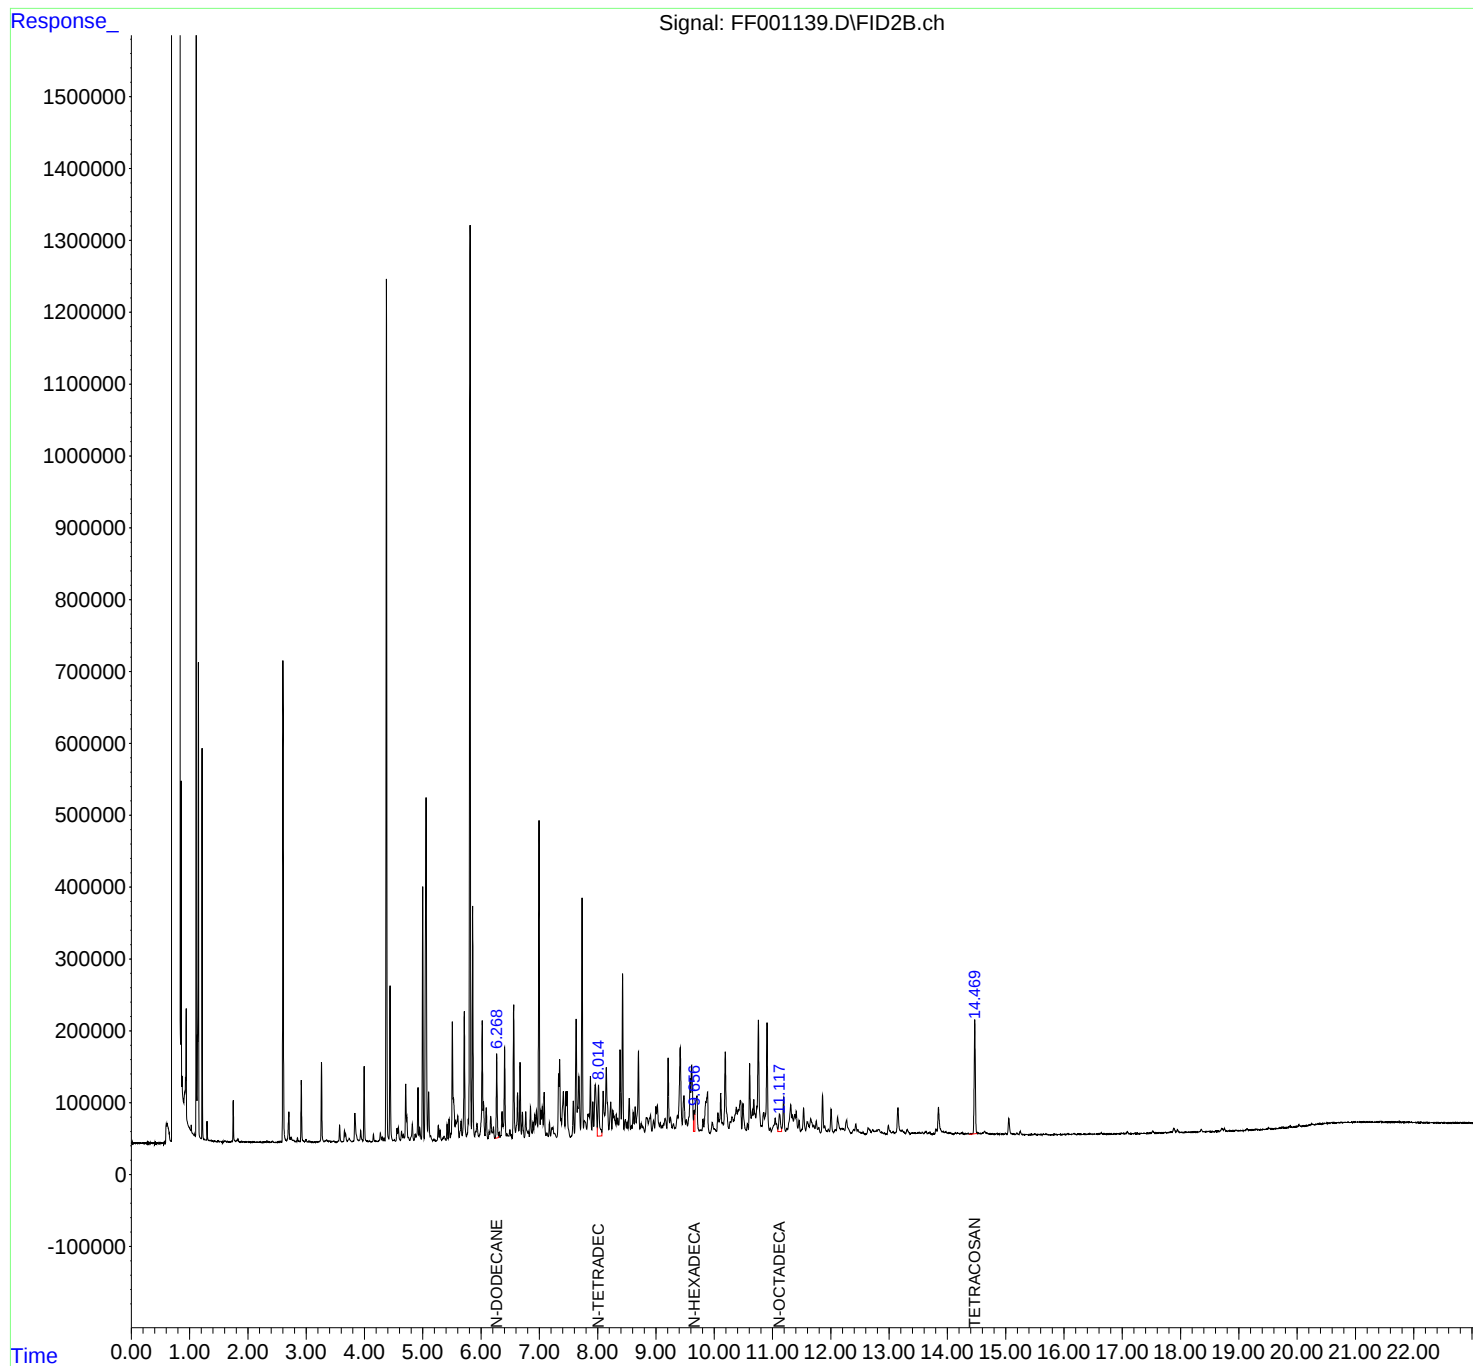


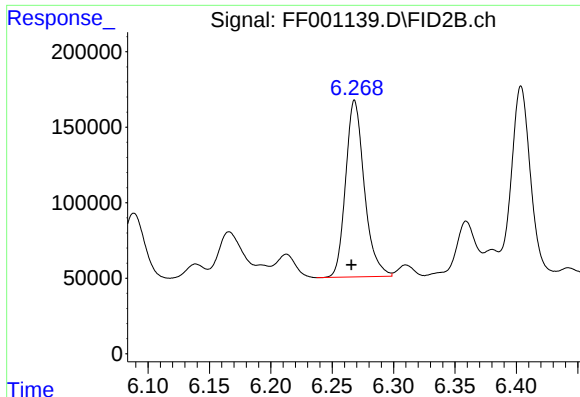

#3 N-DODECANE


R.T.: 6.268 min
Delta R.T.: 0.003 min
Response: 1242447
Conc: 8.86 ug/ml

Instrument :
FID_F
ClientSampleId :

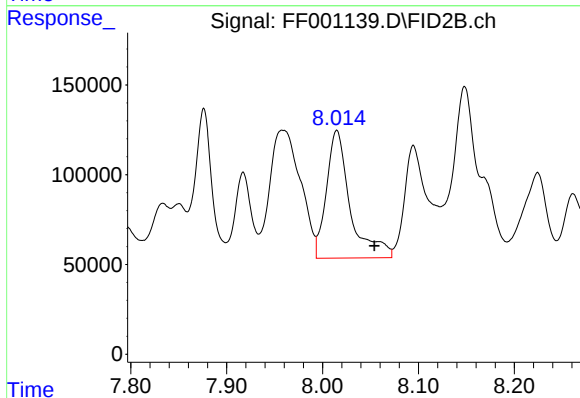


#4 N-TETRADECANE

R.T.: 8.015 min
Delta R.T.: -0.039 min
Response: 1231241
Conc: 8.84 ug/ml

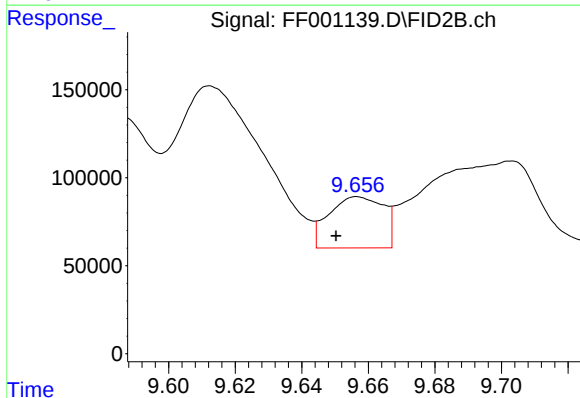


#5 N-HEXADECANE

R.T.: 9.657 min
Delta R.T.: 0.006 min
Response: 330287
Conc: 2.40 ug/ml

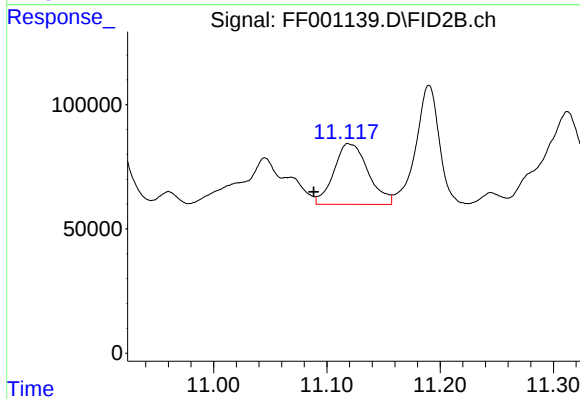

#6 N-OCTADECANE

R.T.: 11.119 min
Delta R.T.: 0.031 min
Response: 514685
Conc: 3.77 ug/ml

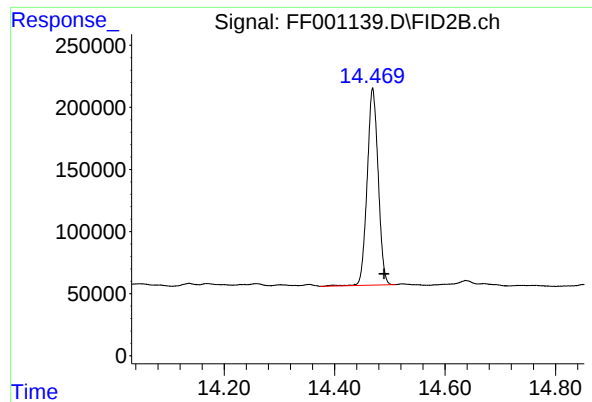

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.469 min
Delta R.T.: -0.021 min
Response: 2192630
Conc: 19.01 ug/ml

Instrument :
FID_F
ClientSampleId :