

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062818\
 Data File : FF001137.D
 Signal(s) : FID2B.ch
 Acq On : 28 Jun 2018 15:59
 Operator : UA\AJ
 Sample : PB110674BS
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB110674BS

Integration File: autoint1.e
 Quant Time: Jun 29 01:22:22 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.469	1976476	17.138 ug/ml
Target Compounds			
2) N-DECANE	4.234	2860274	20.414 ug/ml
3) N-DODECANE	6.247	2774494	19.796 ug/ml
4) N-TETRADECANE	8.035	2719233	19.530 ug/ml
5) N-HEXADECANE	9.631	2644001	19.176 ug/ml
6) N-OCTADECANE	11.068	2585438	18.933 ug/ml
7) N-EICOSANE	12.375	2518471	18.798 ug/ml
8) N-DOCOSANE	13.571	2473678	18.708 ug/ml
10) N-TETRACOSANE	14.672	2484159	19.152 ug/ml
11) N-HEXACOSANE	15.691	2423734	18.870 ug/ml
12) N-OCTACOSANE	16.640	2453024	19.291 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062818\
Data File : FF001137.D
Signal(s) : FID2B.ch
Acq On : 28 Jun 2018 15:59
Operator : UA\AJ
Sample : PB110674BS
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :
PB110674BS

Integration File: autoint1.e
Quant Time: Jun 29 01:22:22 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

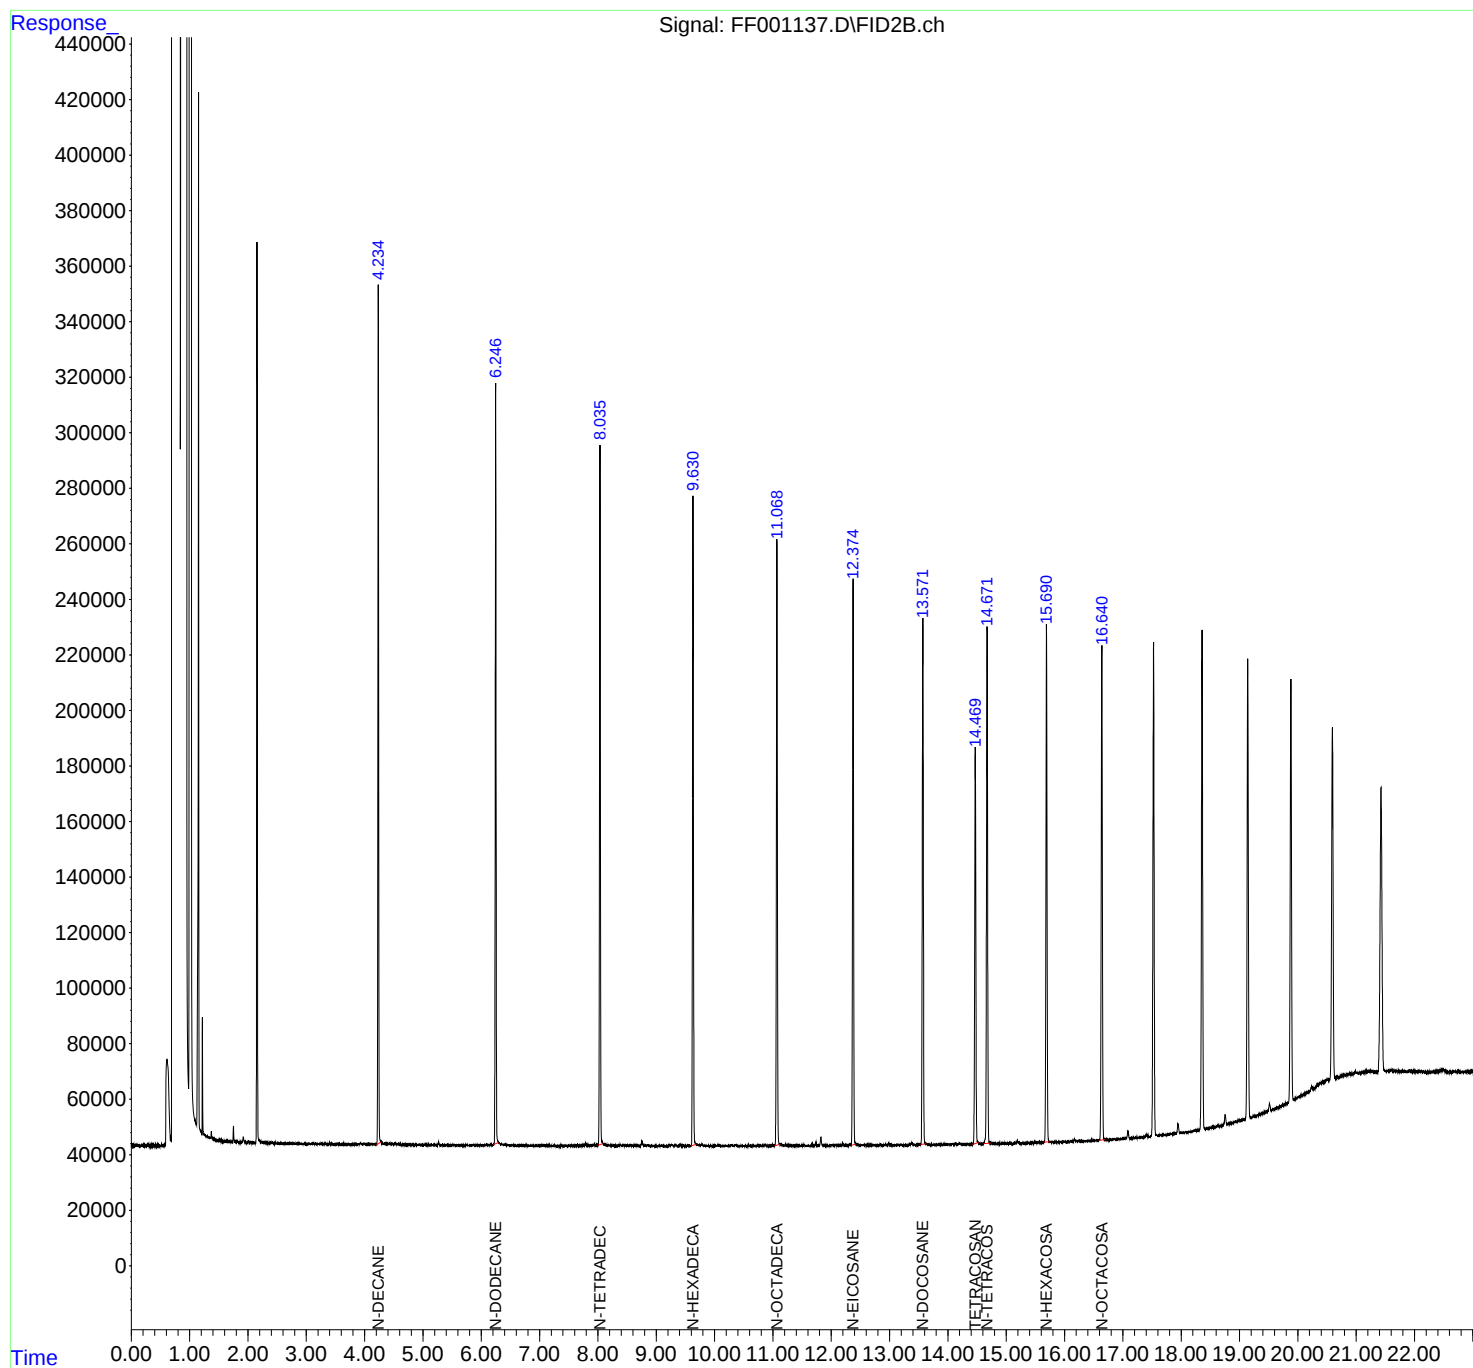


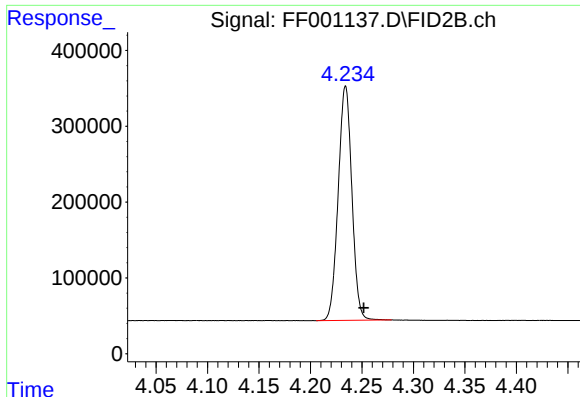

#2 N-DECANE


R.T.: 4.234 min
Delta R.T.: -0.018 min
Response: 2860274
Conc: 20.41 ug/ml

Instrument :
FID_F
ClientSampleId :
PB110674BS

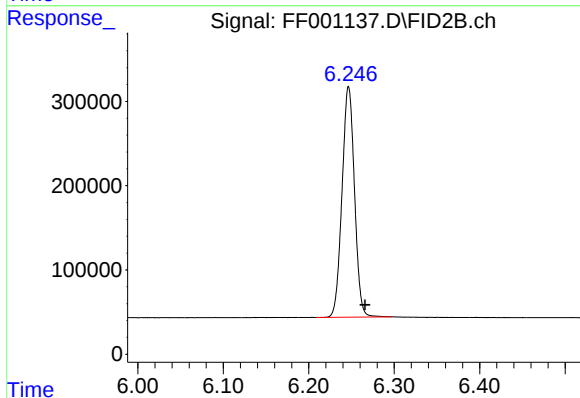


#3 N-DODECANE

R.T.: 6.247 min
Delta R.T.: -0.019 min
Response: 2774494
Conc: 19.80 ug/ml

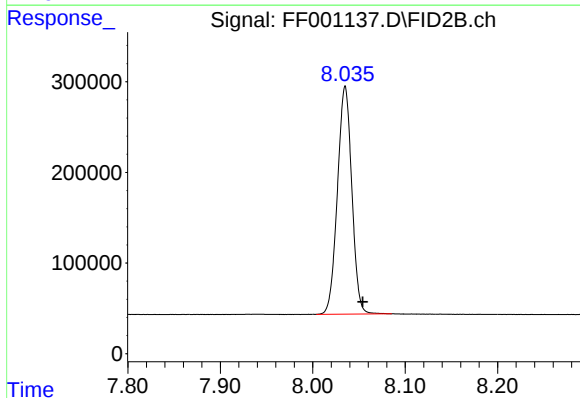


#4 N-TETRADECANE

R.T.: 8.035 min
Delta R.T.: -0.019 min
Response: 2719233
Conc: 19.53 ug/ml

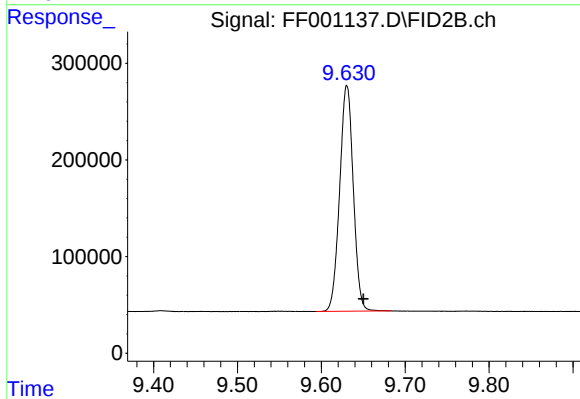

#5 N-HEXADECANE


R.T.: 9.631 min
Delta R.T.: -0.020 min
Response: 2644001
Conc: 19.18 ug/ml

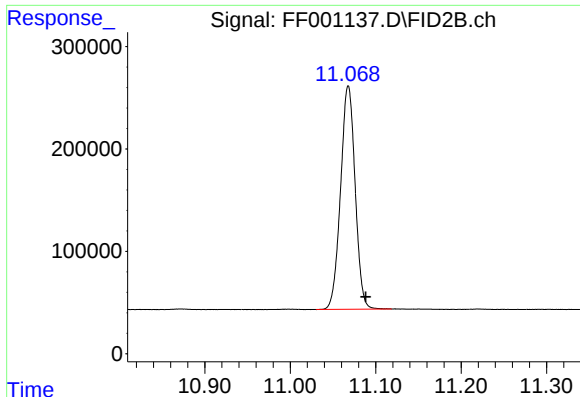

#6 N-OCTADECANE


R.T.: 11.068 min
Delta R.T.: -0.020 min
Response: 2585438
Conc: 18.93 ug/ml

Instrument :
FID_F
ClientSampleId :
PB110674BS

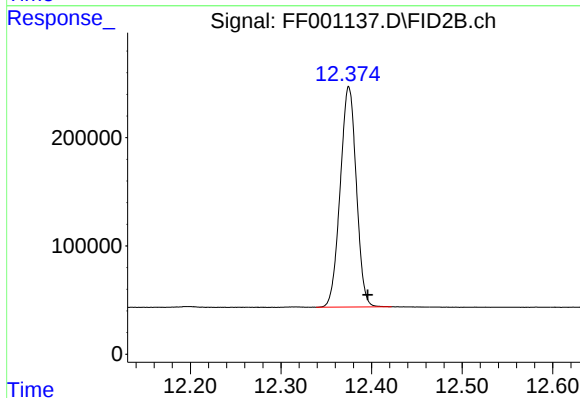


#7 N-EICOSANE

R.T.: 12.375 min
Delta R.T.: -0.021 min
Response: 2518471
Conc: 18.80 ug/ml

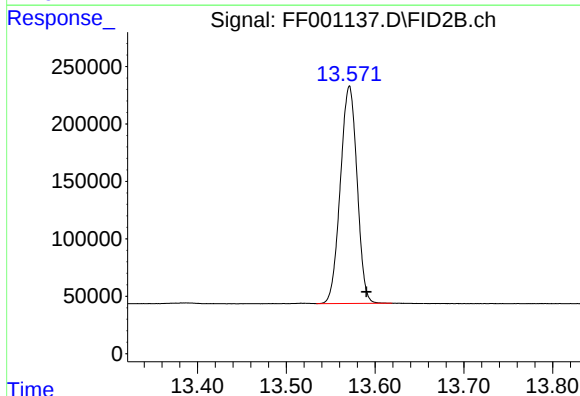


#8 N-DOCOSANE

R.T.: 13.571 min
Delta R.T.: -0.019 min
Response: 2473678
Conc: 18.71 ug/ml

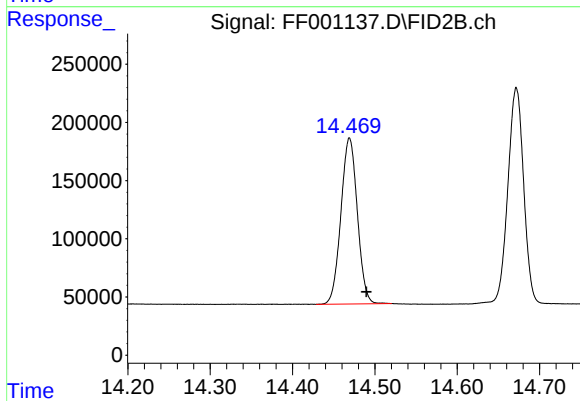

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.469 min
Delta R.T.: -0.021 min
Response: 1976476
Conc: 17.14 ug/ml

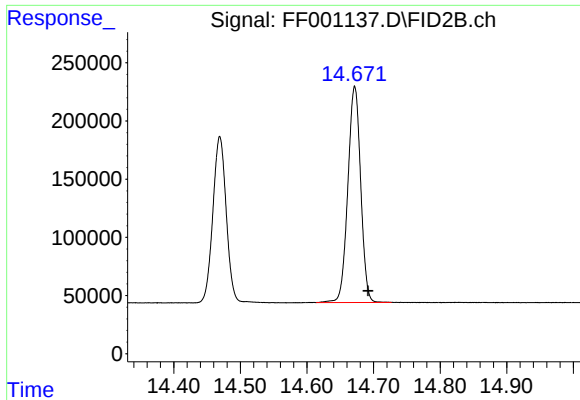

#10 N-TETRACOSANE


R.T.: 14.672 min
Delta R.T.: -0.020 min
Response: 2484159
Conc: 19.15 ug/ml

Instrument :
FID_F
ClientSampleId :
PB110674BS

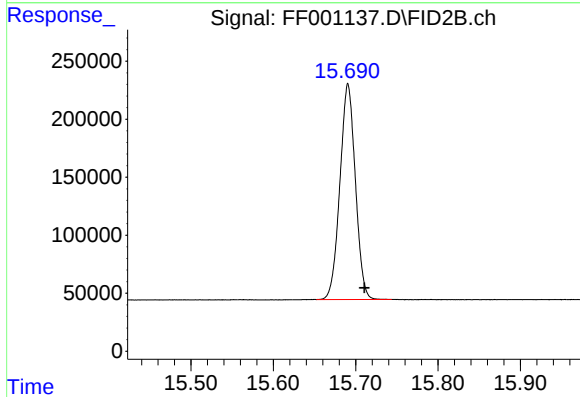

#11 N-HEXACOSANE

R.T.: 15.691 min
Delta R.T.: -0.020 min
Response: 2423734
Conc: 18.87 ug/ml

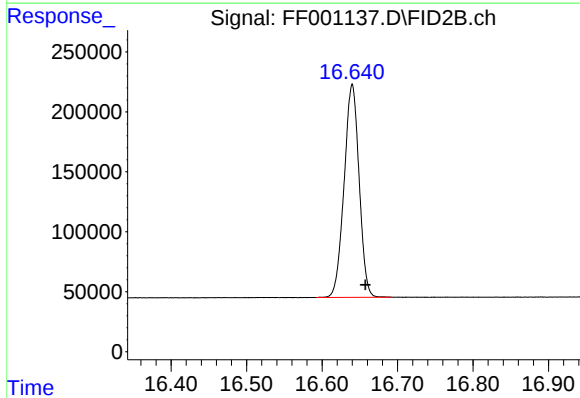

#12 N-OCTACOSANE

R.T.: 16.640 min
Delta R.T.: -0.018 min
Response: 2453024
Conc: 19.29 ug/ml