

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062818\
 Data File : FF001142.D
 Signal(s) : FID2B.ch
 Acq On : 28 Jun 2018 19:01
 Operator : UA\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 29 01:23:27 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.471	5380514	46.656 ug/ml
Target Compounds			
2) N-DECANE	4.236	8137348	58.075 ug/ml
3) N-DODECANE	6.249	7670001	54.726 ug/ml
4) N-TETRADECANE	8.037	7233581	51.954 ug/ml
5) N-HEXADECANE	9.633	6868075	49.813 ug/ml
6) N-OCTADECANE	11.071	6592013	48.274 ug/ml
7) N-EICOSANE	12.378	6322578	47.191 ug/ml
8) N-DOCOSANE	13.573	6155972	46.556 ug/ml
10) N-TETRACOSANE	14.675	6076349	46.846 ug/ml
11) N-HEXACOSANE	15.694	6039864	47.023 ug/ml
12) N-OCTACOSANE	16.642	6128814	48.198 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062818\
Data File : FF001142.D
Signal(s) : FID2B.ch
Acq On : 28 Jun 2018 19:01
Operator : UA\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 29 01:23:27 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

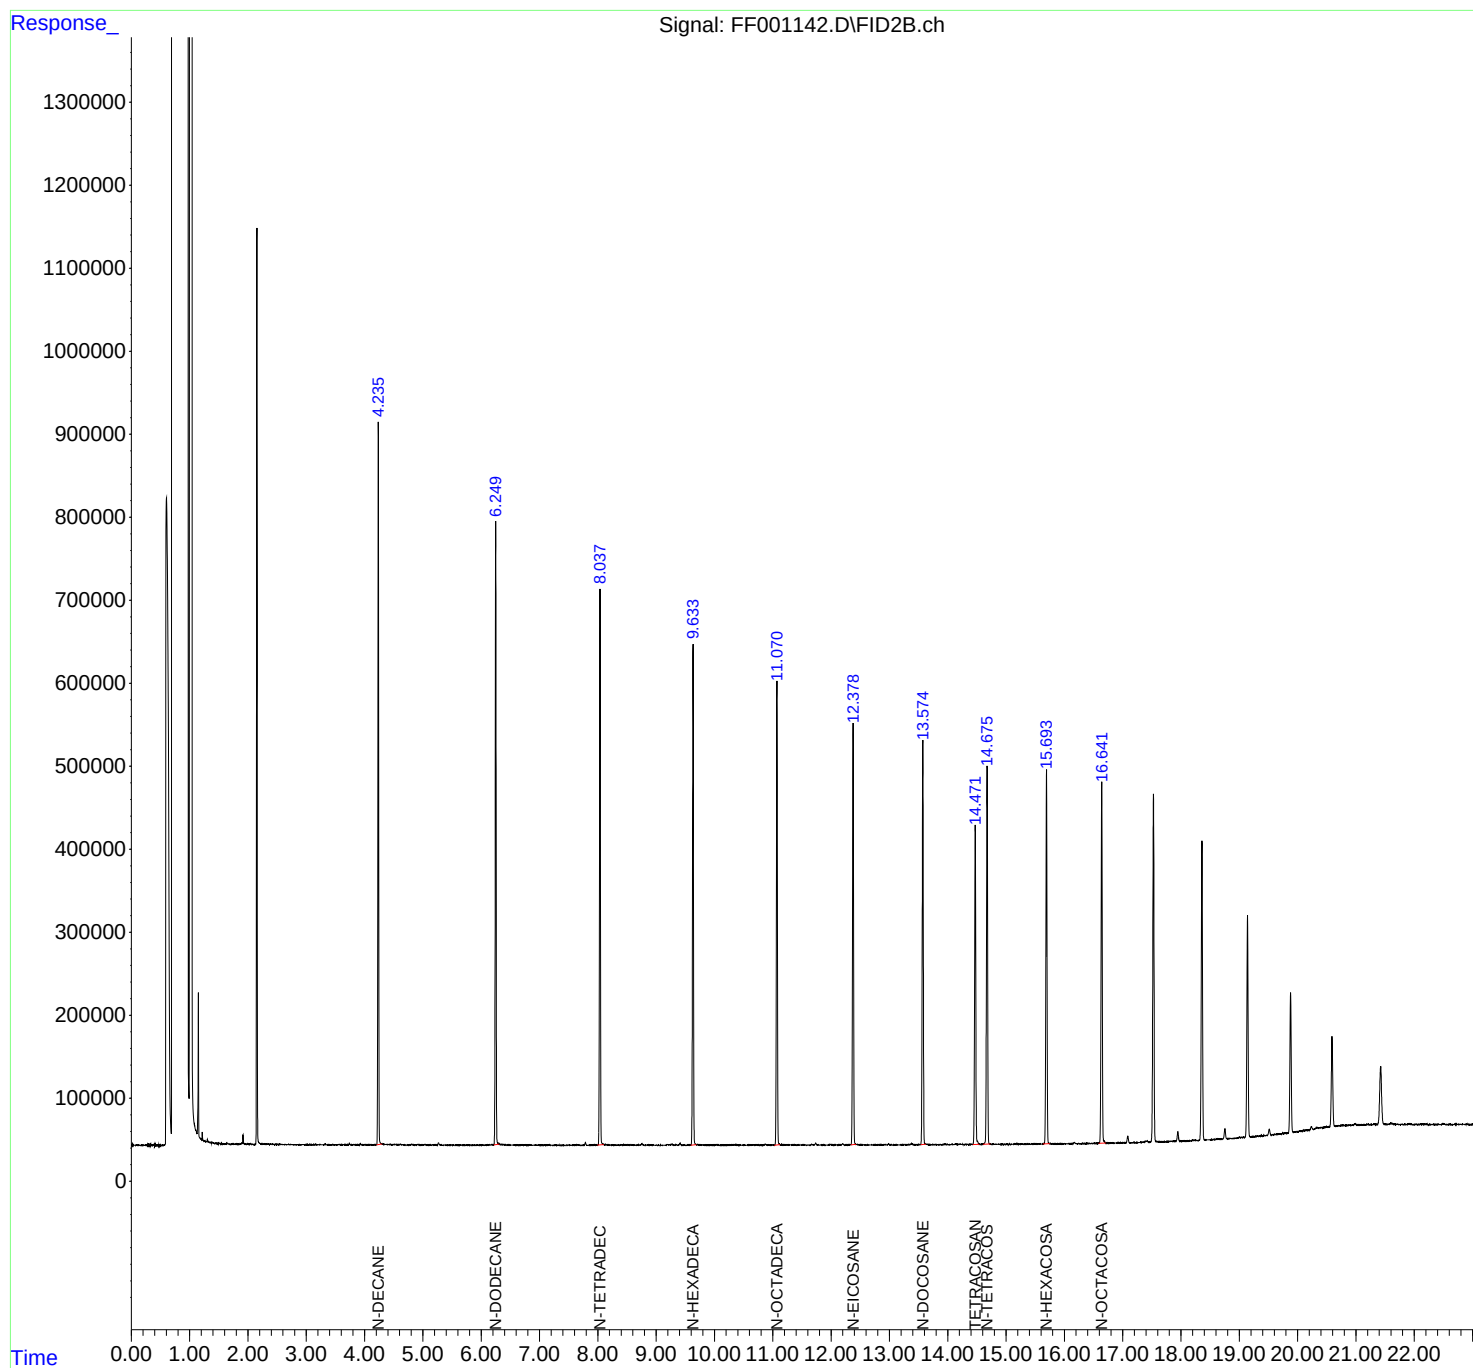


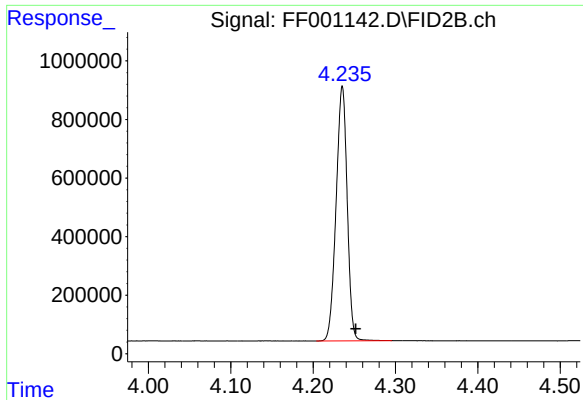

#2 N-DECANE


R.T.: 4.236 min
Delta R.T.: -0.016 min
Response: 8137348
Conc: 58.08 ug/ml

Instrument :
FID_F
ClientSampleId :

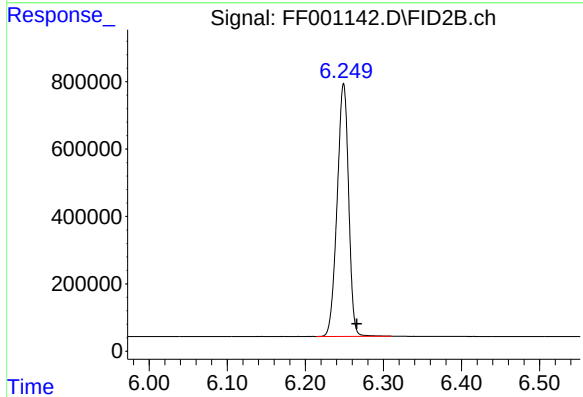


#3 N-DODECANE

R.T.: 6.249 min
Delta R.T.: -0.017 min
Response: 7670001
Conc: 54.73 ug/ml

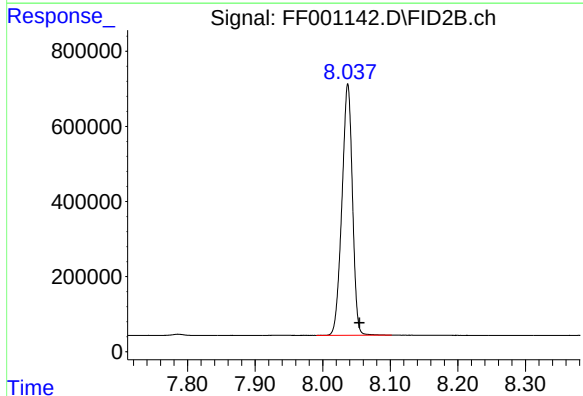


#4 N-TETRADECANE

R.T.: 8.037 min
Delta R.T.: -0.017 min
Response: 7233581
Conc: 51.95 ug/ml

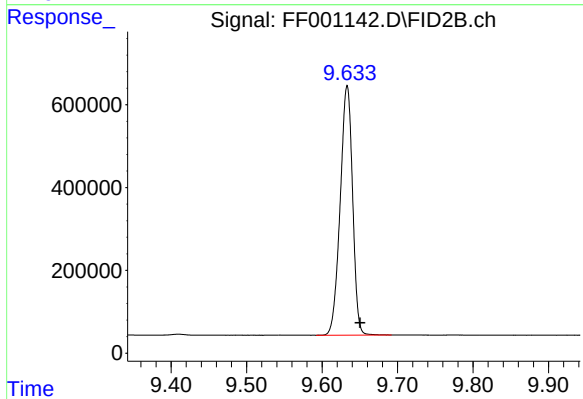

#5 N-HEXADECANE


R.T.: 9.633 min
Delta R.T.: -0.017 min
Response: 6868075
Conc: 49.81 ug/ml

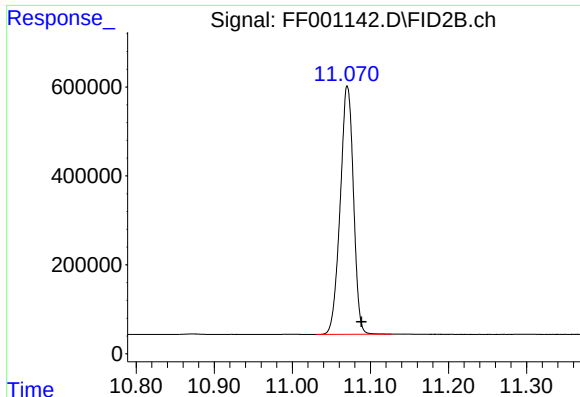

#6 N-OCTADECANE


R.T.: 11.071 min
Delta R.T.: -0.018 min
Response: 6592013
Conc: 48.27 ug/ml

Instrument :
FID_F
ClientSampleId :

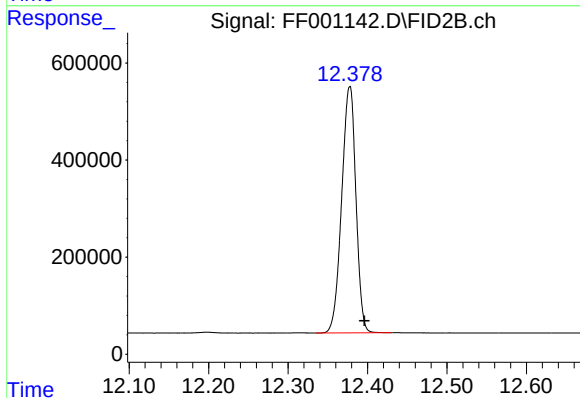


#7 N-EICOSANE

R.T.: 12.378 min
Delta R.T.: -0.018 min
Response: 6322578
Conc: 47.19 ug/ml

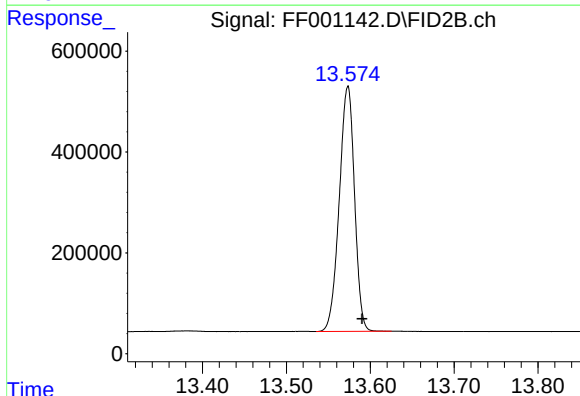


#8 N-DOCOSANE

R.T.: 13.573 min
Delta R.T.: -0.017 min
Response: 6155972
Conc: 46.56 ug/ml

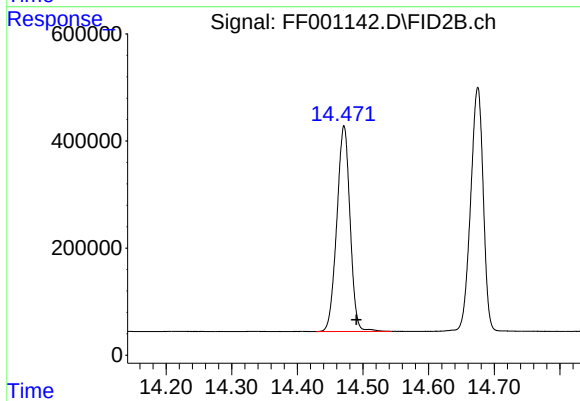

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.471 min
Delta R.T.: -0.019 min
Response: 5380514
Conc: 46.66 ug/ml

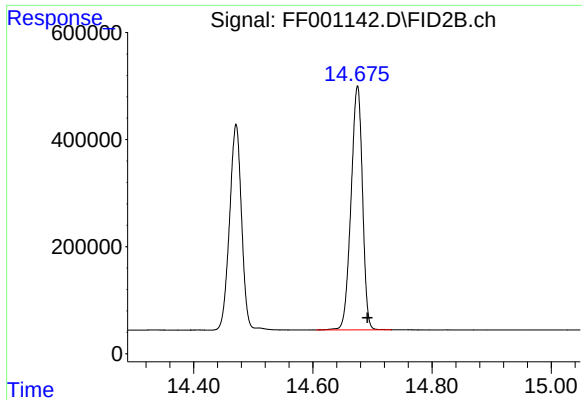

#10 N-TETRACOSANE


R.T.: 14.675 min
Delta R.T.: -0.017 min
Response: 6076349
Conc: 46.85 ug/ml

Instrument :
FID_F
ClientSampleId :

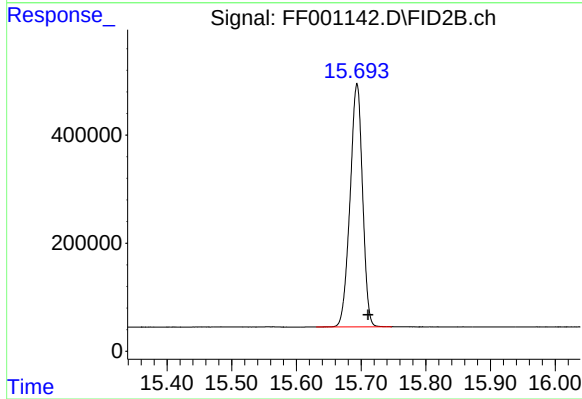

#11 N-HEXACOSANE

R.T.: 15.694 min
Delta R.T.: -0.017 min
Response: 6039864
Conc: 47.02 ug/ml

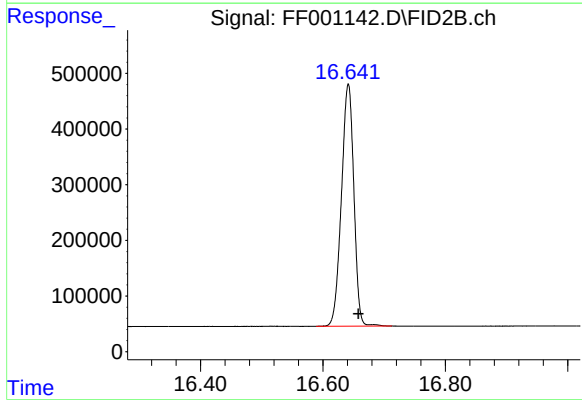

#12 N-OCTACOSANE

R.T.: 16.642 min
Delta R.T.: -0.016 min
Response: 6128814
Conc: 48.20 ug/ml