

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062821\
 Data File : FF008654.D
 Signal(s) : FID2B.ch
 Acq On : 28 Jun 2021 10:37
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Jun 29 01:34:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
 Quant Title :
 QLast Update : Thu Jun 24 08:07:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.519	2776872	20.418 ug/ml
12) N-OCTACOSANE	16.914	2514918	20.333 ug/ml
14) N-DOTRIACONTANE	18.628	190724	1.628 ug/ml
16) N-HEXATRIACONTANE	20.183	232719	2.478 ug/ml
18) N-TETRACONTANE	21.845	221429	2.393 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062821\
Data File : FF008654.D
Signal(s) : FID2B.ch
Acq On : 28 Jun 2021 10:37
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Jun 29 01:34:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

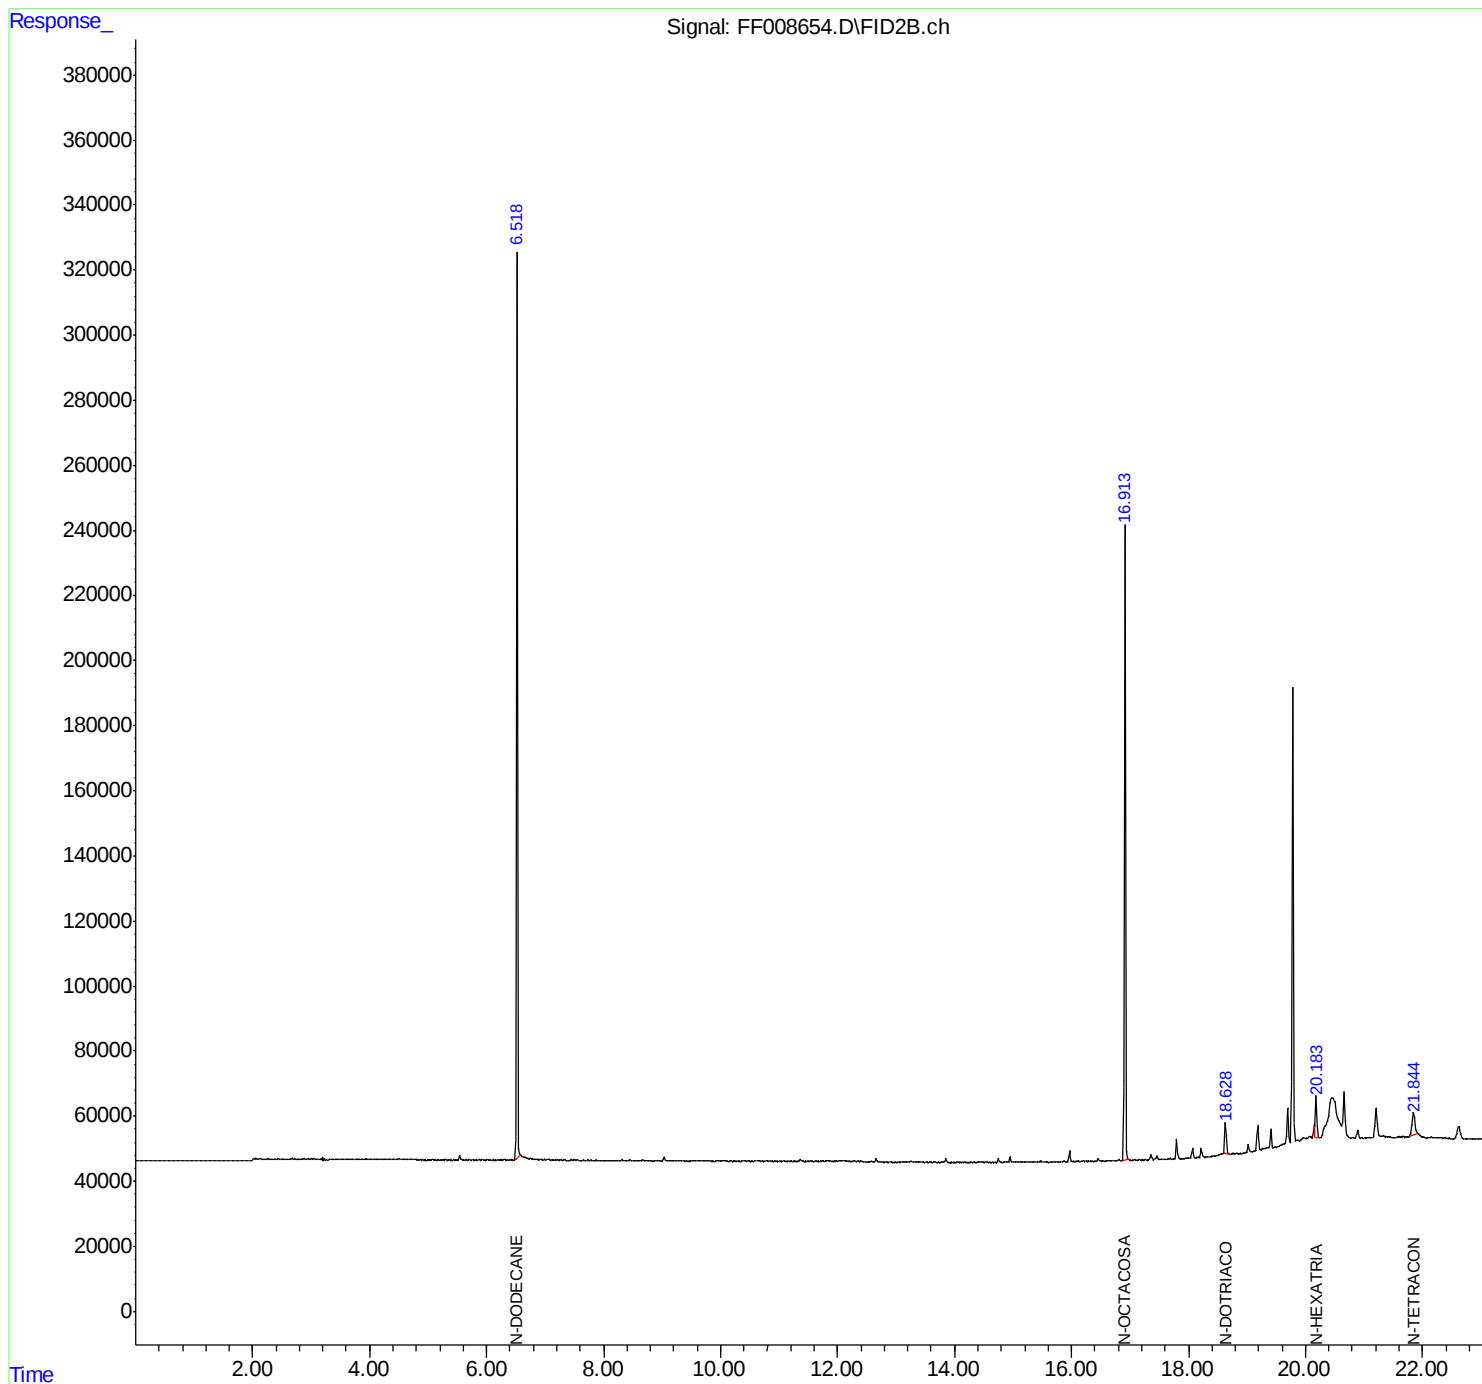


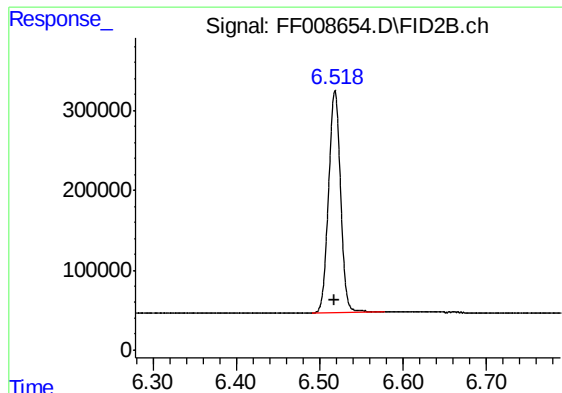

#3 N-DODECANE


R.T.: 6.519 min
Delta R.T.: 0.000 min
Response: 2776872
Conc: 20.42 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

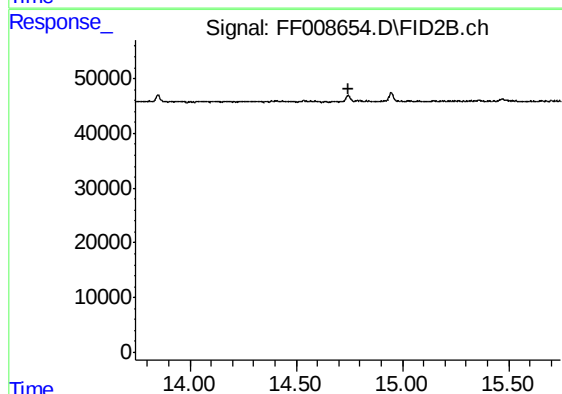


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.744 min
Response: 0
Conc: N.D.

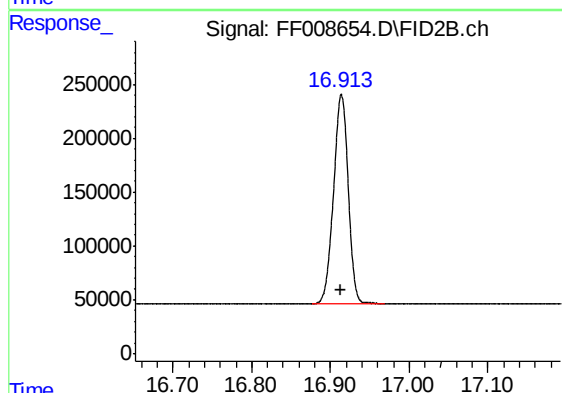


#12 N-OCTACOSANE

R.T.: 16.914 min
Delta R.T.: 0.000 min
Response: 2514918
Conc: 20.33 ug/ml

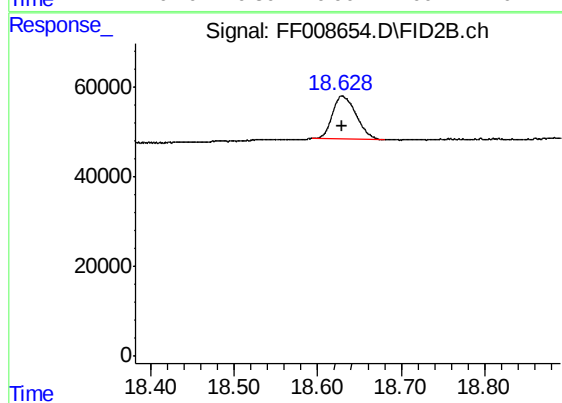

#14 N-DOTRIACONTANE


R.T.: 18.628 min
Delta R.T.: 0.000 min
Response: 190724
Conc: 1.63 ug/ml

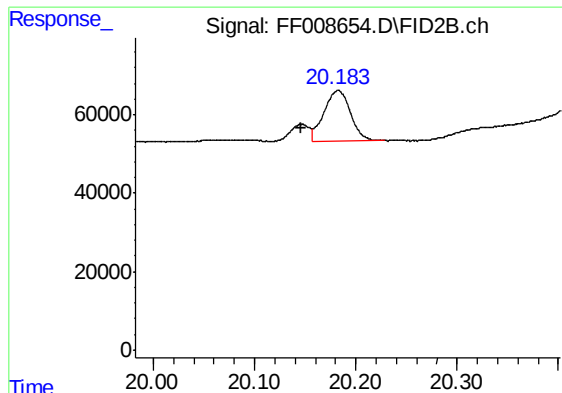

#16 N-HEXATRIACONTANE

R.T.: 20.183 min
Delta R.T.: 0.037 min
Response: 232719
Conc: 2.48 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

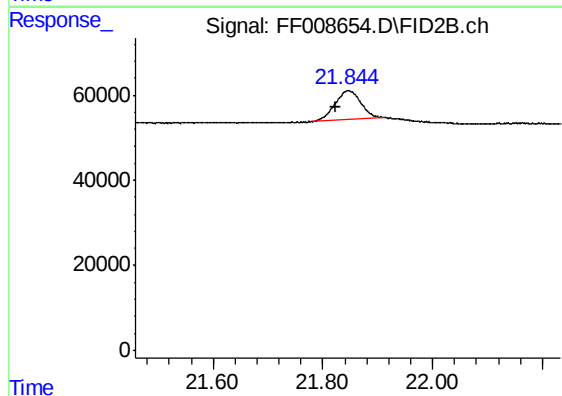

#18 N-TETRACONTANE

R.T.: 21.845 min
Delta R.T.: 0.022 min
Response: 221429
Conc: 2.39 ug/ml