

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062821\
Data File : FF008657.D
Signal(s) : FID2B.ch
Acq On : 28 Jun 2021 12:10
Operator : DD\AJ
Sample : M2856-02
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-01-COMP

Integration File: autoint1.e
Quant Time: Jun 29 01:35:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.744	2267946	19.900 ug/ml
Target Compounds			
18) N-TETRACONTANE	21.850	307224	3.320 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062821\
Data File : FF008657.D
Signal(s) : FID2B.ch
Acq On : 28 Jun 2021 12:10
Operator : DD\AJ
Sample : M2856-02
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-01-COMP

Integration File: autoint1.e
Quant Time: Jun 29 01:35:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

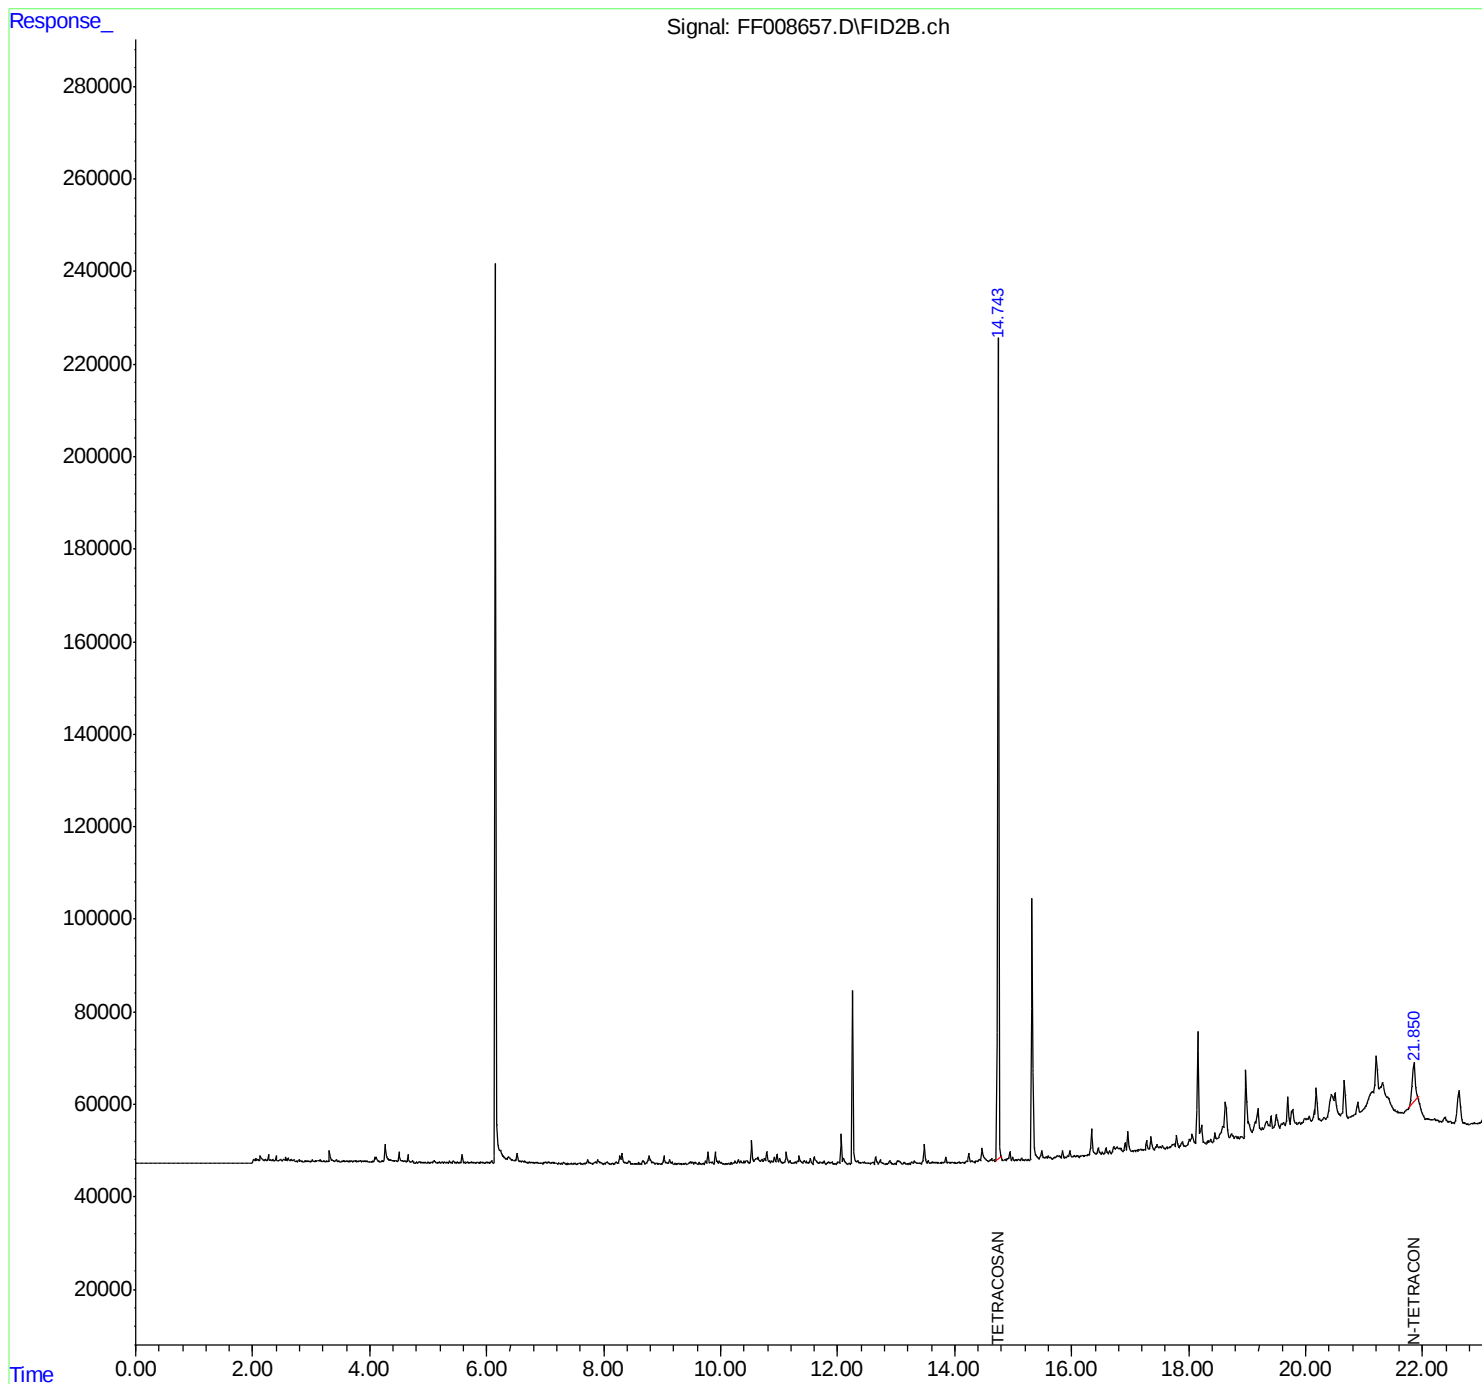


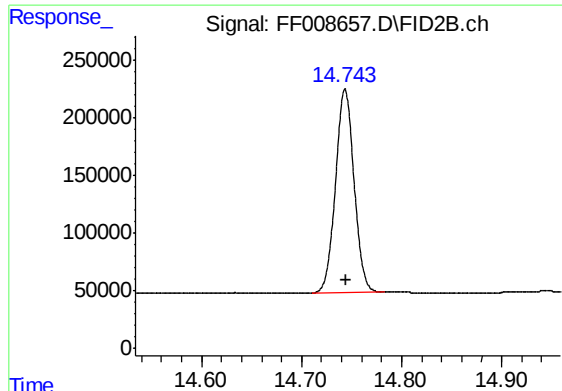

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.744 min
Delta R.T.: 0.000 min
Response: 2267946
Conc: 19.90 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-01-COMP

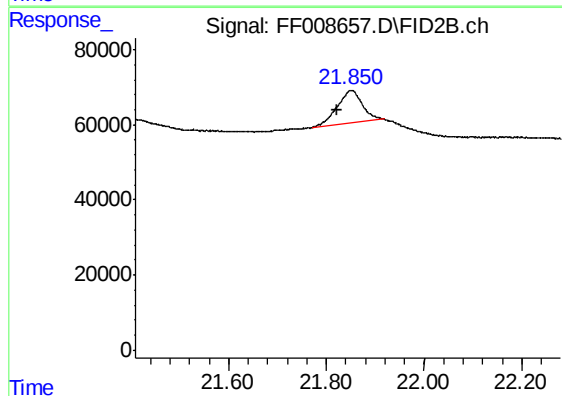

#18 N-TETRACONTANE

R.T.: 21.850 min
Delta R.T.: 0.027 min
Response: 307224
Conc: 3.32 ug/ml