

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062821\
 Data File : FF008658.D
 Signal(s) : FID2B.ch
 Acq On : 28 Jun 2021 12:41
 Operator : DD\AJ
 Sample : M2856-04
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SB-02-COMP

Integration File: autoint1.e
 Quant Time: Jun 29 01:35:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
 Quant Title :
 QLast Update : Thu Jun 24 08:07:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.745	1782864	15.643 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.629	184839	1.578 ug/ml
16) N-HEXATRIACONTANE	20.183	160274	1.706 ug/ml
18) N-TETRACONTANE	21.853	374809	4.050 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062821\
Data File : FF008658.D
Signal(s) : FID2B.ch
Acq On : 28 Jun 2021 12:41
Operator : DD\AJ
Sample : M2856-04
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-02-COMP

Integration File: autoint1.e
Quant Time: Jun 29 01:35:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

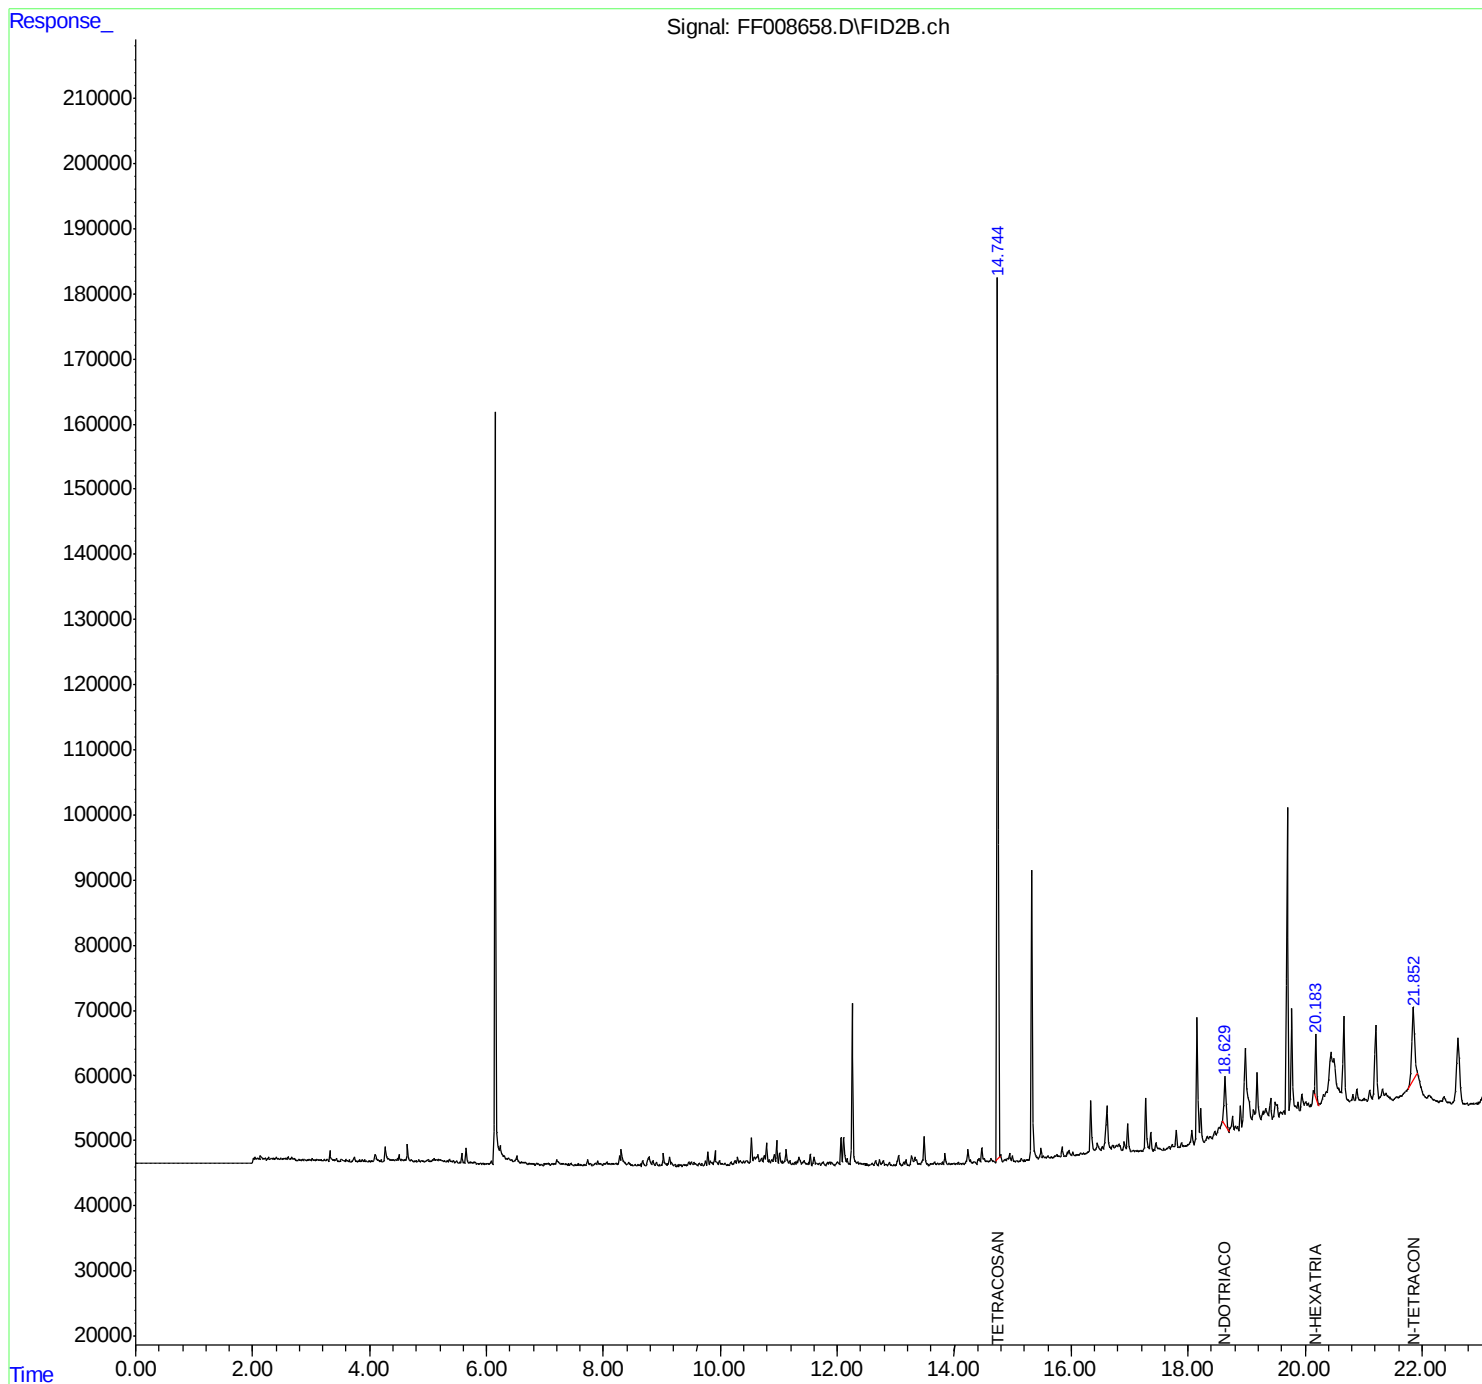


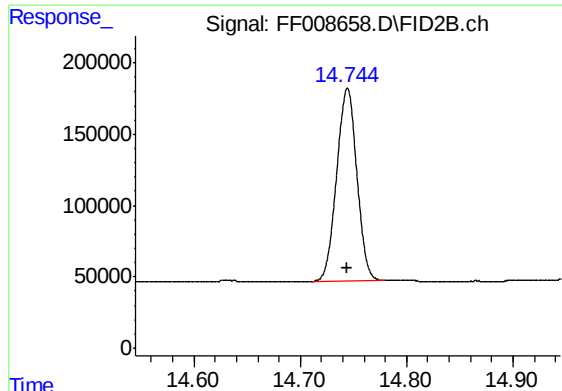

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.745 min
Delta R.T.: 0.000 min
Response: 1782864
Conc: 15.64 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-02-COMP

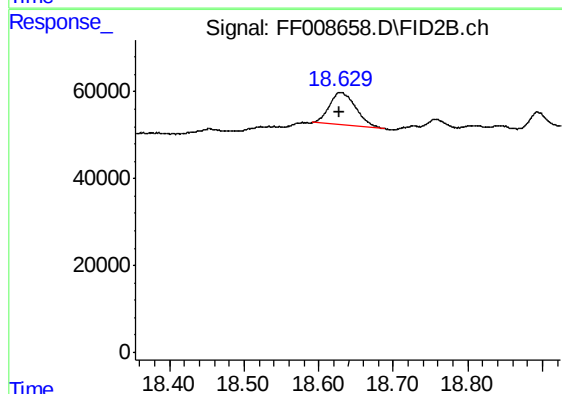


#14 N-DOTRIACONTANE

R.T.: 18.629 min
Delta R.T.: 0.000 min
Response: 184839
Conc: 1.58 ug/ml

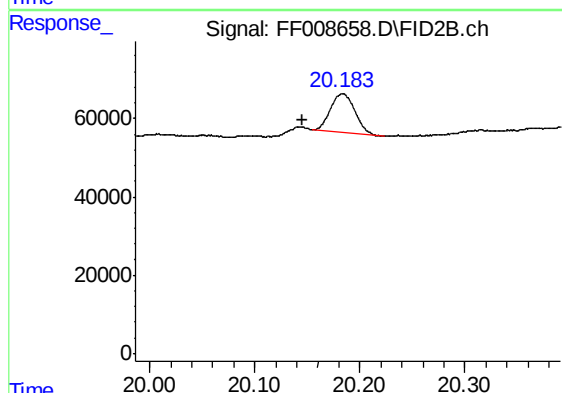

#16 N-HEXATRIACONTANE

R.T.: 20.183 min
Delta R.T.: 0.037 min
Response: 160274
Conc: 1.71 ug/ml

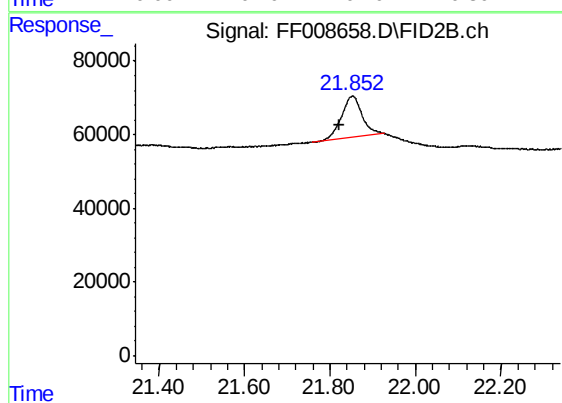

#18 N-TETRACONTANE

R.T.: 21.853 min
Delta R.T.: 0.030 min
Response: 374809
Conc: 4.05 ug/ml