

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062821\
Data File : FF008674.D
Signal(s) : FID2B.ch
Acq On : 28 Jun 2021 21:07
Operator : DD\AJ
Sample : M2828-13
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PW-2R

Integration File: autoint1.e
Quant Time: Jun 29 01:44:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.744	1710699	15.010 ug/ml
Target Compounds				
3)	N-DODECANE	6.542	134927	0.992 ug/ml
4)	N-TETRADECANE	8.299	444381	3.294 ug/ml
5)	N-HEXADECANE	9.926	620438	4.542 ug/ml
10)	N-TETRACOSANE	14.897f	76441	0.580 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062821\
Data File : FF008674.D
Signal(s) : FID2B.ch
Acq On : 28 Jun 2021 21:07
Operator : DD\AJ
Sample : M2828-13
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PW-2R

Integration File: autoint1.e
Quant Time: Jun 29 01:44:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

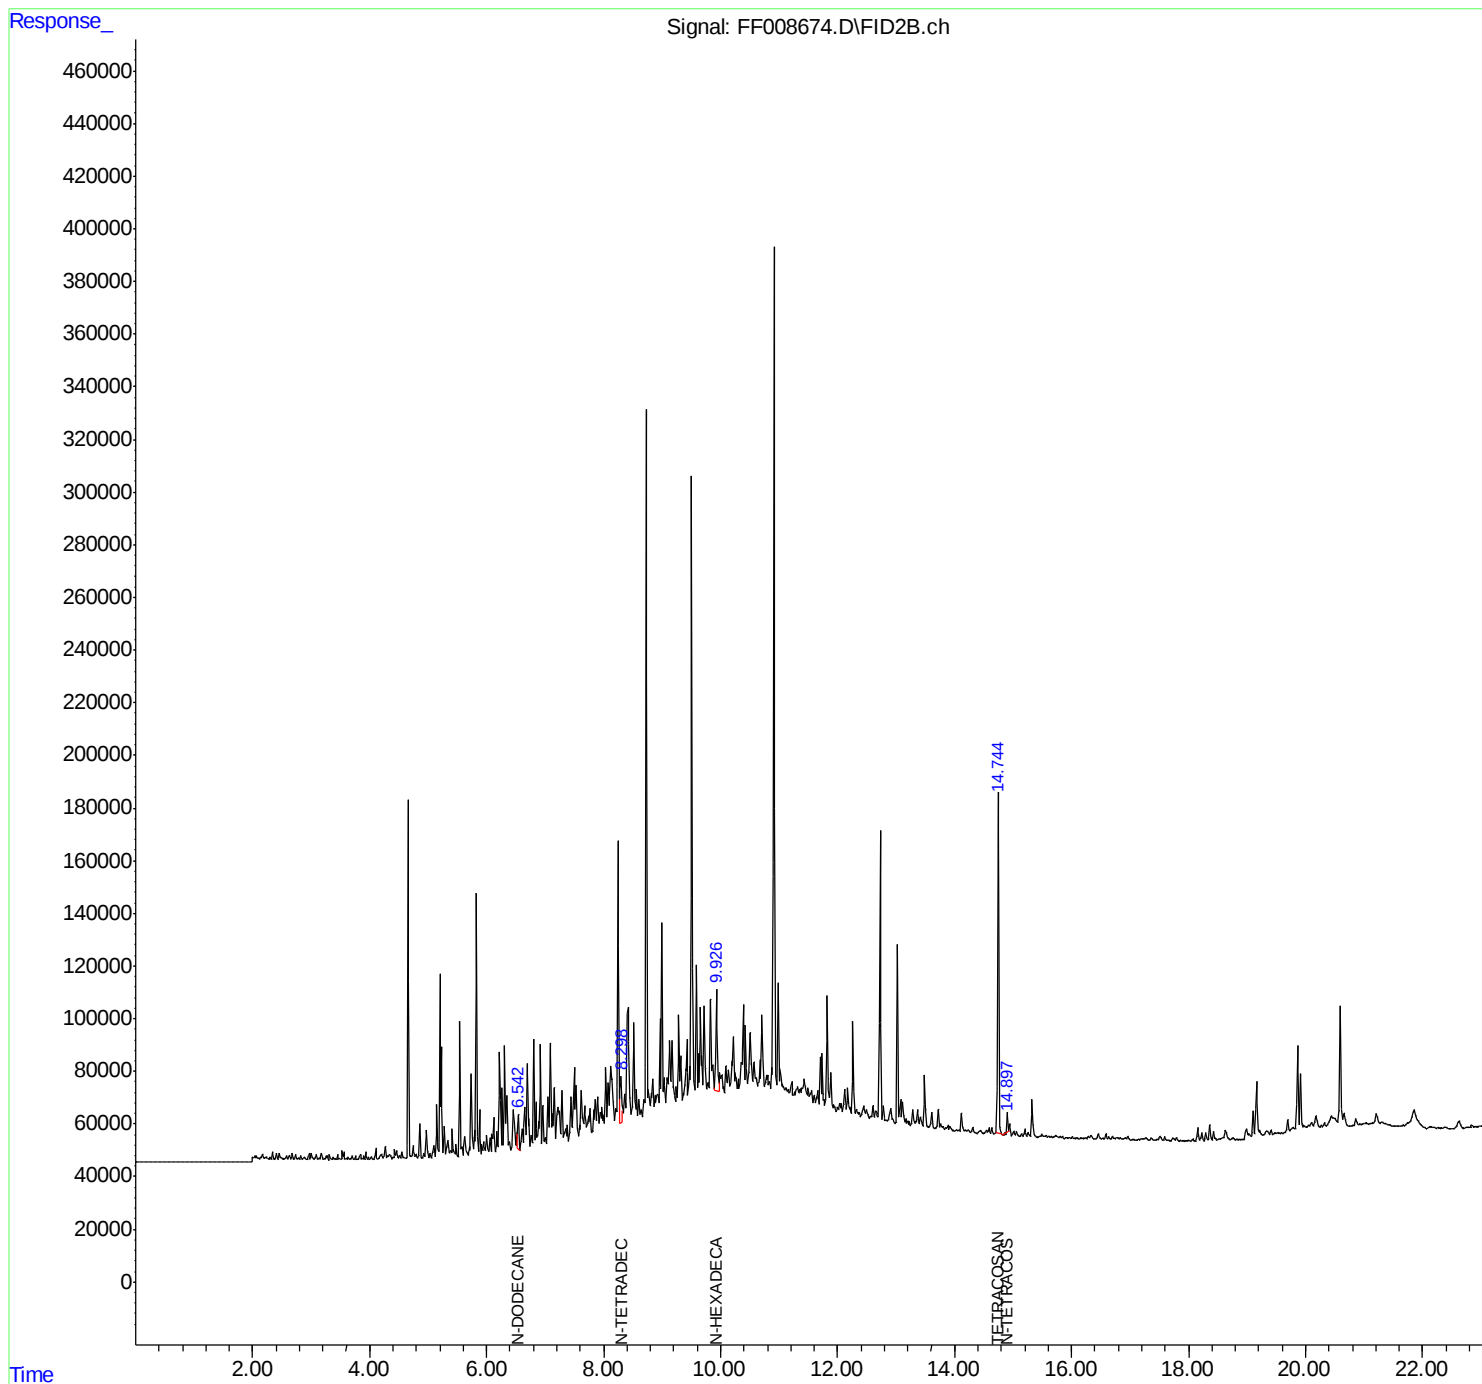


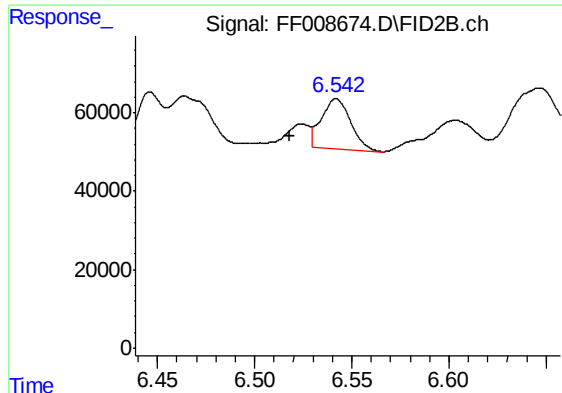

#3 N-DODECANE


R.T.: 6.542 min
Delta R.T.: 0.024 min
Response: 134927
Conc: 0.99 ug/ml

Instrument :
FID_F
ClientSampleId :
PW-2R

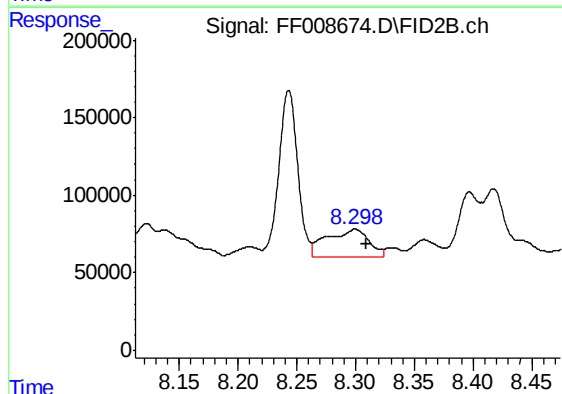


#4 N-TETRADECANE

R.T.: 8.299 min
Delta R.T.: -0.010 min
Response: 444381
Conc: 3.29 ug/ml

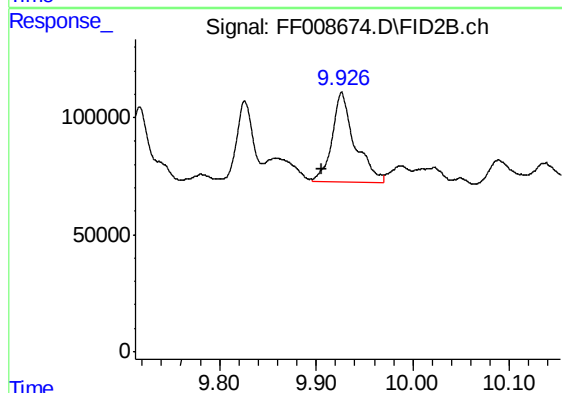


#5 N-HEXADECANE

R.T.: 9.926 min
Delta R.T.: 0.020 min
Response: 620438
Conc: 4.54 ug/ml

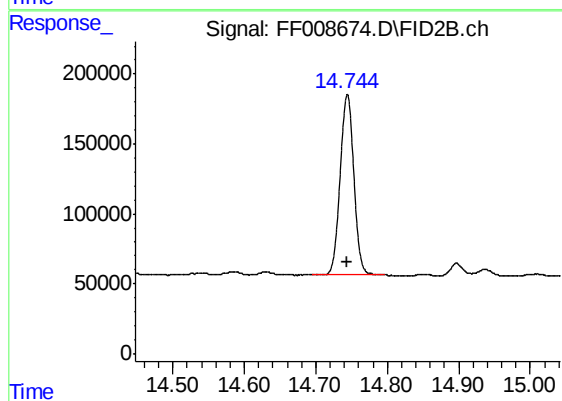

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.744 min
Delta R.T.: 0.000 min
Response: 1710699
Conc: 15.01 ug/ml

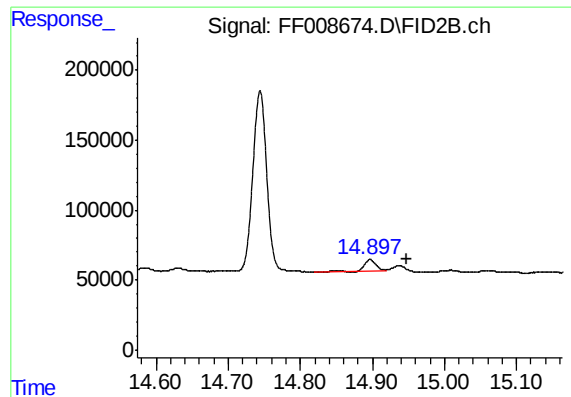

#10 N-TETRACOSANE

R.T.: 14.897 min
Delta R.T.: -0.051 min
Response: 76441
Conc: 0.58 ug/ml

Instrument :
FID_F
ClientSampleId :
PW-2R