

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF062821\  
 Data File : FF008677.D  
 Signal(s) : FID2B.ch  
 Acq On : 28 Jun 2021 22:42  
 Operator : DD\AJ  
 Sample : M2876-03  
 Misc :  
 ALS Vial : 75 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :  
 DW-3

Integration File: autoint1.e  
 Quant Time: Jun 29 01:45:59 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF062321.M  
 Quant Title :  
 QLast Update : Thu Jun 24 08:07:11 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.745 | 1960301  | 17.200 ug/ml |
| Target Compounds              |        |          |              |
| 2) N-DECANE                   | 4.501  | 131700   | 0.977 ug/ml  |
| 3) N-DODECANE                 | 6.517  | 589603   | 4.335 ug/ml  |
| 4) N-TETRADECANE              | 8.308  | 701408   | 5.199 ug/ml  |
| 5) N-HEXADECANE               | 9.905  | 514986   | 3.770 ug/ml  |
| 6) N-OCTADECANE               | 11.343 | 193931   | 1.393 ug/ml  |
| 7) N-EICOSANE                 | 12.649 | 80414    | 0.586 ug/ml  |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF062821\  
Data File : FF008677.D  
Signal(s) : FID2B.ch  
Acq On : 28 Jun 2021 22:42  
Operator : DD\AJ  
Sample : M2876-03  
Misc :  
ALS Vial : 75 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
DW-3

Integration File: autoint1.e  
Quant Time: Jun 29 01:45:59 2021  
Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF062321.M  
Quant Title :  
QLast Update : Thu Jun 24 08:07:11 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

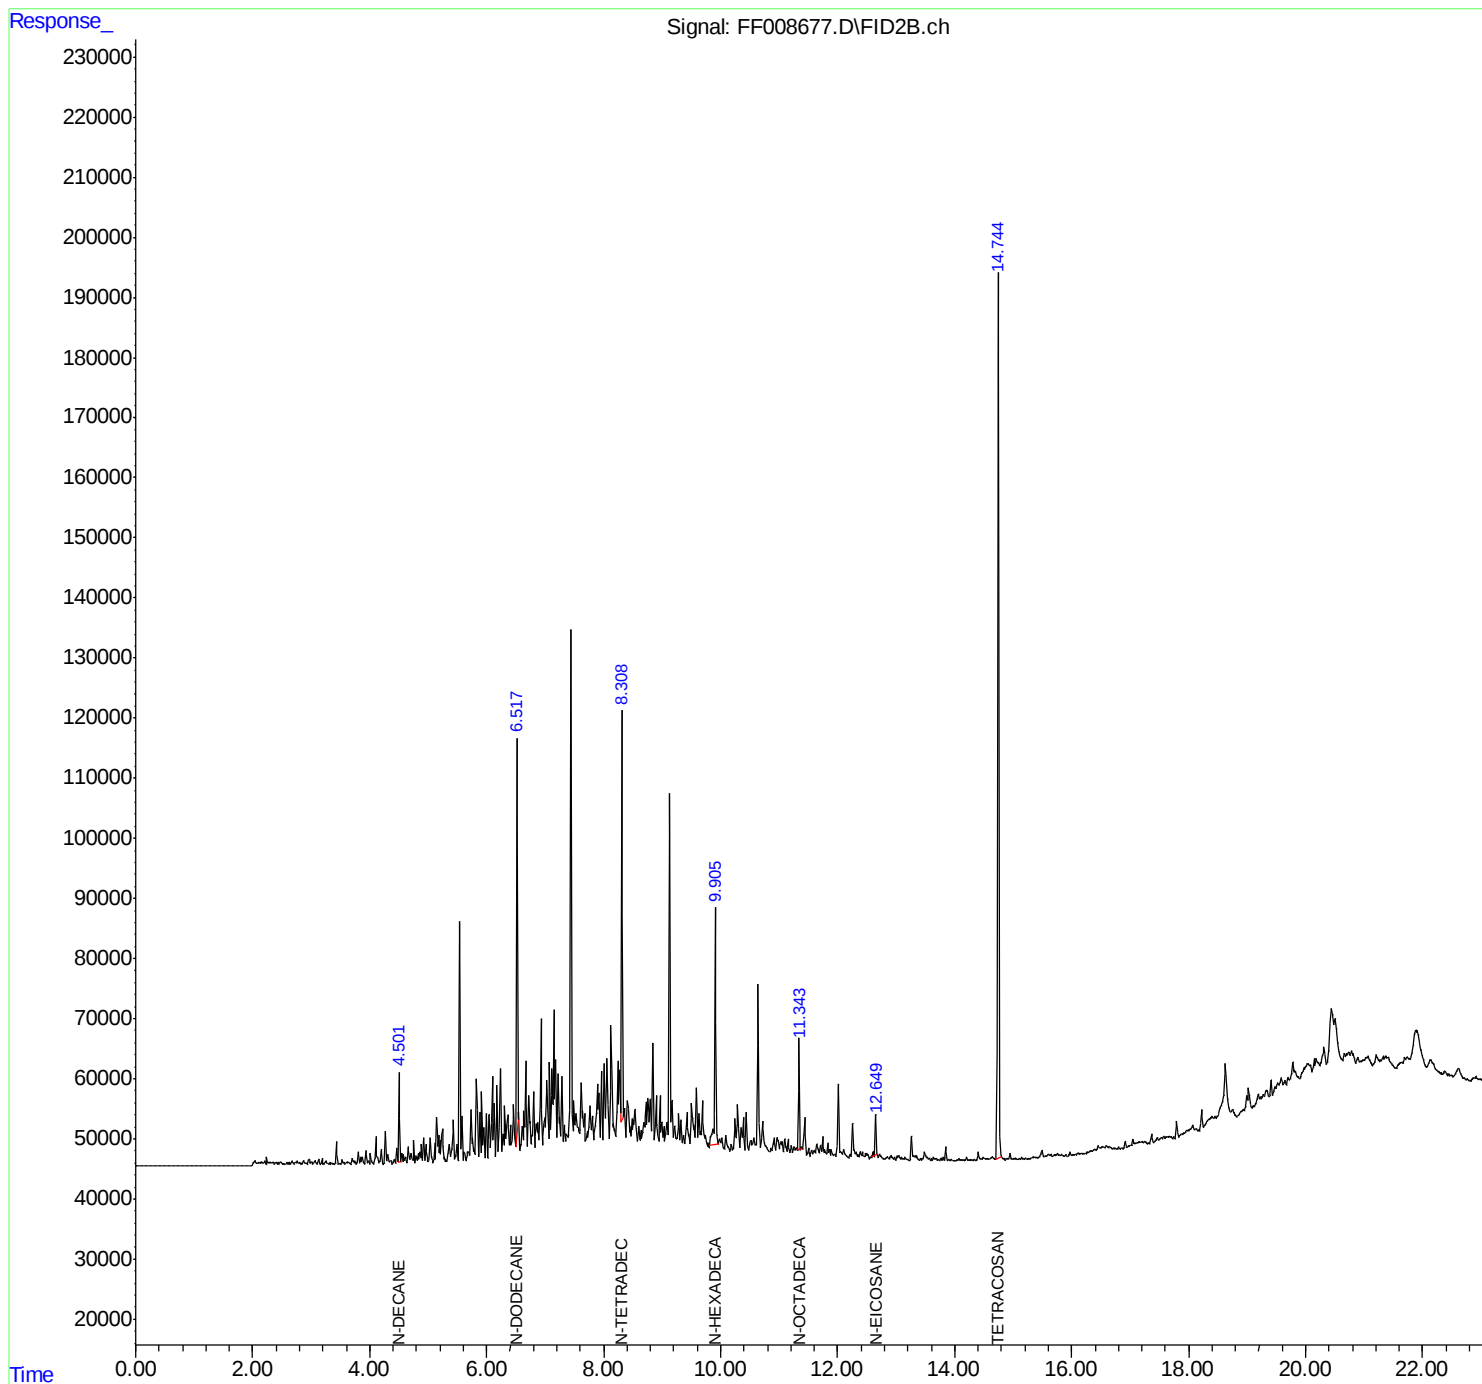


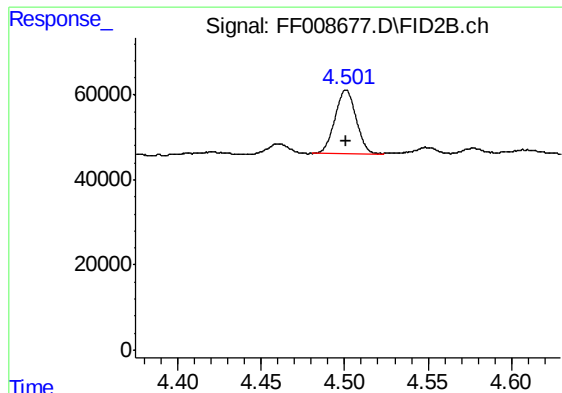

#2 N-DECANE


R.T.: 4.501 min  
Delta R.T.: 0.000 min  
Response: 131700  
Conc: 0.98 ug/ml

Instrument :  
FID\_F  
ClientSampleId :  
DW-3

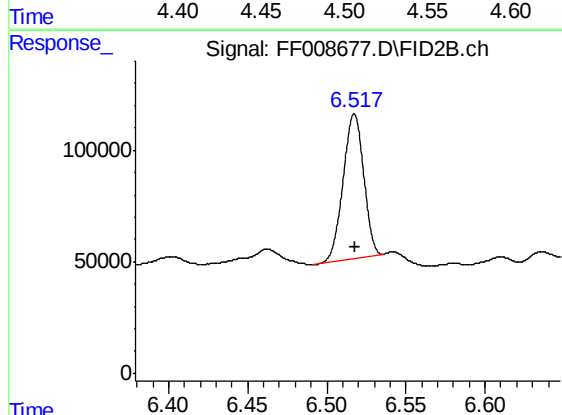


#3 N-DODECANE

R.T.: 6.517 min  
Delta R.T.: 0.000 min  
Response: 589603  
Conc: 4.34 ug/ml

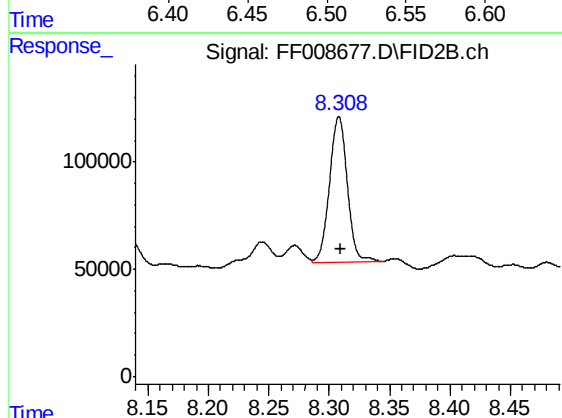


#4 N-TETRADECANE

R.T.: 8.308 min  
Delta R.T.: -0.002 min  
Response: 701408  
Conc: 5.20 ug/ml

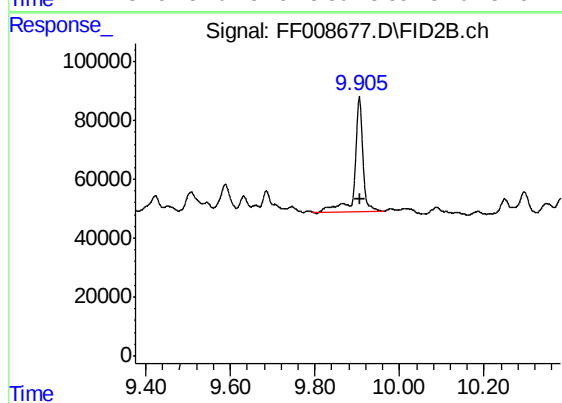

#5 N-HEXADECANE


R.T.: 9.905 min  
Delta R.T.: -0.001 min  
Response: 514986  
Conc: 3.77 ug/ml

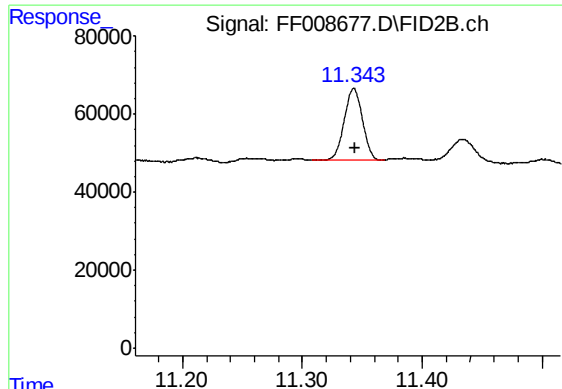

#6 N-OCTADECANE


R.T.: 11.343 min  
Delta R.T.: -0.001 min  
Response: 193931  
Conc: 1.39 ug/ml

Instrument :  
FID\_F  
ClientSampleId :  
DW-3

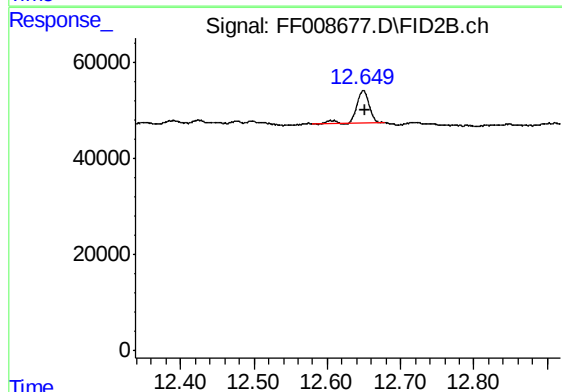

#7 N-EICOSANE

R.T.: 12.649 min  
Delta R.T.: -0.002 min  
Response: 80414  
Conc: 0.59 ug/ml

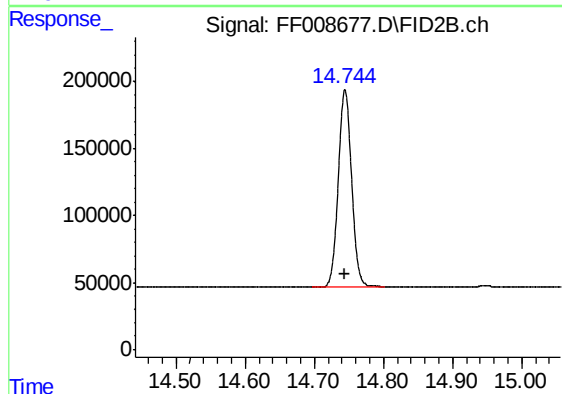

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.745 min  
Delta R.T.: 0.000 min  
Response: 1960301  
Conc: 17.20 ug/ml