

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062822\
Data File : FF010904.D
Signal(s) : FID2B.ch
Acq On : 28 Jun 2022 06:27
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 29 01:08:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.550	2487343	20.467 ug/ml
12) N-OCTACOSANE	16.998	2236834	18.329 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062822\
Data File : FF010904.D
Signal(s) : FID2B.ch
Acq On : 28 Jun 2022 06:27
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 29 01:08:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

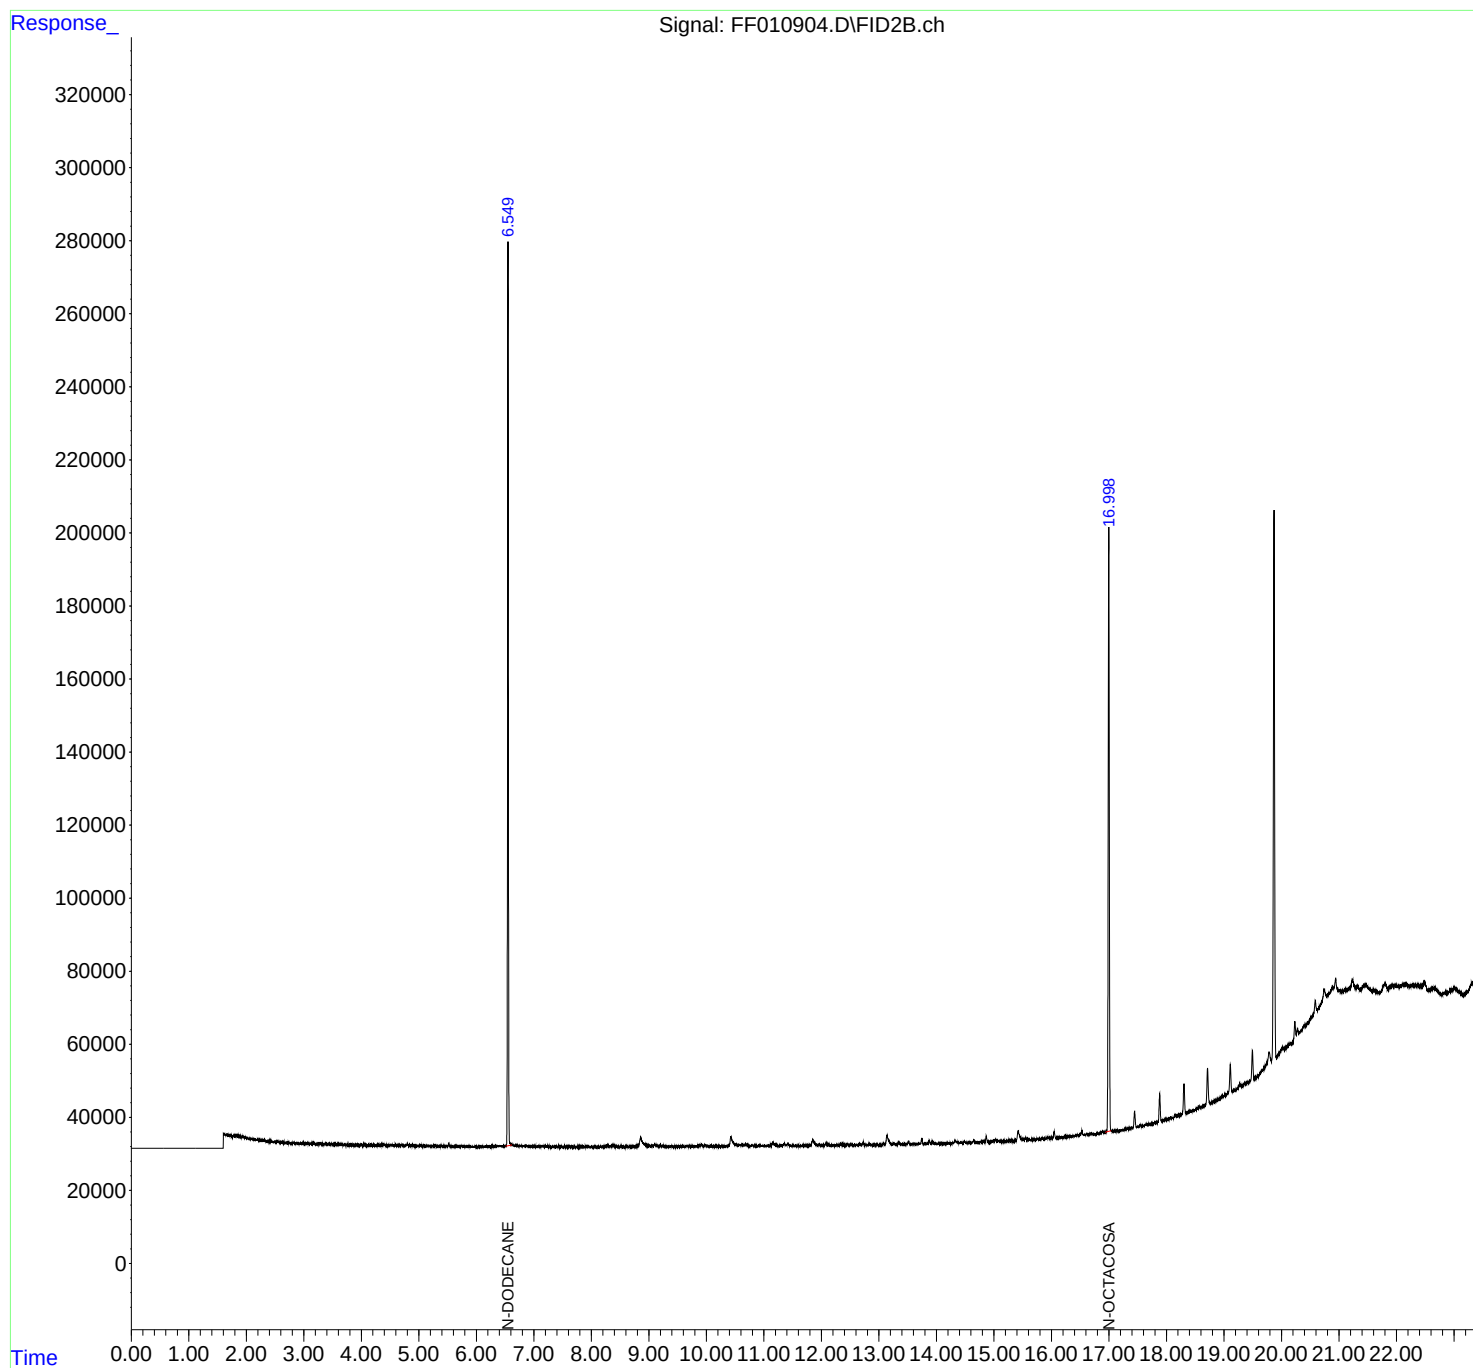


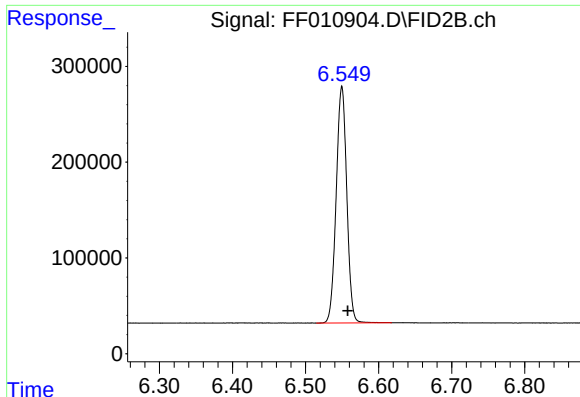

#3 N-DODECANE


R.T.: 6.550 min
Delta R.T.: -0.008 min
Response: 2487343
Conc: 20.47 ug/ml

Instrument :
FID_F
ClientSampleId :

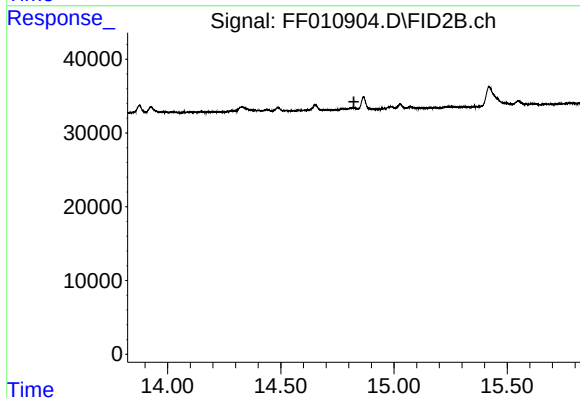

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.823 min
Response: 0
Conc: N.D.

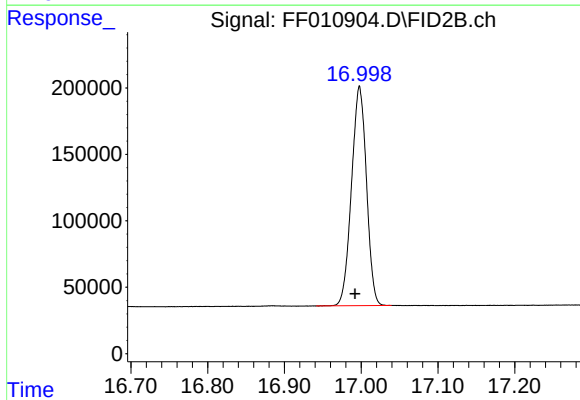

#12 N-OCTACOSANE

R.T.: 16.998 min
Delta R.T.: 0.006 min
Response: 2236834
Conc: 18.33 ug/ml