

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062918\
 Data File : FF001152.D
 Signal(s) : FID2B.ch
 Acq On : 29 Jun 2018 14:58
 Operator : UA\AJ
 Sample : J3774-01
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 29 23:31:54 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.468	1679694	14.565 ug/ml
Target Compounds			
4) N-TETRADECANE	8.088	722962	5.193 ug/ml
5) N-HEXADECANE	9.628	176430	1.280 ug/ml
7) N-EICOSANE	12.420	3748763	27.981 ug/ml
8) N-DOCOSANE	13.577	304843	2.305 ug/ml
10) N-TETRACOSANE	14.633f	1690792	13.035 ug/ml
12) N-OCTACOSANE	16.633	500666	3.937 ug/ml
13) N-TRIACONTANE	17.523	310364	2.458 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062918\
Data File : FF001152.D
Signal(s) : FID2B.ch
Acq On : 29 Jun 2018 14:58
Operator : UA\AJ
Sample : J3774-01
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 29 23:31:54 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

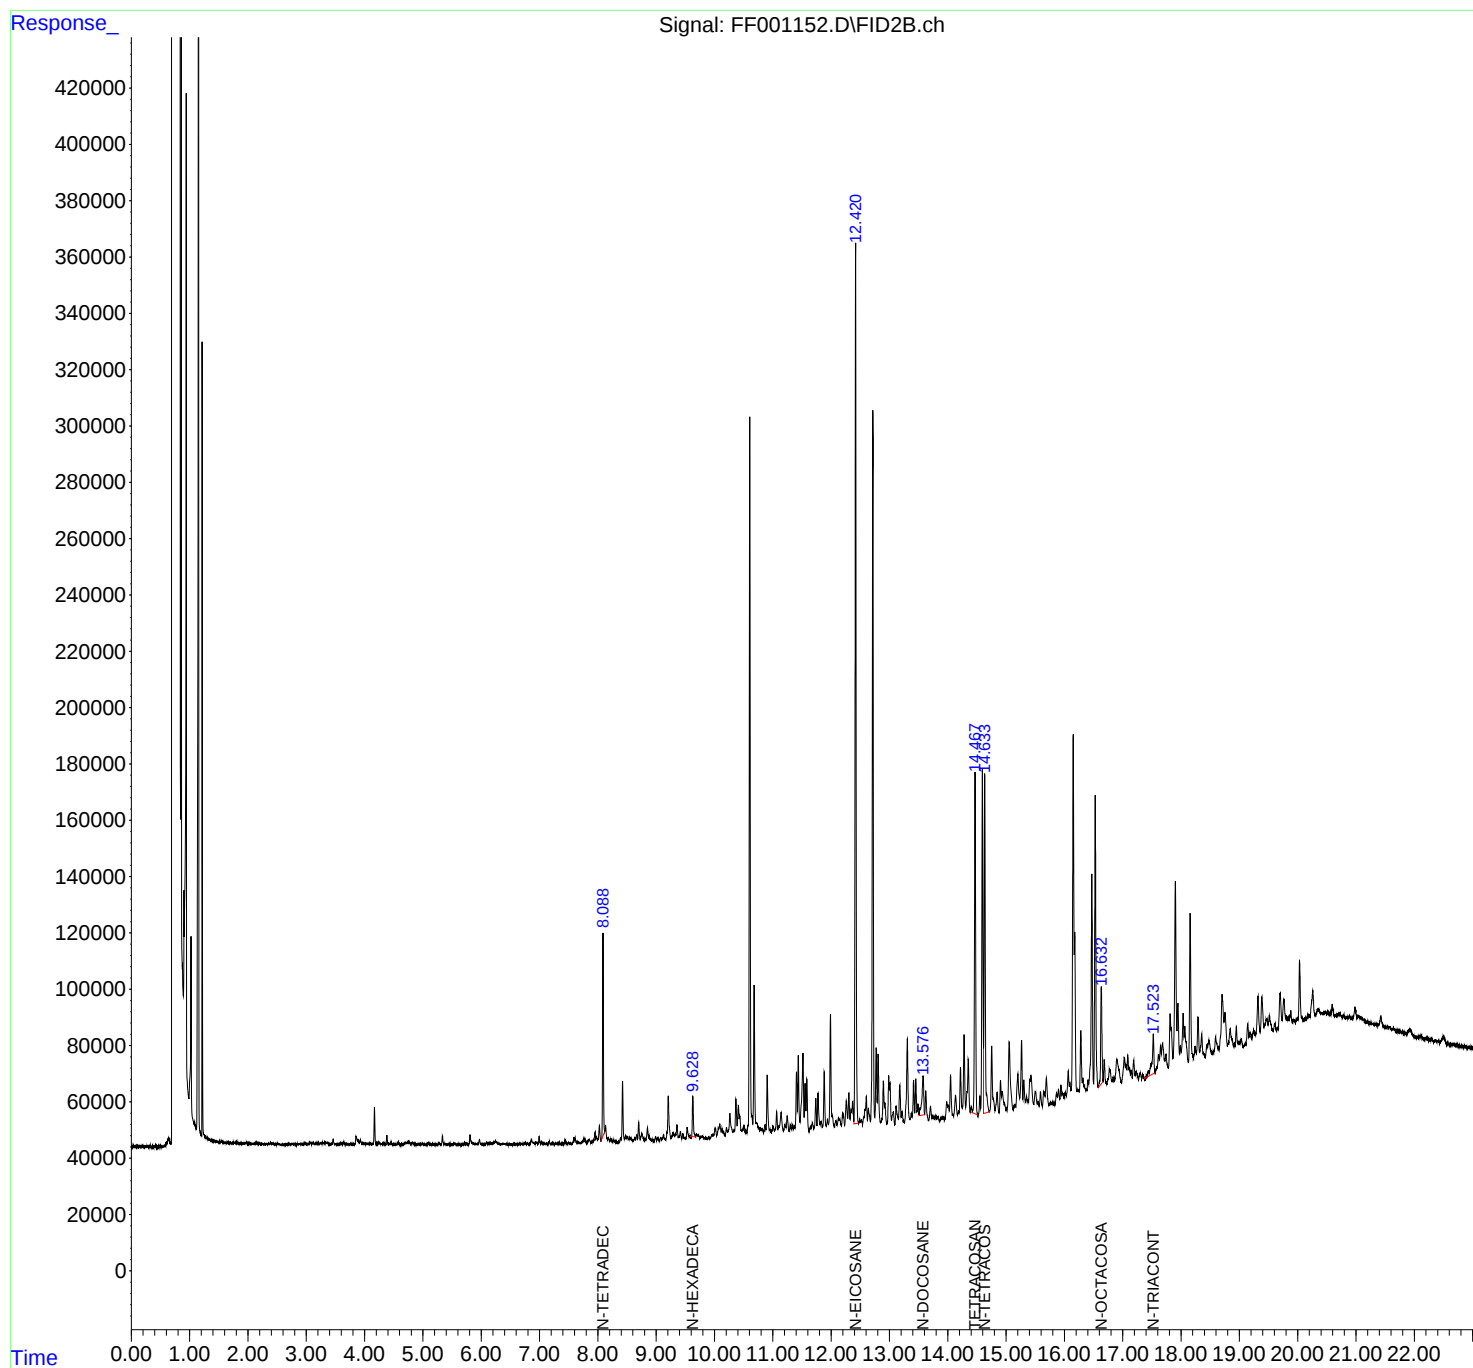


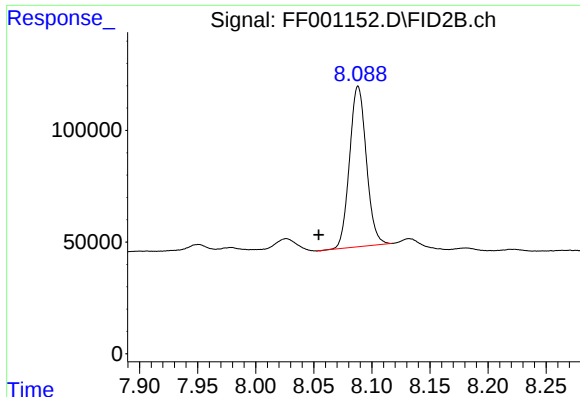

#4 N-TETRADECANE


R.T.: 8.088 min
Delta R.T.: 0.034 min
Response: 722962
Conc: 5.19 ug/ml

Instrument :
FID_F
ClientSampleId :

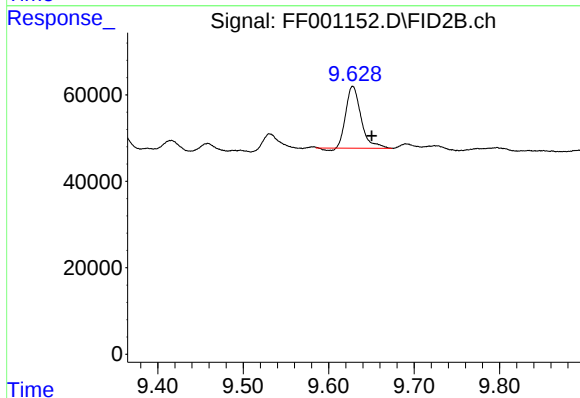


#5 N-HEXADECANE

R.T.: 9.628 min
Delta R.T.: -0.022 min
Response: 176430
Conc: 1.28 ug/ml

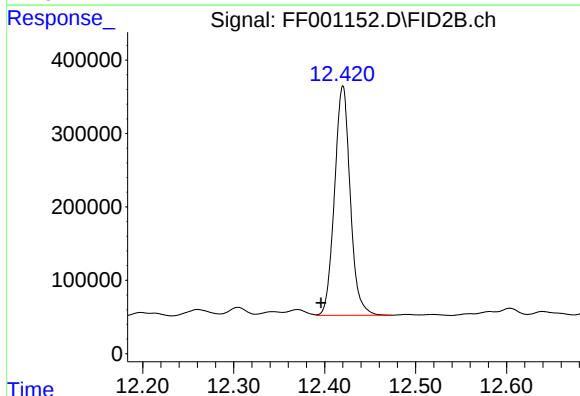


#7 N-EICOSANE

R.T.: 12.420 min
Delta R.T.: 0.024 min
Response: 3748763
Conc: 27.98 ug/ml

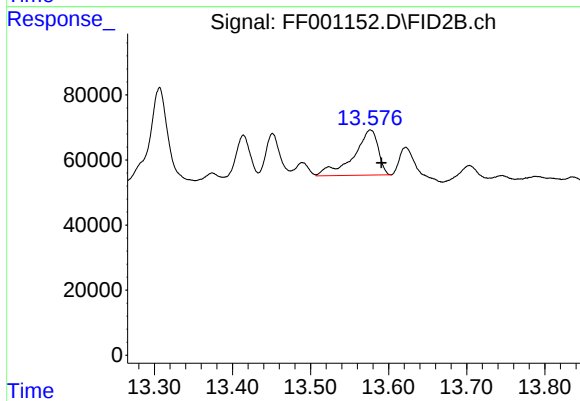

#8 N-DOCOSANE


R.T.: 13.577 min
Delta R.T.: -0.014 min
Response: 304843
Conc: 2.31 ug/ml

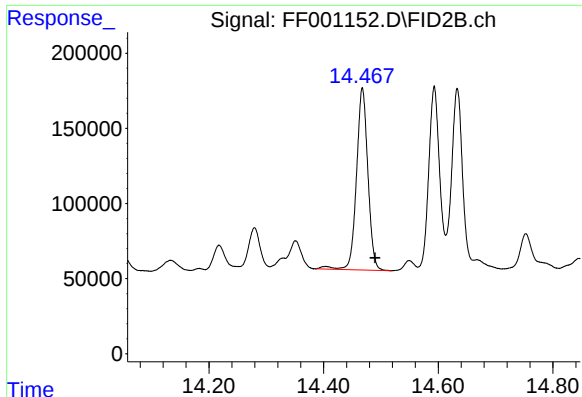

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.468 min
Delta R.T.: -0.022 min
Response: 1679694
Conc: 14.56 ug/ml

Instrument :
FID_F
ClientSampleId :

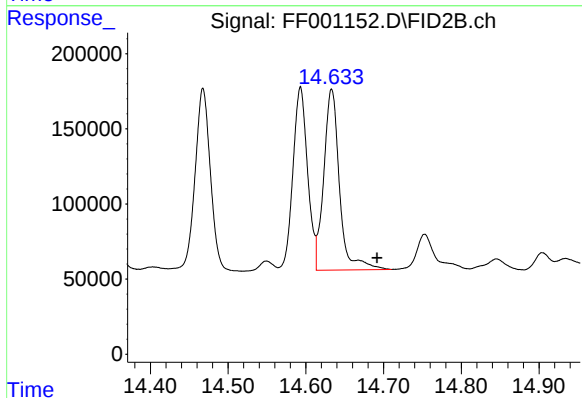


#10 N-TETRACOSANE

R.T.: 14.633 min
Delta R.T.: -0.058 min
Response: 1690792
Conc: 13.04 ug/ml

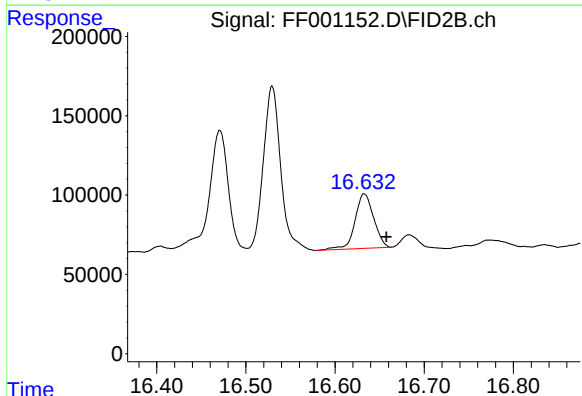

#12 N-OCTACOSANE

R.T.: 16.633 min
Delta R.T.: -0.025 min
Response: 500666
Conc: 3.94 ug/ml

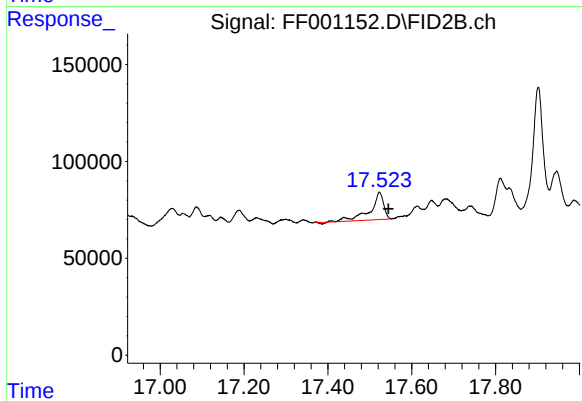

#13 N-TRIACONTANE

R.T.: 17.523 min
Delta R.T.: -0.021 min
Response: 310364
Conc: 2.46 ug/ml