

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062918\
Data File : FF001155.D
Signal(s) : FID2B.ch
Acq On : 29 Jun 2018 16:39
Operator : UA\AJ
Sample : J3774-03
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 29 23:32:43 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.467	1501099	13.016 ug/ml
Target Compounds			
4) N-TETRADECANE	8.089	684409	4.916 ug/ml
7) N-EICOSANE	12.420	424385	3.168 ug/ml
10) N-TETRACOSANE	14.635f	193238	1.490 ug/ml
12) N-OCTACOSANE	16.637	186625	1.468 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062918\
Data File : FF001155.D
Signal(s) : FID2B.ch
Acq On : 29 Jun 2018 16:39
Operator : UA\AJ
Sample : J3774-03
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 29 23:32:43 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

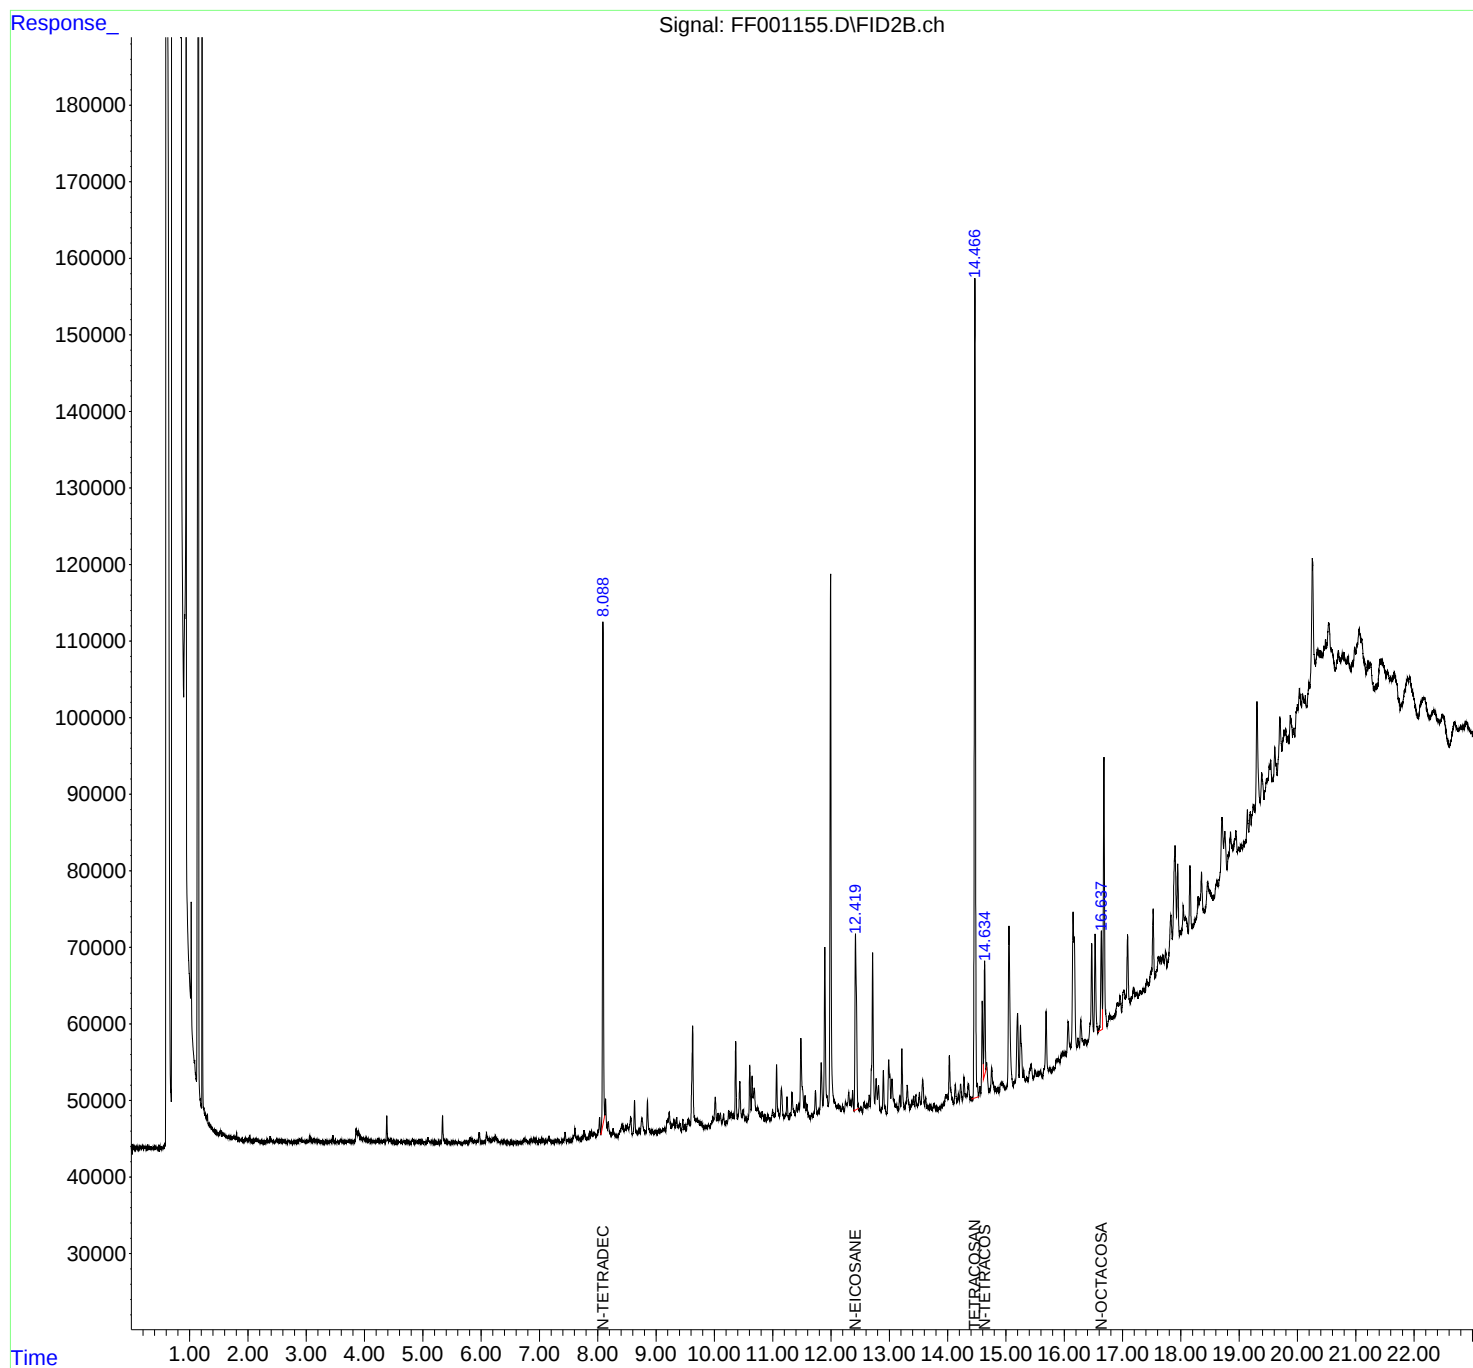


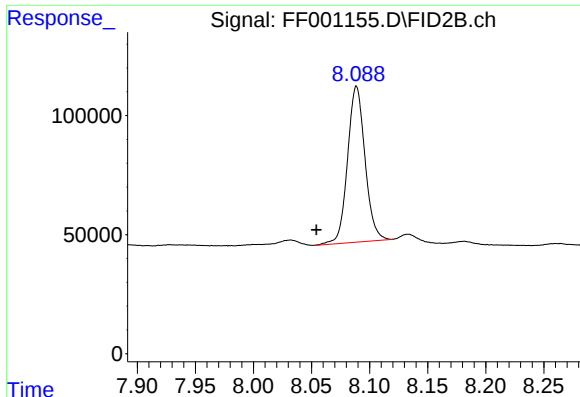

#4 N-TETRADECANE


R.T.: 8.089 min
Delta R.T.: 0.035 min
Response: 684409
Conc: 4.92 ug/ml

Instrument :
FID_F
ClientSampleId :

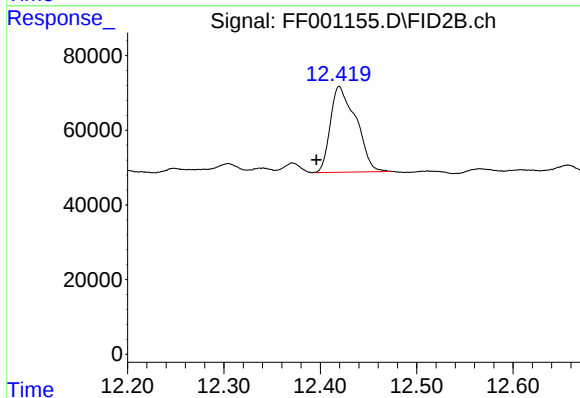


#7 N-EICOSANE

R.T.: 12.420 min
Delta R.T.: 0.024 min
Response: 424385
Conc: 3.17 ug/ml

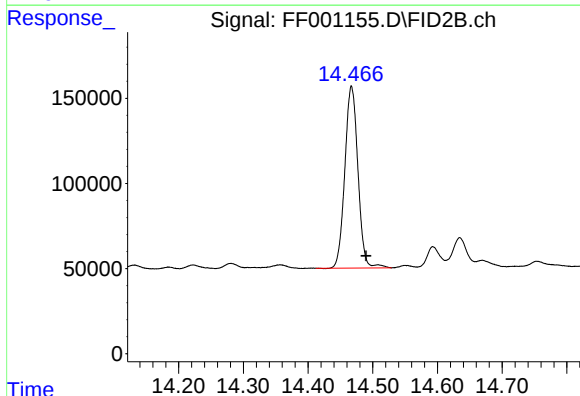


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.467 min
Delta R.T.: -0.023 min
Response: 1501099
Conc: 13.02 ug/ml

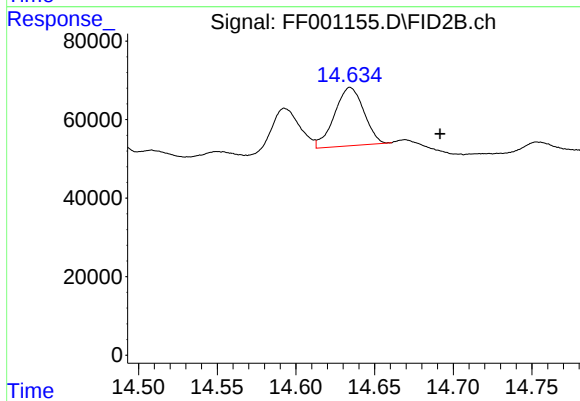

#10 N-TETRACOSANE

R.T.: 14.635 min
Delta R.T.: -0.057 min
Response: 193238
Conc: 1.49 ug/ml

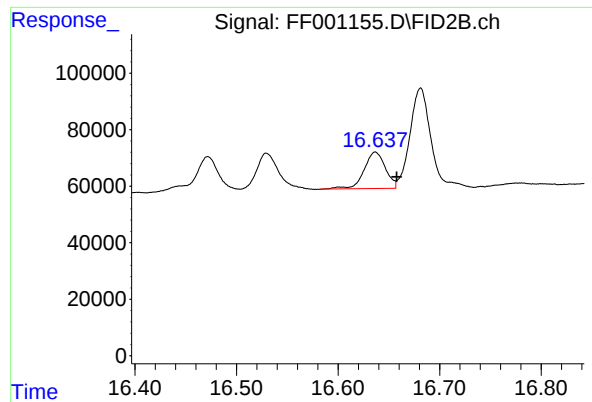

#12 N-OCTACOSANE

R.T.: 16.637 min
Delta R.T.: -0.021 min
Response: 186625
Conc: 1.47 ug/ml

Instrument :
FID_F
ClientSampleId :