

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG062918\  
Data File : FG001516.D  
Signal(s) : FID1A.ch  
Acq On : 29 Jun 2018 08:54  
Operator : UA\AJ  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jun 29 23:58:28 2018  
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID\_G\Method\FG060118.M  
Quant Title :  
QLast Update : Fri Jun 01 15:28:31 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    |               | R.T.    | Response | Conc Units  |
|-----------------------------|---------------|---------|----------|-------------|
| -----                       |               |         |          |             |
| System Monitoring Compounds |               |         |          |             |
| Target Compounds            |               |         |          |             |
| 7)                          | N-EICOSANE    | 12.413  | 255469   | 1.814 ug/ml |
| 8)                          | N-DOCOSANE    | 13.621  | 232005   | 1.655 ug/ml |
| 10)                         | N-TETRACOSANE | 14.695f | 549293   | 3.950 ug/ml |
| -----                       |               |         |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG062918\  
Data File : FG001516.D  
Signal(s) : FID1A.ch  
Acq On : 29 Jun 2018 08:54  
Operator : UA\AJ  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jun 29 23:58:28 2018  
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID\_G\Method\FG060118.M  
Quant Title :  
QLast Update : Fri Jun 01 15:28:31 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

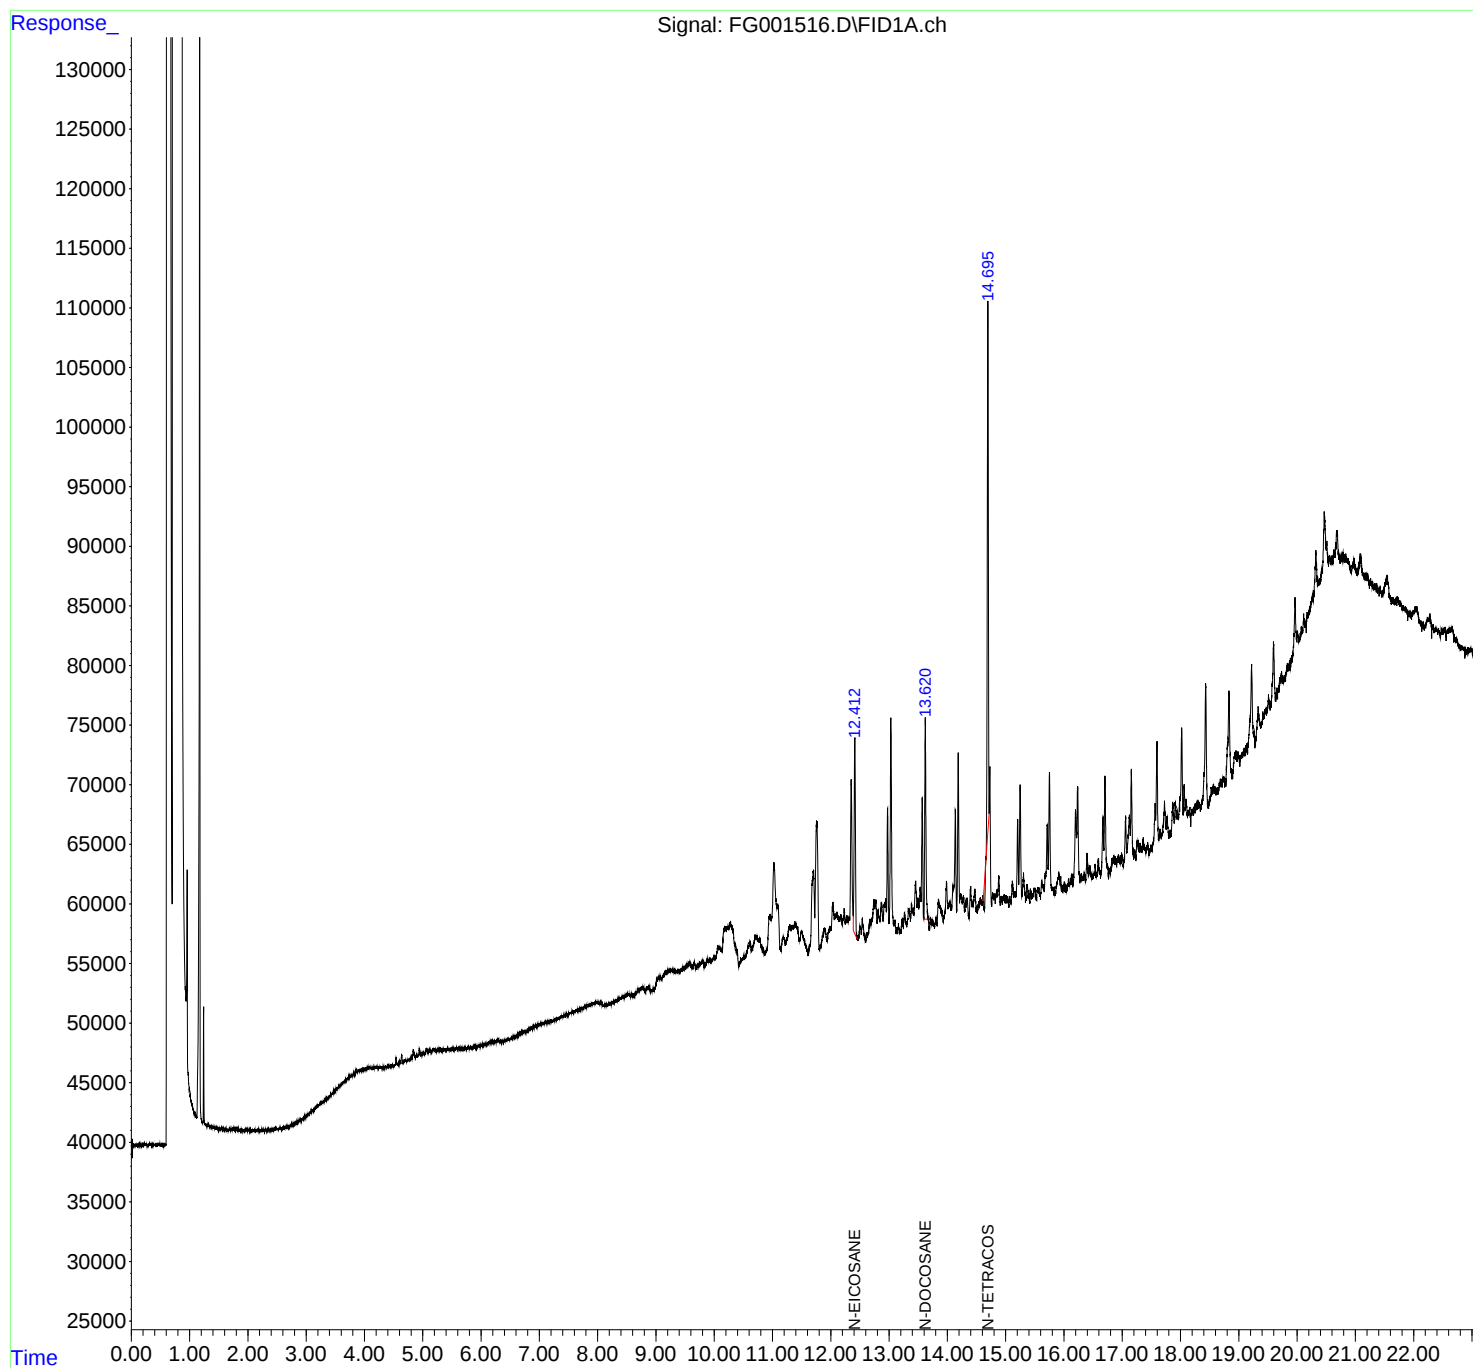


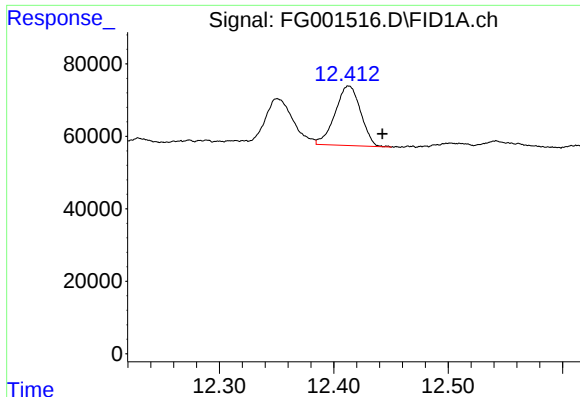

#7 N-EICOSANE


R.T.: 12.413 min  
Delta R.T.: -0.029 min  
Response: 255469  
Conc: 1.81 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

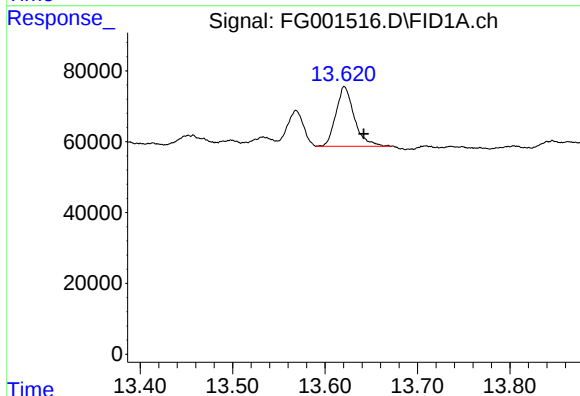


#8 N-DOCOSANE

R.T.: 13.621 min  
Delta R.T.: -0.021 min  
Response: 232005  
Conc: 1.66 ug/ml

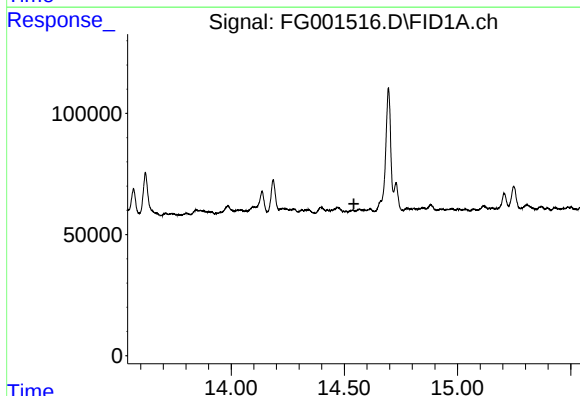

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T. : 14.542 min  
Response: 0  
Conc: N.D.

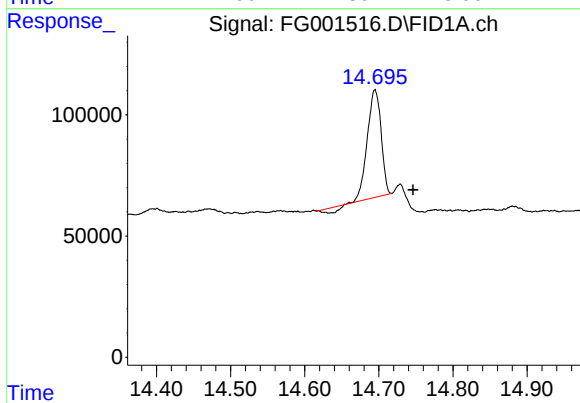

#10 N-TETRACOSANE

R.T.: 14.695 min  
Delta R.T.: -0.051 min  
Response: 549293  
Conc: 3.95 ug/ml