

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF063018\
 Data File : FF001161.D
 Signal(s) : FID2B.ch
 Acq On : 30 Jun 2018 08:58
 Operator : UA\AJ
 Sample : J3774-01
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 02 00:56:48 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.464	1765960	15.313 ug/ml
Target Compounds			
4) N-TETRADECANE	8.085	843423	6.058 ug/ml
5) N-HEXADECANE	9.626	195549	1.418 ug/ml
7) N-EICOSANE	12.417	3955312	29.522 ug/ml
8) N-DOCOSANE	13.573	323309	2.445 ug/ml
10) N-TETRACOSANE	14.750f	394657	3.043 ug/ml
12) N-OCTACOSANE	16.629	518918	4.081 ug/ml
13) N-TRIACONTANE	17.520	283426	2.245 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF063018\
Data File : FF001161.D
Signal(s) : FID2B.ch
Acq On : 30 Jun 2018 08:58
Operator : UA\AJ
Sample : J3774-01
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 02 00:56:48 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

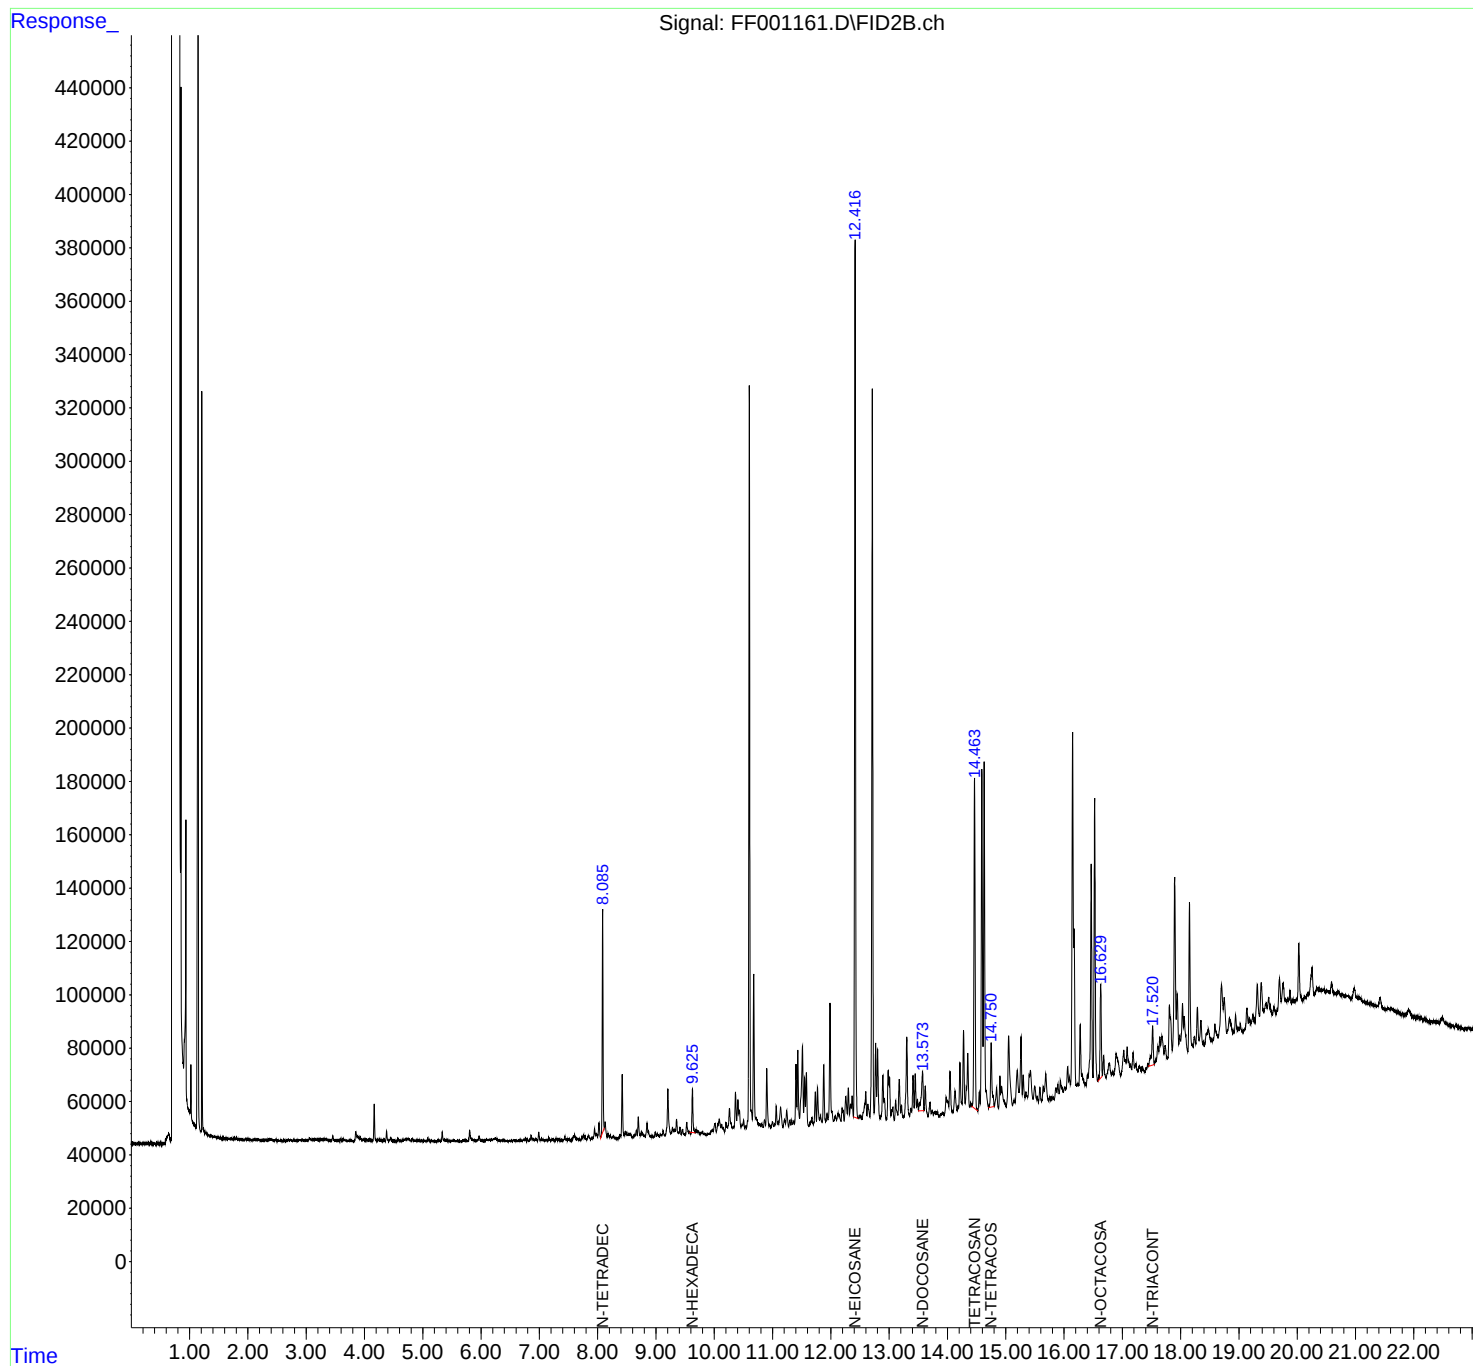


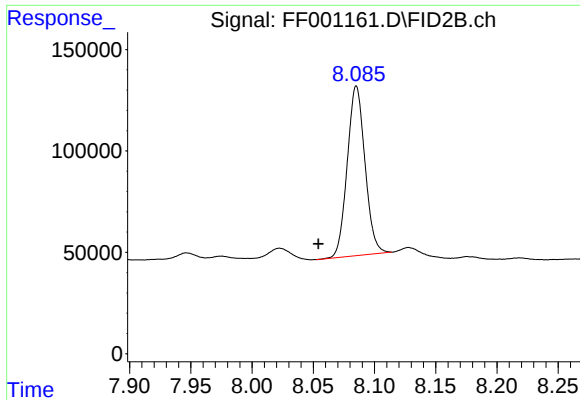

#4 N-TETRADECANE


R.T.: 8.085 min
Delta R.T.: 0.031 min
Response: 843423
Conc: 6.06 ug/ml

Instrument :
FID_F
ClientSampleId :

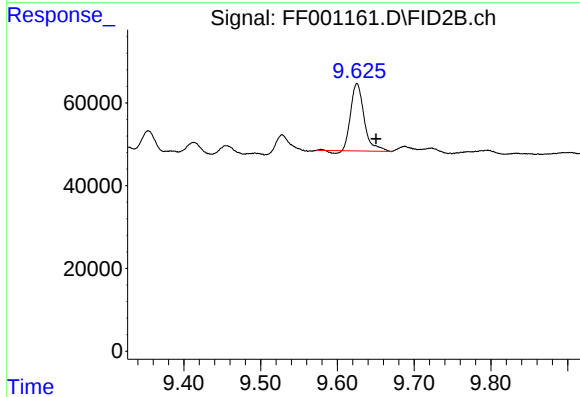


#5 N-HEXADECANE

R.T.: 9.626 min
Delta R.T.: -0.025 min
Response: 195549
Conc: 1.42 ug/ml

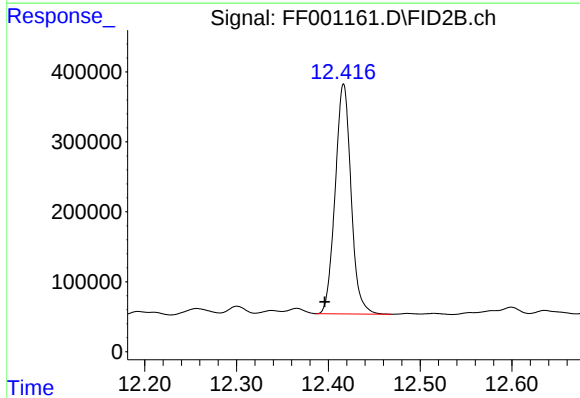


#7 N-EICOSANE

R.T.: 12.417 min
Delta R.T.: 0.021 min
Response: 3955312
Conc: 29.52 ug/ml

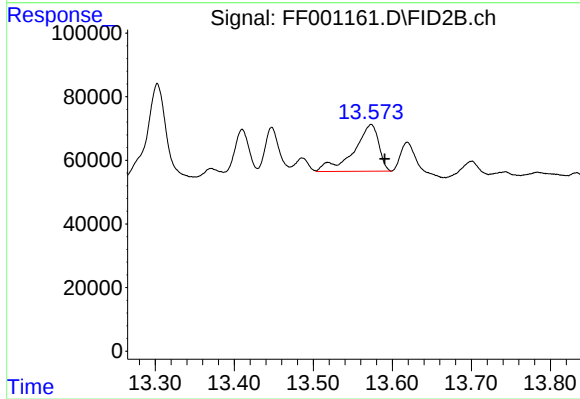

#8 N-DOCOSANE


R.T.: 13.573 min
Delta R.T.: -0.017 min
Response: 323309
Conc: 2.45 ug/ml

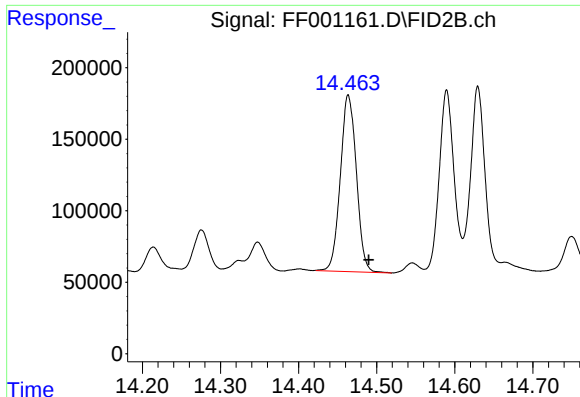

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.464 min
Delta R.T.: -0.026 min
Response: 1765960
Conc: 15.31 ug/ml

Instrument :
FID_F
ClientSampleId :

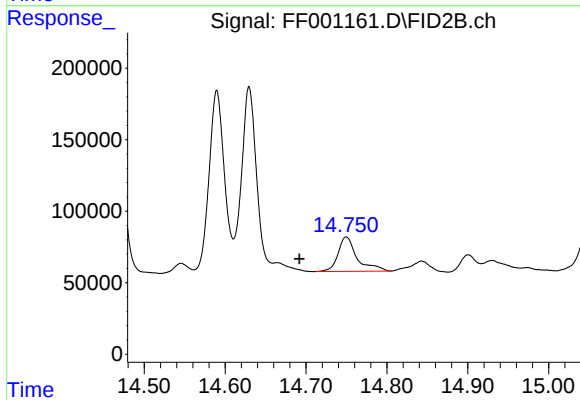


#10 N-TETRACOSANE

R.T.: 14.750 min
Delta R.T.: 0.058 min
Response: 394657
Conc: 3.04 ug/ml

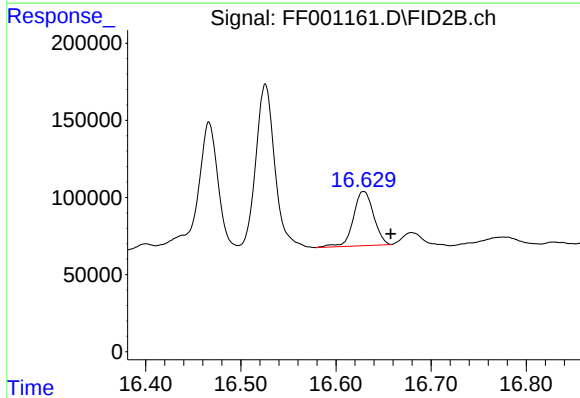

#12 N-OCTACOSANE

R.T.: 16.629 min
Delta R.T.: -0.029 min
Response: 518918
Conc: 4.08 ug/ml

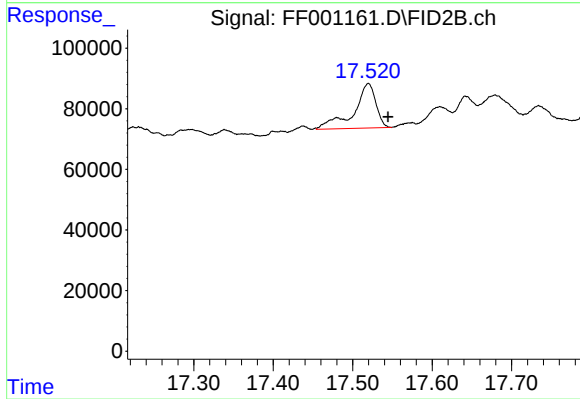

#13 N-TRIACONTANE

R.T.: 17.520 min
Delta R.T.: -0.025 min
Response: 283426
Conc: 2.24 ug/ml