

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF063018\
Data File : FF001164.D
Signal(s) : FID2B.ch
Acq On : 30 Jun 2018 10:28
Operator : UA\AJ
Sample : J3774-03
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 02 00:57:54 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.466	1634456	14.173 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.088	742635	5.334 ug/ml
5)	N-HEXADECANE	9.626	212217	1.539 ug/ml
7)	N-EICOSANE	12.418	468046	3.493 ug/ml
10)	N-TETRACOSANE	14.632f	212812	1.641 ug/ml
12)	N-OCTACOSANE	16.678	546303	4.296 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF063018\
Data File : FF001164.D
Signal(s) : FID2B.ch
Acq On : 30 Jun 2018 10:28
Operator : UA\AJ
Sample : J3774-03
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 02 00:57:54 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

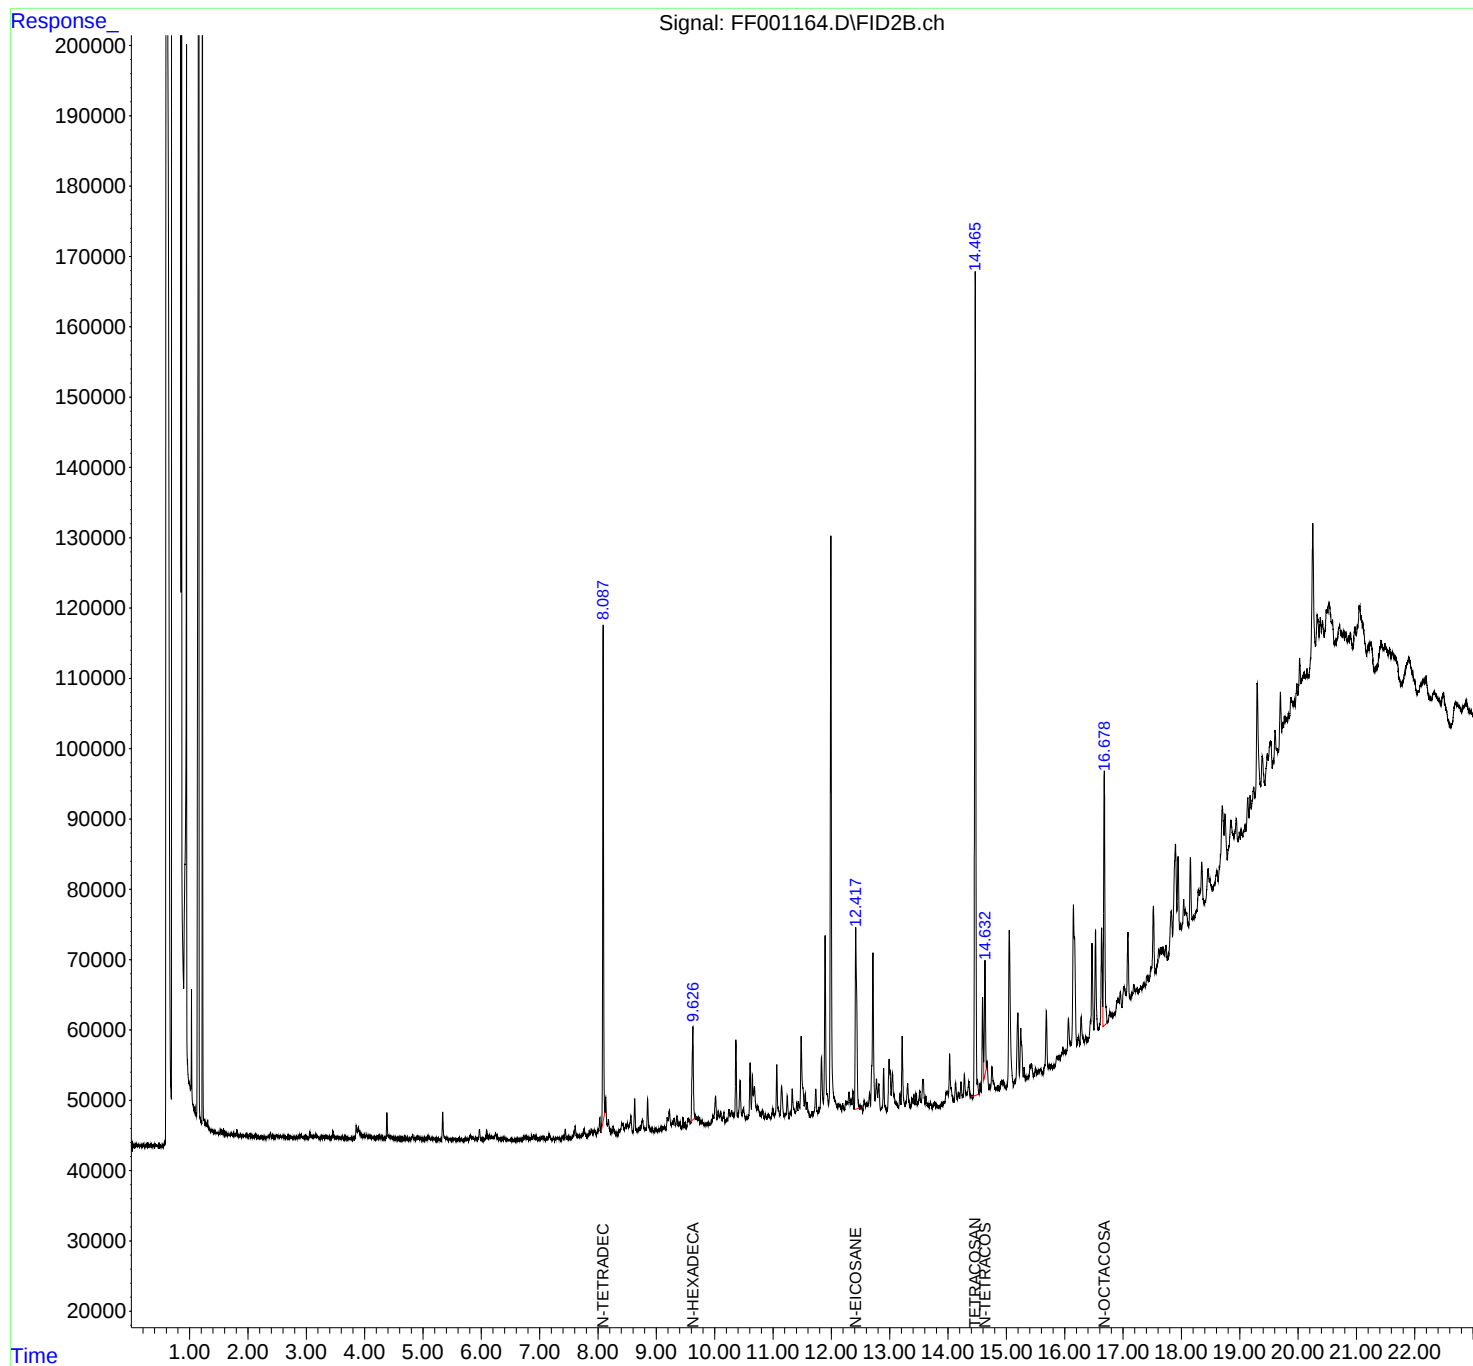


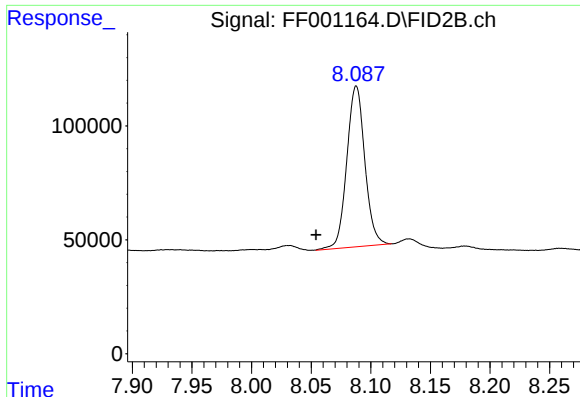

#4 N-TETRADECANE


R.T.: 8.088 min
Delta R.T.: 0.034 min
Response: 742635
Conc: 5.33 ug/ml

Instrument :
FID_F
ClientSampleId :

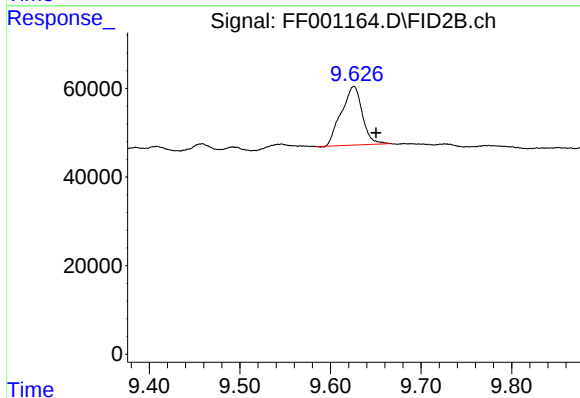


#5 N-HEXADECANE

R.T.: 9.626 min
Delta R.T.: -0.024 min
Response: 212217
Conc: 1.54 ug/ml

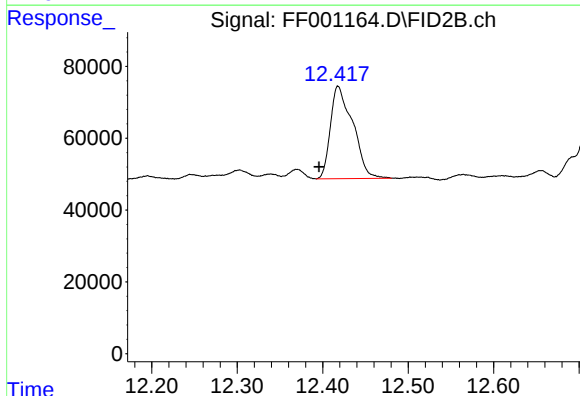


#7 N-EICOSANE

R.T.: 12.418 min
Delta R.T.: 0.022 min
Response: 468046
Conc: 3.49 ug/ml

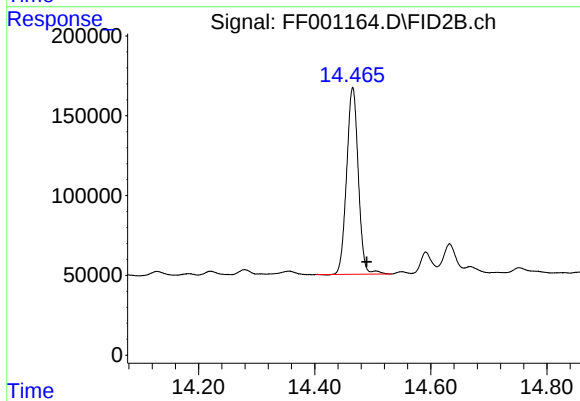

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.466 min
Delta R.T.: -0.024 min
Response: 1634456
Conc: 14.17 ug/ml

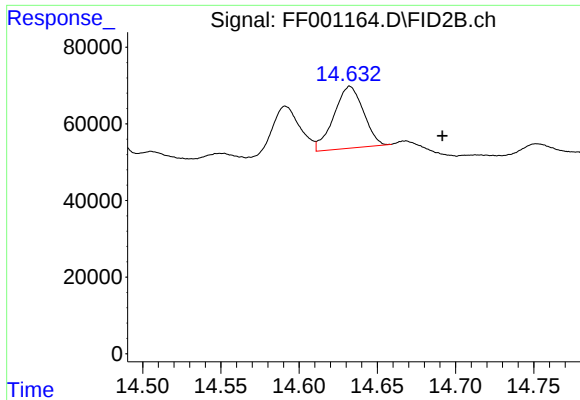

#10 N-TETRACOSANE

R.T.: 14.632 min
Delta R.T.: -0.059 min
Response: 212812
Conc: 1.64 ug/ml

Instrument :
FID_F
ClientSampleId :

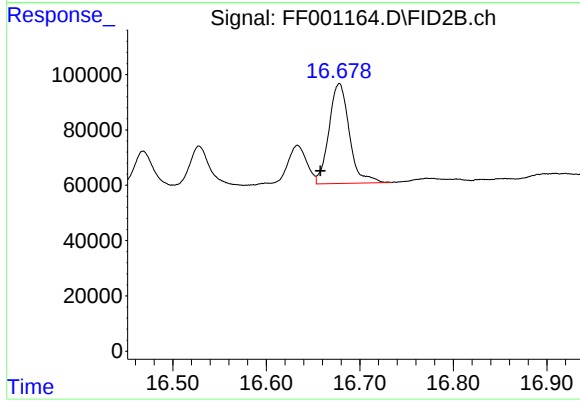

#12 N-OCTACOSANE

R.T.: 16.678 min
Delta R.T.: 0.020 min
Response: 546303
Conc: 4.30 ug/ml