

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF063018\
 Data File : FF001165.D
 Signal(s) : FID2B.ch
 Acq On : 30 Jun 2018 10:58
 Operator : UA\AJ
 Sample : J3774-06
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 02 00:58:07 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.465	1582962	13.726 ug/ml
Target Compounds			
4) N-TETRADECANE	8.088	717403	5.153 ug/ml
7) N-EICOSANE	12.418	682053	5.091 ug/ml
8) N-DOCOSANE	13.576	344079	2.602 ug/ml
10) N-TETRACOSANE	14.751f	934247	7.203 ug/ml
12) N-OCTACOSANE	16.679	1269271	9.982 ug/ml
13) N-TRIACONTANE	17.521	220115	1.743 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF063018\
Data File : FF001165.D
Signal(s) : FID2B.ch
Acq On : 30 Jun 2018 10:58
Operator : UA\AJ
Sample : J3774-06
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 02 00:58:07 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

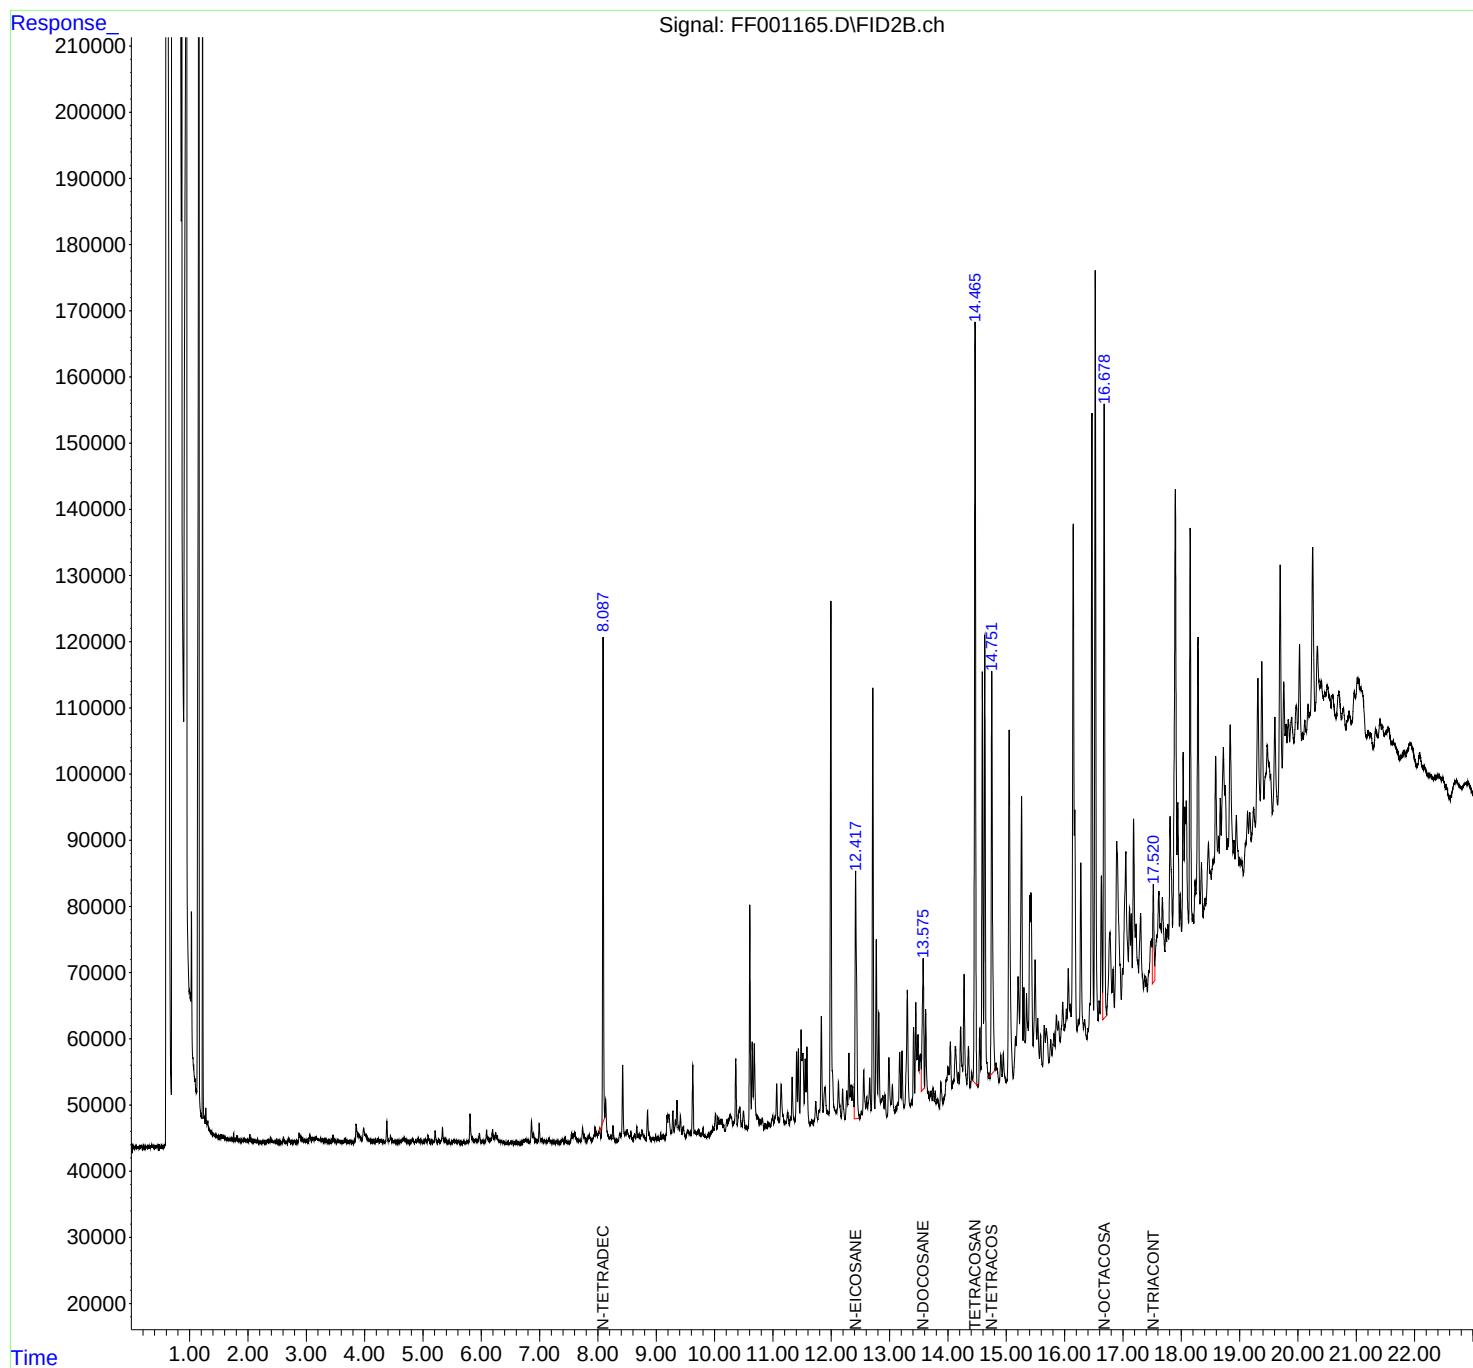


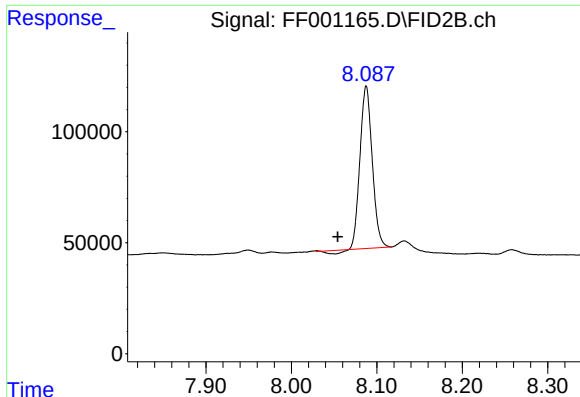

#4 N-TETRADECANE


R.T.: 8.088 min
Delta R.T.: 0.033 min
Response: 717403
Conc: 5.15 ug/ml

Instrument :
FID_F
ClientSampleId :

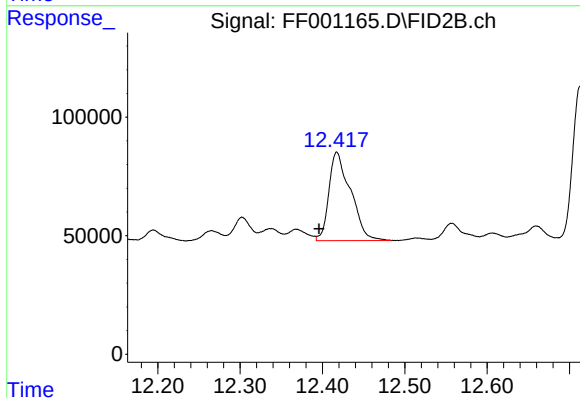


#7 N-EICOSANE

R.T.: 12.418 min
Delta R.T.: 0.022 min
Response: 682053
Conc: 5.09 ug/ml

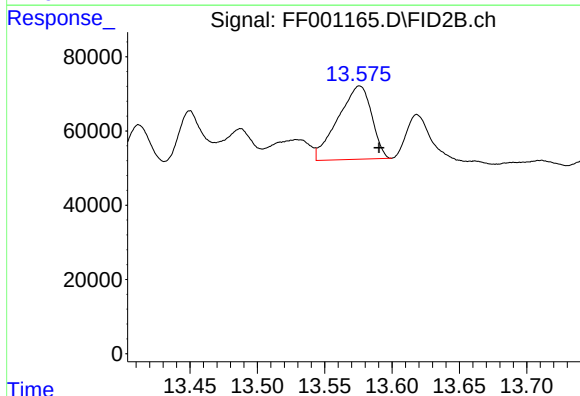


#8 N-DOCOSANE

R.T.: 13.576 min
Delta R.T.: -0.015 min
Response: 344079
Conc: 2.60 ug/ml

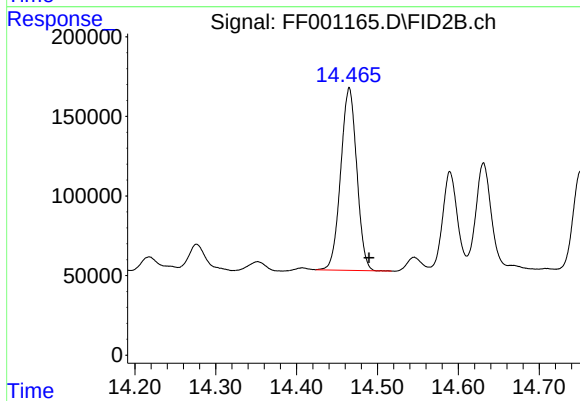

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.465 min
Delta R.T.: -0.025 min
Response: 1582962
Conc: 13.73 ug/ml

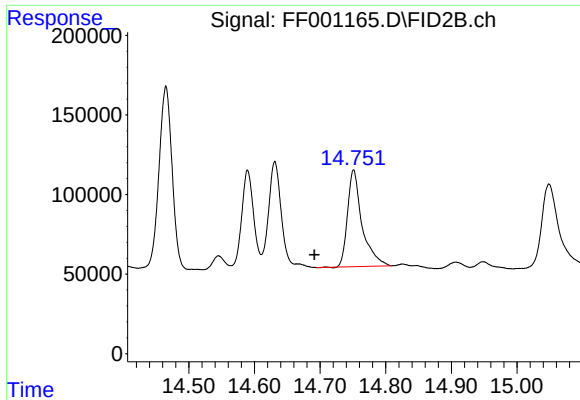

#10 N-TETRACOSANE


R.T.: 14.751 min
Delta R.T.: 0.059 min
Response: 934247
Conc: 7.20 ug/ml

Instrument :
FID_F
ClientSampleId :

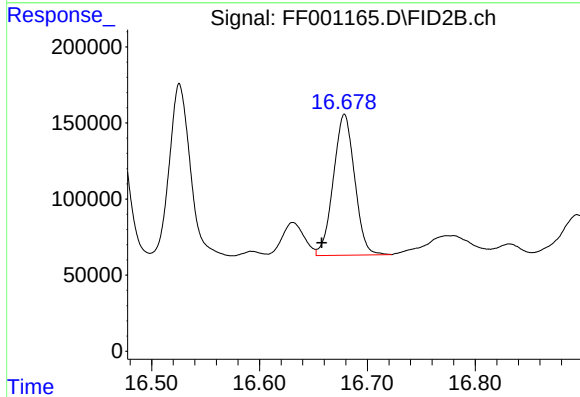

#12 N-OCTACOSANE

R.T.: 16.679 min
Delta R.T.: 0.021 min
Response: 1269271
Conc: 9.98 ug/ml

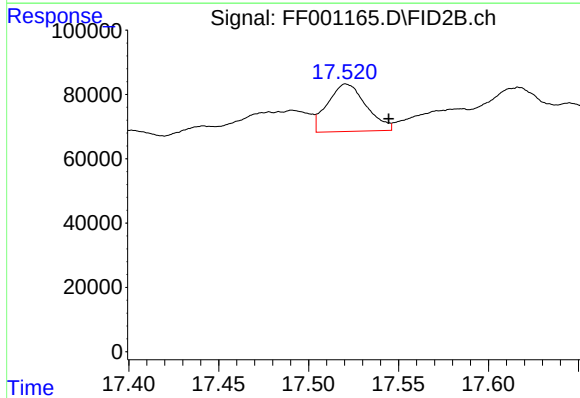

#13 N-TRIACONTANE

R.T.: 17.521 min
Delta R.T.: -0.024 min
Response: 220115
Conc: 1.74 ug/ml