

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF063018\
 Data File : FF001175.D
 Signal(s) : FID2B.ch
 Acq On : 30 Jun 2018 15:59
 Operator : UA\AJ
 Sample : J3248-07 10X
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 02 01:05:52 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.464	197863	1.716 ug/ml
Target Compounds			
5) N-HEXADECANE	9.626	301910	2.190 ug/ml
6) N-OCTADECANE	11.064	267265	1.957 ug/ml
7) N-EICOSANE	12.418	521135	3.890 ug/ml
8) N-DOCOSANE	13.572	69911	0.529 ug/ml
10) N-TETRACOSANE	14.633f	110305	0.850 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF063018\
Data File : FF001175.D
Signal(s) : FID2B.ch
Acq On : 30 Jun 2018 15:59
Operator : UA\AJ
Sample : J3248-07 10X
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 02 01:05:52 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

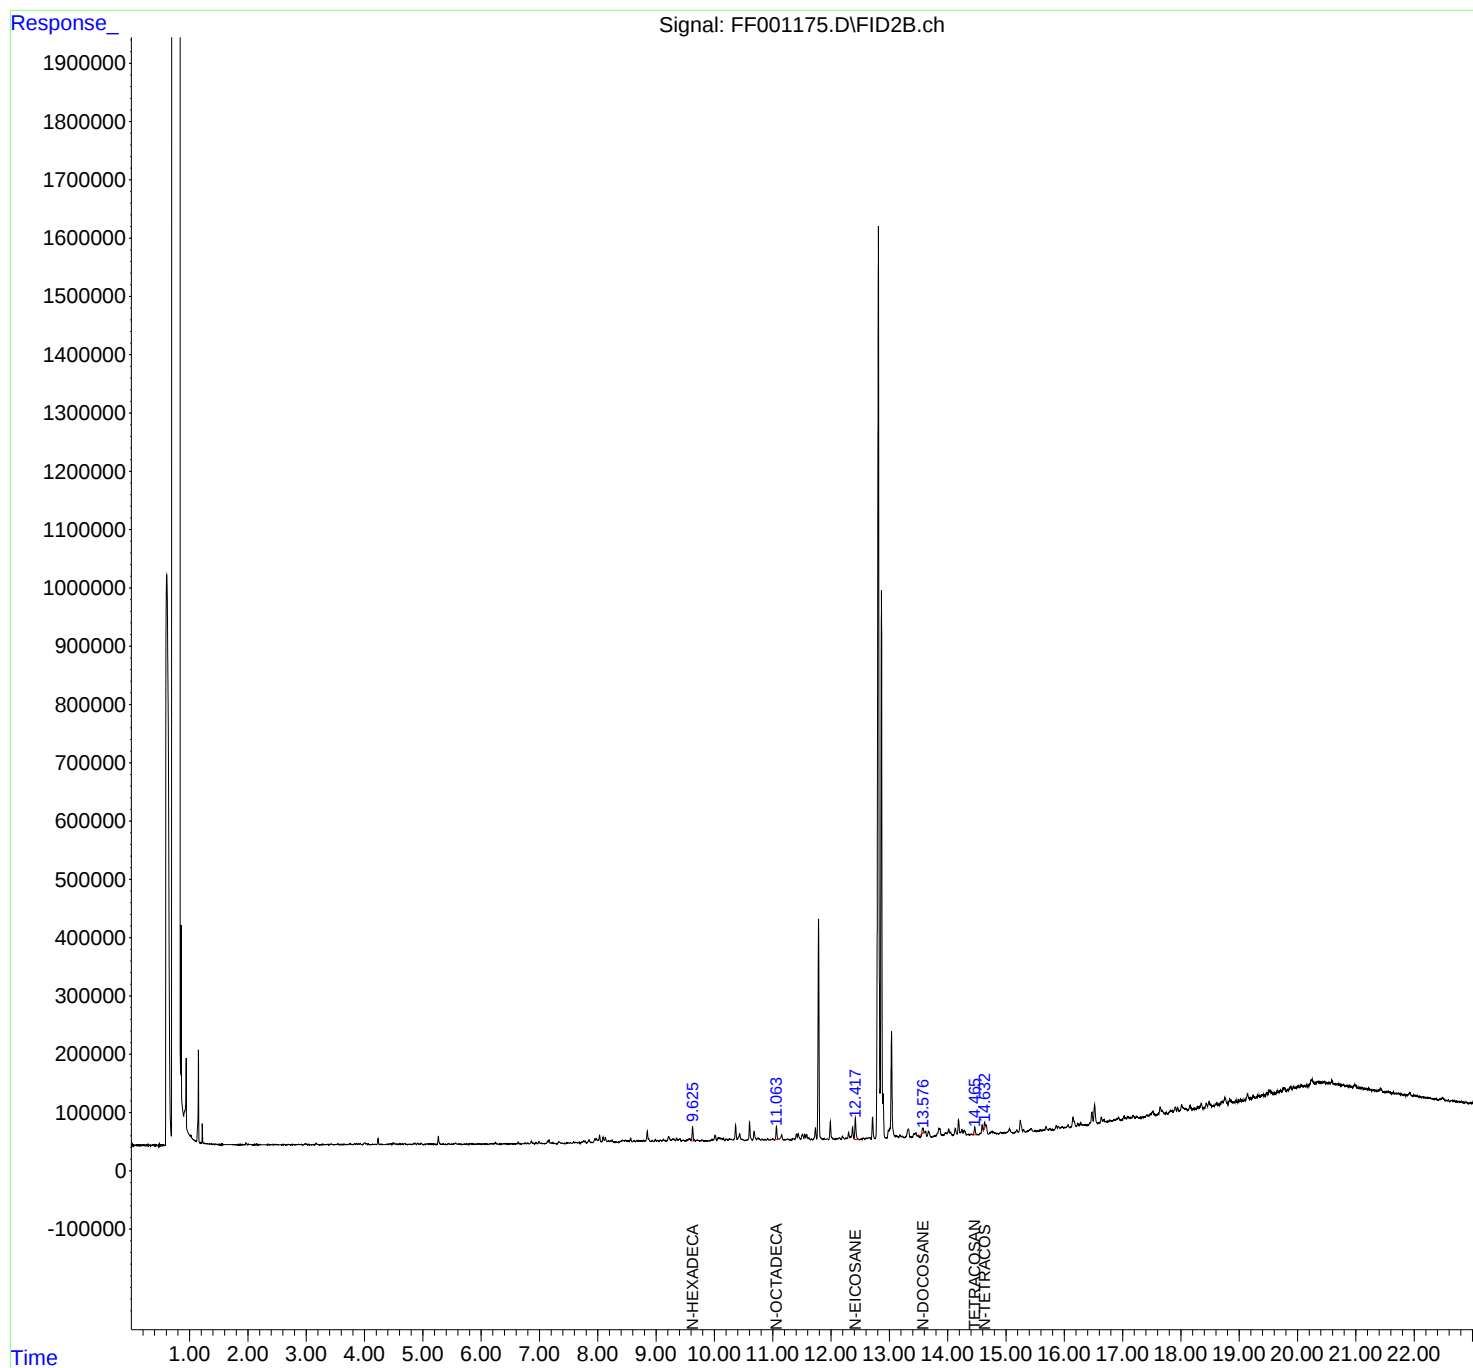


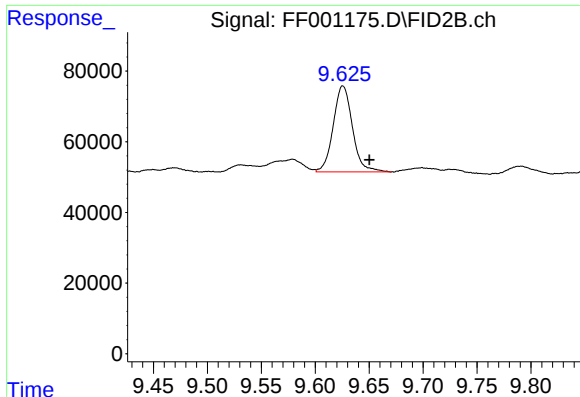

#5 N-HEXADECANE


R.T.: 9.626 min
Delta R.T.: -0.025 min
Response: 301910
Conc: 2.19 ug/ml

Instrument :
FID_F
ClientSampleId :

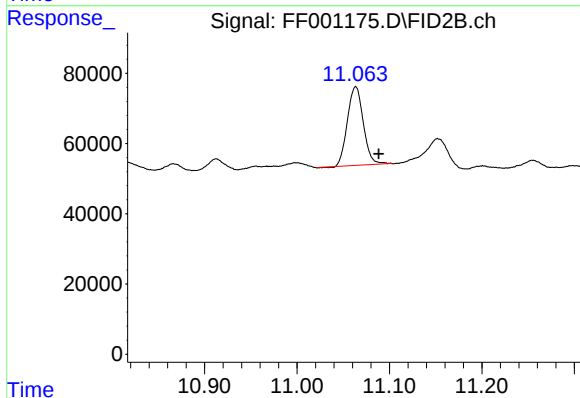


#6 N-OCTADECANE

R.T.: 11.064 min
Delta R.T.: -0.025 min
Response: 267265
Conc: 1.96 ug/ml

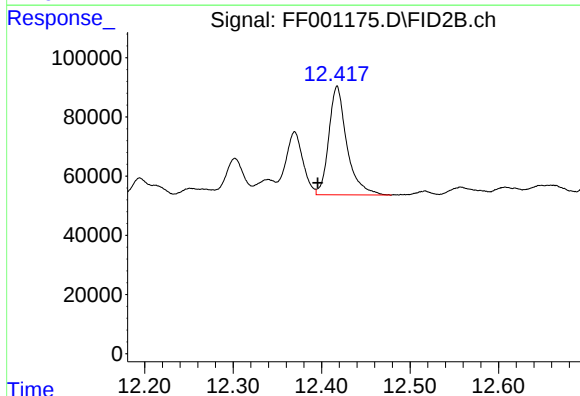


#7 N-EICOSANE

R.T.: 12.418 min
Delta R.T.: 0.022 min
Response: 521135
Conc: 3.89 ug/ml

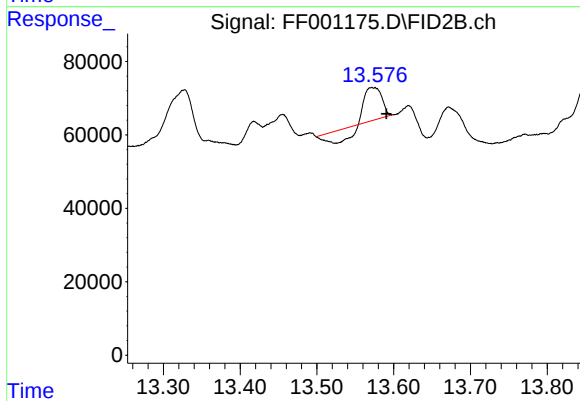

#8 N-DOCOSANE


R.T.: 13.572 min
Delta R.T.: -0.019 min
Response: 69911
Conc: 0.53 ug/ml

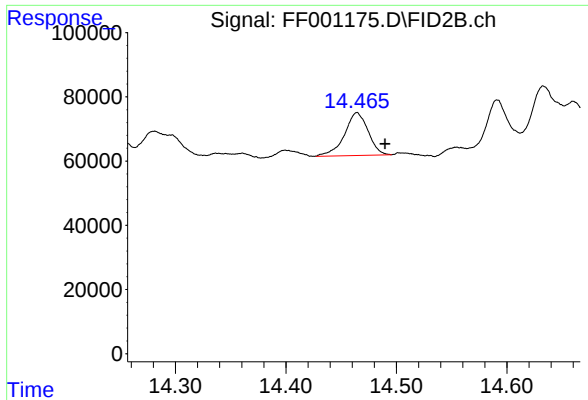

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.464 min
Delta R.T.: -0.026 min
Response: 197863
Conc: 1.72 ug/ml

Instrument :
FID_F
ClientSampleId :

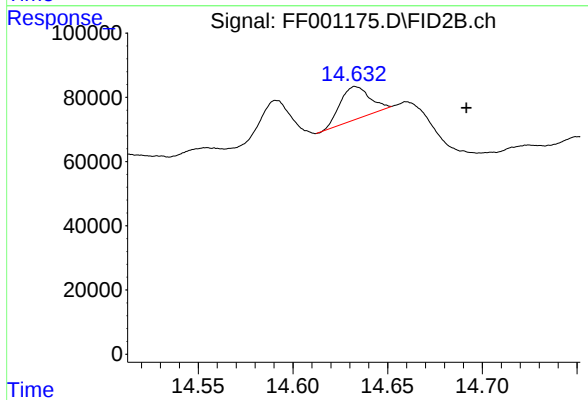

#10 N-TETRACOSANE

R.T.: 14.633 min
Delta R.T.: -0.059 min
Response: 110305
Conc: 0.85 ug/ml