

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF063021\
 Data File : FF008698.D
 Signal(s) : FID2B.ch
 Acq On : 30 Jun 2021 10:07
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 01 01:16:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
 Quant Title :
 QLast Update : Thu Jun 24 08:07:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.743	3171428	27.827 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.630	273204	2.332 ug/ml
16) N-HEXATRIACONTANE	20.181	162351	1.728 ug/ml
18) N-TETRACONTANE	21.853	581183	6.280 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF063021\
Data File : FF008698.D
Signal(s) : FID2B.ch
Acq On : 30 Jun 2021 10:07
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 01 01:16:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

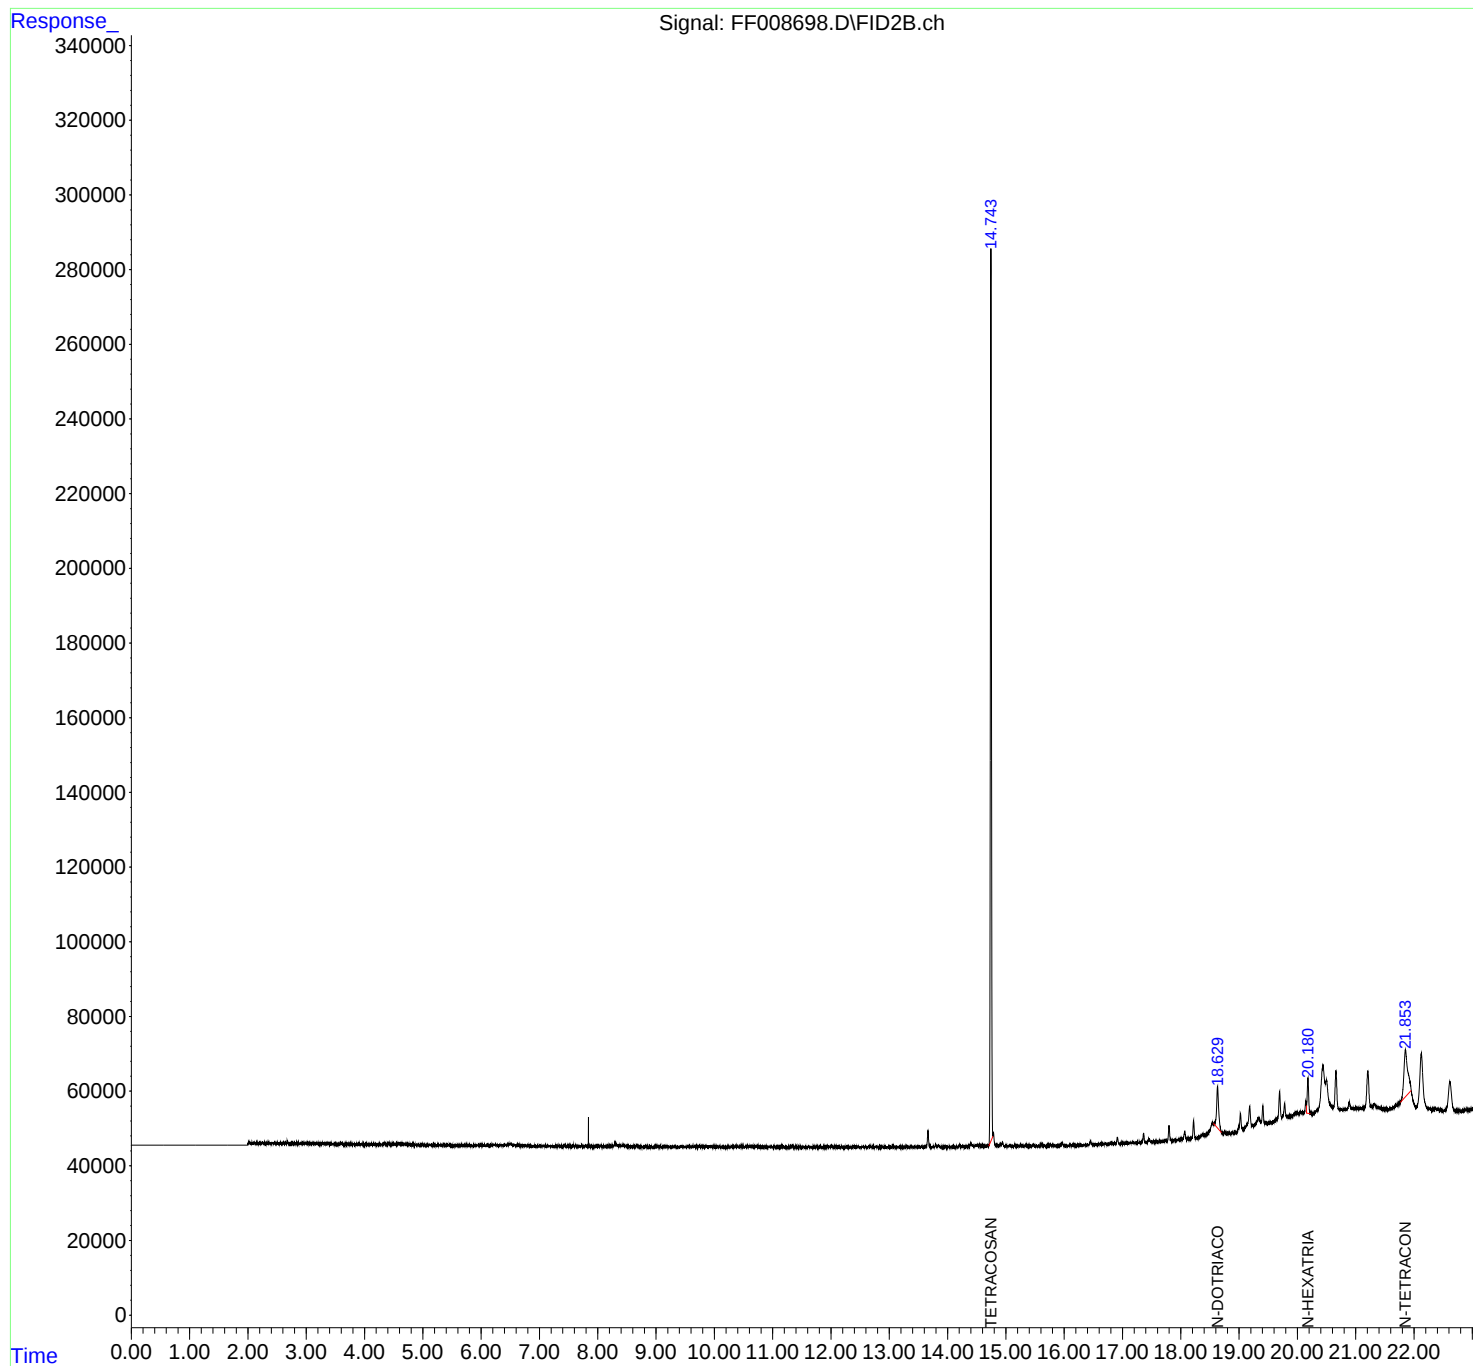


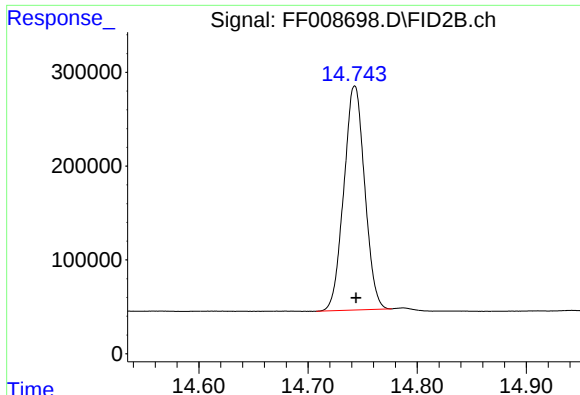

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.743 min
Delta R.T.: 0.000 min
Response: 3171428
Conc: 27.83 ug/ml

Instrument :
FID_F
ClientSampleId :

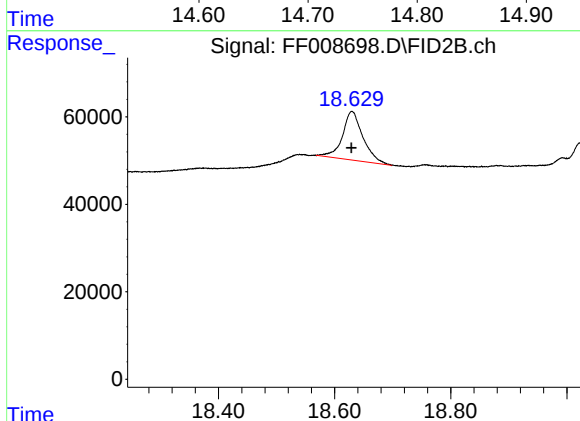


#14 N-DOTRIACONTANE

R.T.: 18.630 min
Delta R.T.: 0.000 min
Response: 273204
Conc: 2.33 ug/ml

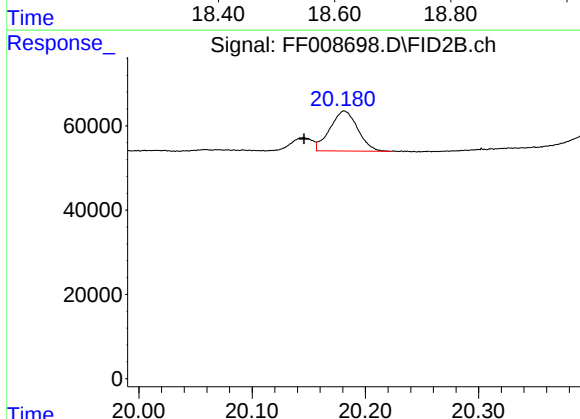

#16 N-HEXATRIACONTANE

R.T.: 20.181 min
Delta R.T.: 0.036 min
Response: 162351
Conc: 1.73 ug/ml

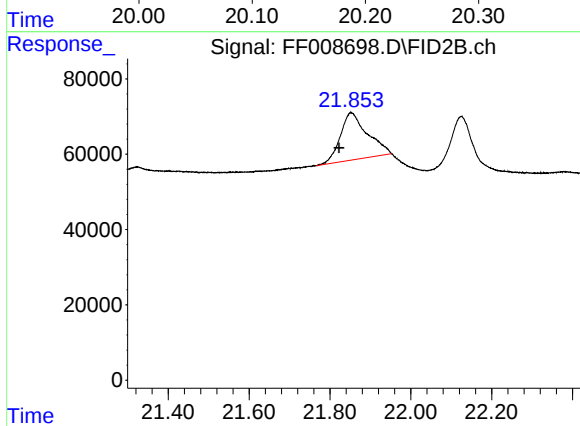

#18 N-TETRACONTANE

R.T.: 21.853 min
Delta R.T.: 0.030 min
Response: 581183
Conc: 6.28 ug/ml