

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF063021\  
 Data File : FF008700.D  
 Signal(s) : FID2B.ch  
 Acq On : 30 Jun 2021 11:11  
 Operator : DD\AJ  
 Sample : RT MARKER  
 Misc :  
 ALS Vial : 54 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Jul 01 01:16:25 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF062321.M  
 Quant Title :  
 QLast Update : Thu Jun 24 08:07:11 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                    | R.T.   | Response | Conc Units   |
|-----------------------------|--------|----------|--------------|
| -----                       |        |          |              |
| System Monitoring Compounds |        |          |              |
| Target Compounds            |        |          |              |
| 3) N-DODECANE               | 6.518  | 4629687  | 34.041 ug/ml |
| 12) N-OCTACOSANE            | 16.914 | 3911274  | 31.622 ug/ml |
| 13) N-TRIACONTANE           | 17.797 | 235082   | 1.962 ug/ml  |
| 14) N-DOTRIACONTANE         | 18.627 | 338601   | 2.890 ug/ml  |
| 15) N-TETRATRIACONTANE      | 19.407 | 256828   | 2.456 ug/ml  |
| 16) N-HEXATRIACONTANE       | 20.144 | 169160   | 1.801 ug/ml  |
| 17) N-OCTATRIACONTANE       | 20.888 | 131791   | 1.599 ug/ml  |
| -----                       |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF063021\  
Data File : FF008700.D  
Signal(s) : FID2B.ch  
Acq On : 30 Jun 2021 11:11  
Operator : DD\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 54 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jul 01 01:16:25 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF062321.M  
Quant Title :  
QLast Update : Thu Jun 24 08:07:11 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

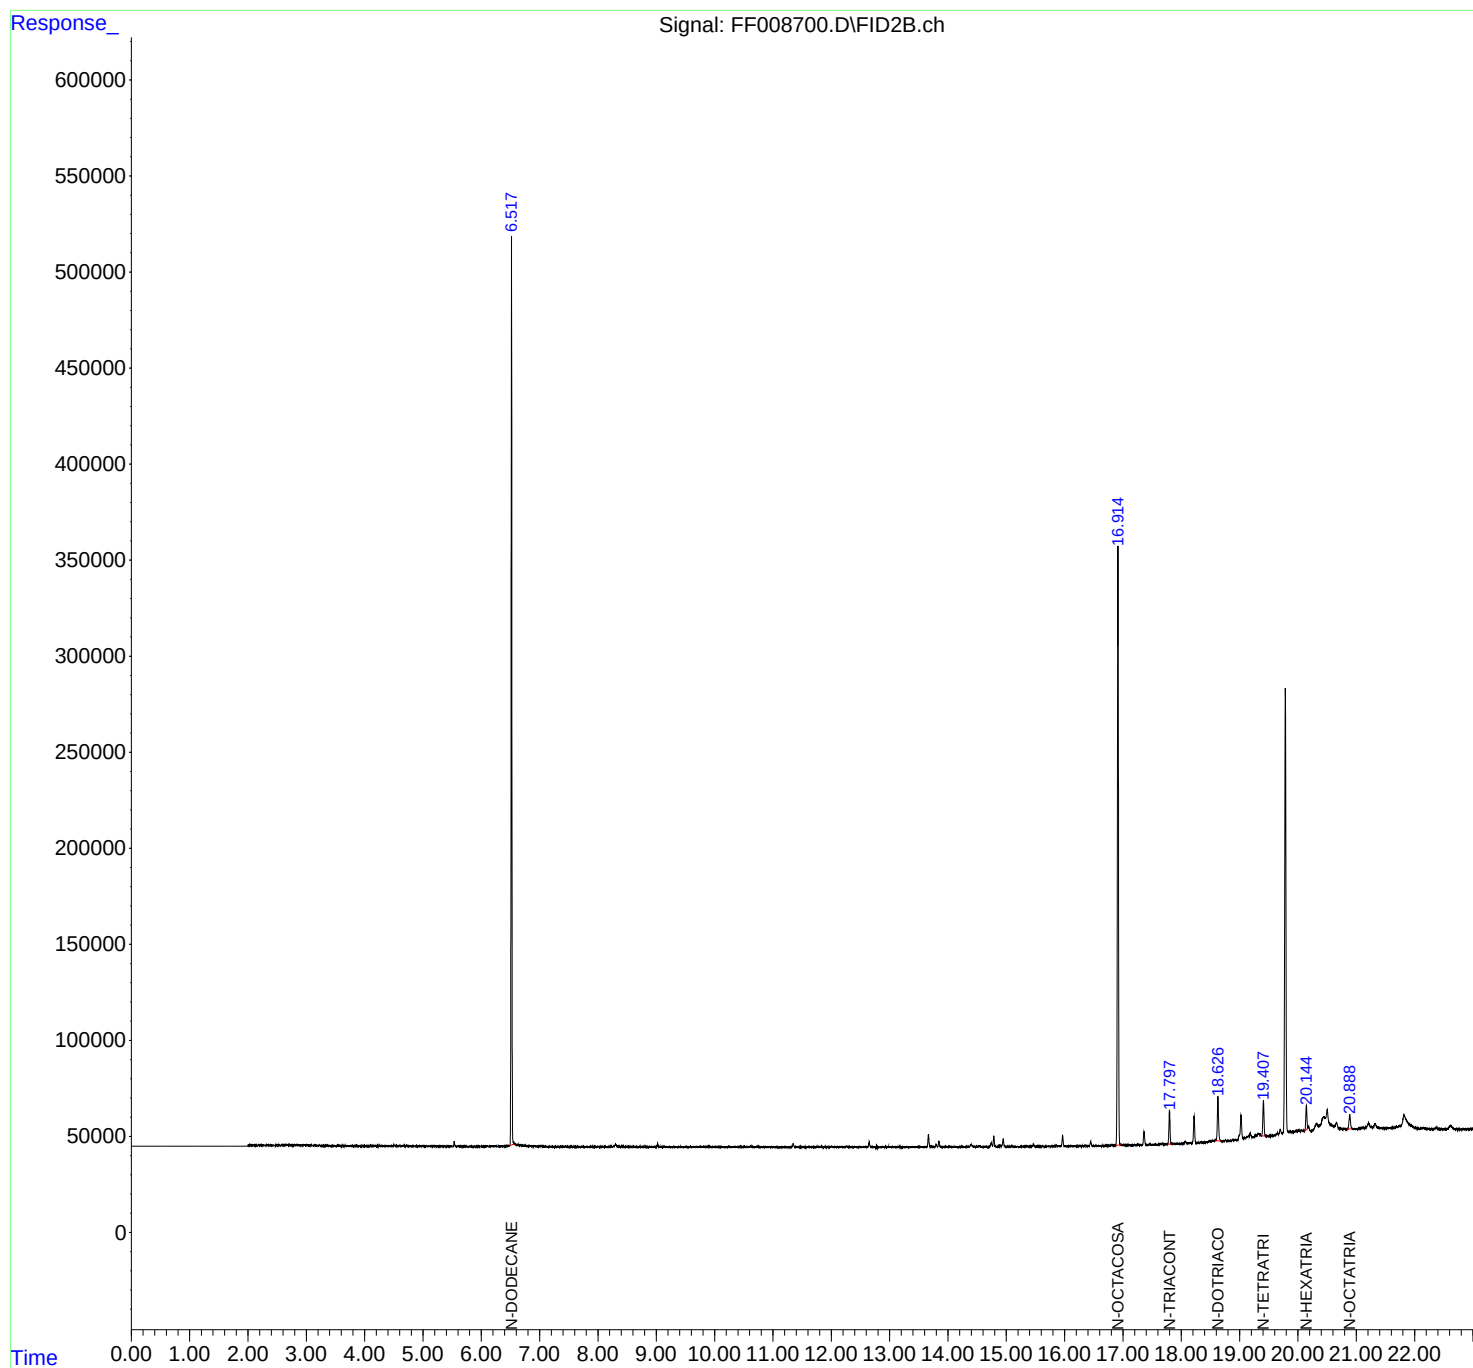


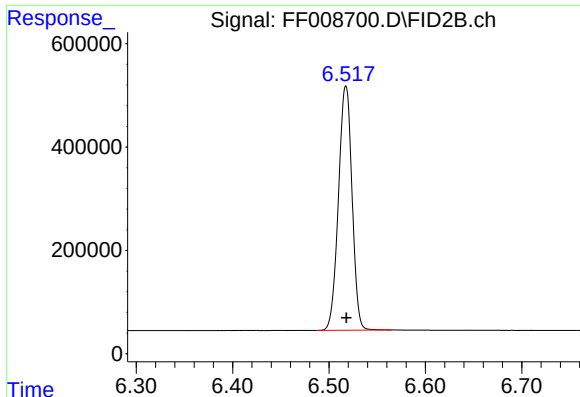

#3 N-DODECANE


R.T.: 6.518 min  
Delta R.T.: 0.000 min  
Response: 4629687  
Conc: 34.04 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

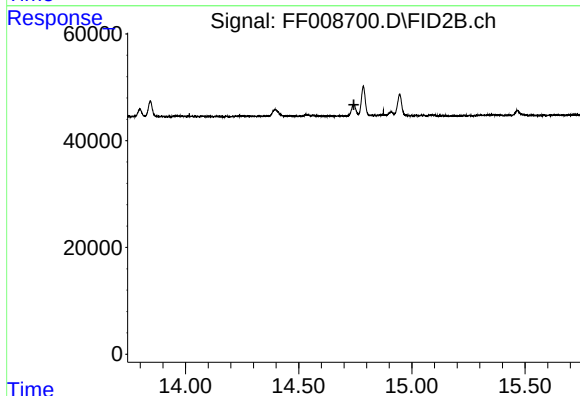


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T. : 14.744 min  
Response: 0  
Conc: N.D.

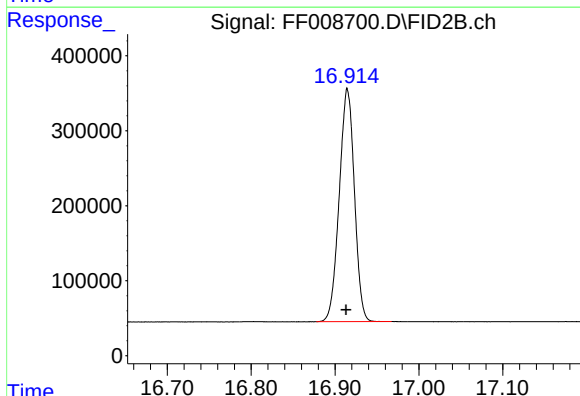


#12 N-OCTACOSANE

R.T.: 16.914 min  
Delta R.T.: 0.001 min  
Response: 3911274  
Conc: 31.62 ug/ml

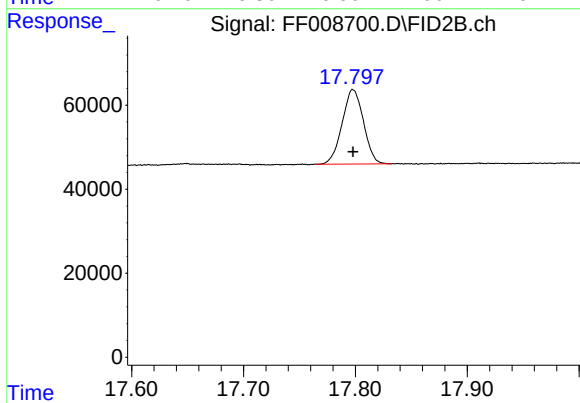

#13 N-TRIACONTANE


R.T.: 17.797 min  
Delta R.T.: 0.000 min  
Response: 235082  
Conc: 1.96 ug/ml

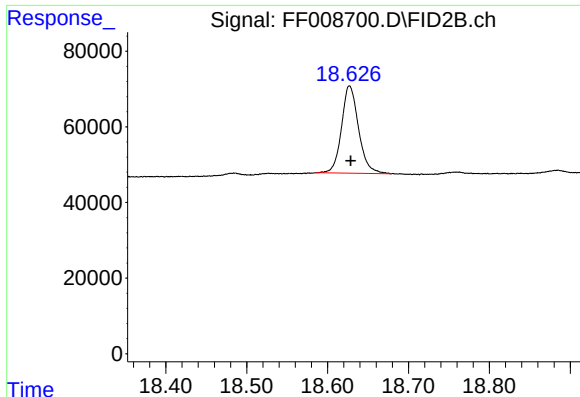

#14 N-DOTRIACONTANE


R.T.: 18.627 min  
Delta R.T.: -0.002 min  
Response: 338601  
Conc: 2.89 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

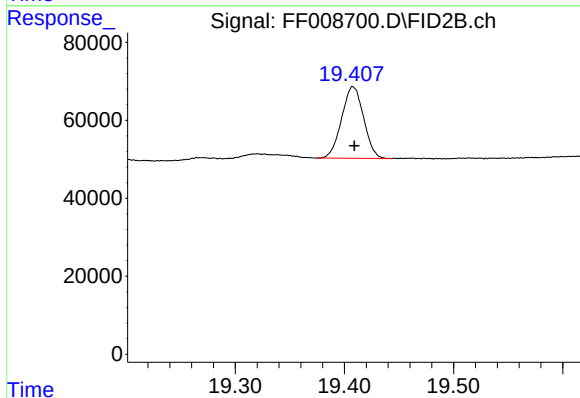


#15 N-TETRATRIACONTANE

R.T.: 19.407 min  
Delta R.T.: -0.002 min  
Response: 256828  
Conc: 2.46 ug/ml

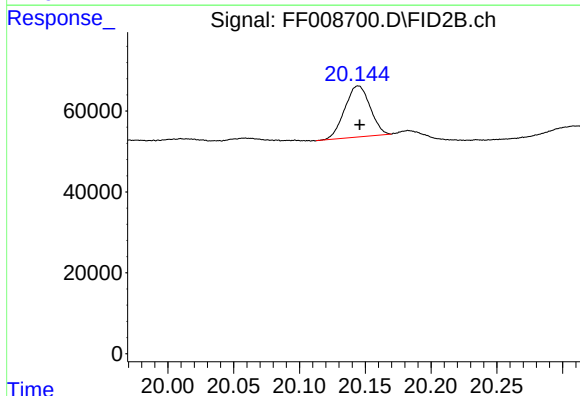

#16 N-HEXATRIACONTANE

R.T.: 20.144 min  
Delta R.T.: -0.001 min  
Response: 169160  
Conc: 1.80 ug/ml

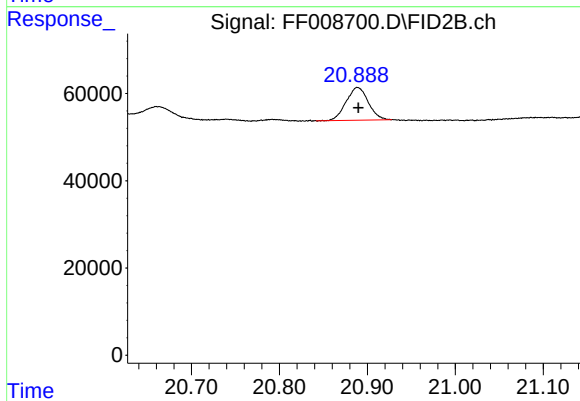

#17 N-OCTATRIACONTANE

R.T.: 20.888 min  
Delta R.T.: -0.002 min  
Response: 131791  
Conc: 1.60 ug/ml