

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF063021\
 Data File : FF008703.D
 Signal(s) : FID2B.ch
 Acq On : 30 Jun 2021 12:45
 Operator : DD\AJ
 Sample : M2828-11 5X
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 01 01:16:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
 Quant Title :
 QLast Update : Thu Jun 24 08:07:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.742	531515	4.664 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.634	151120	1.290 ug/ml
16) N-HEXATRIACONTANE	20.183	252638	2.690 ug/ml
18) N-TETRACONTANE	21.854	372125	4.021 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF063021\
Data File : FF008703.D
Signal(s) : FID2B.ch
Acq On : 30 Jun 2021 12:45
Operator : DD\AJ
Sample : M2828-11 5X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 01 01:16:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

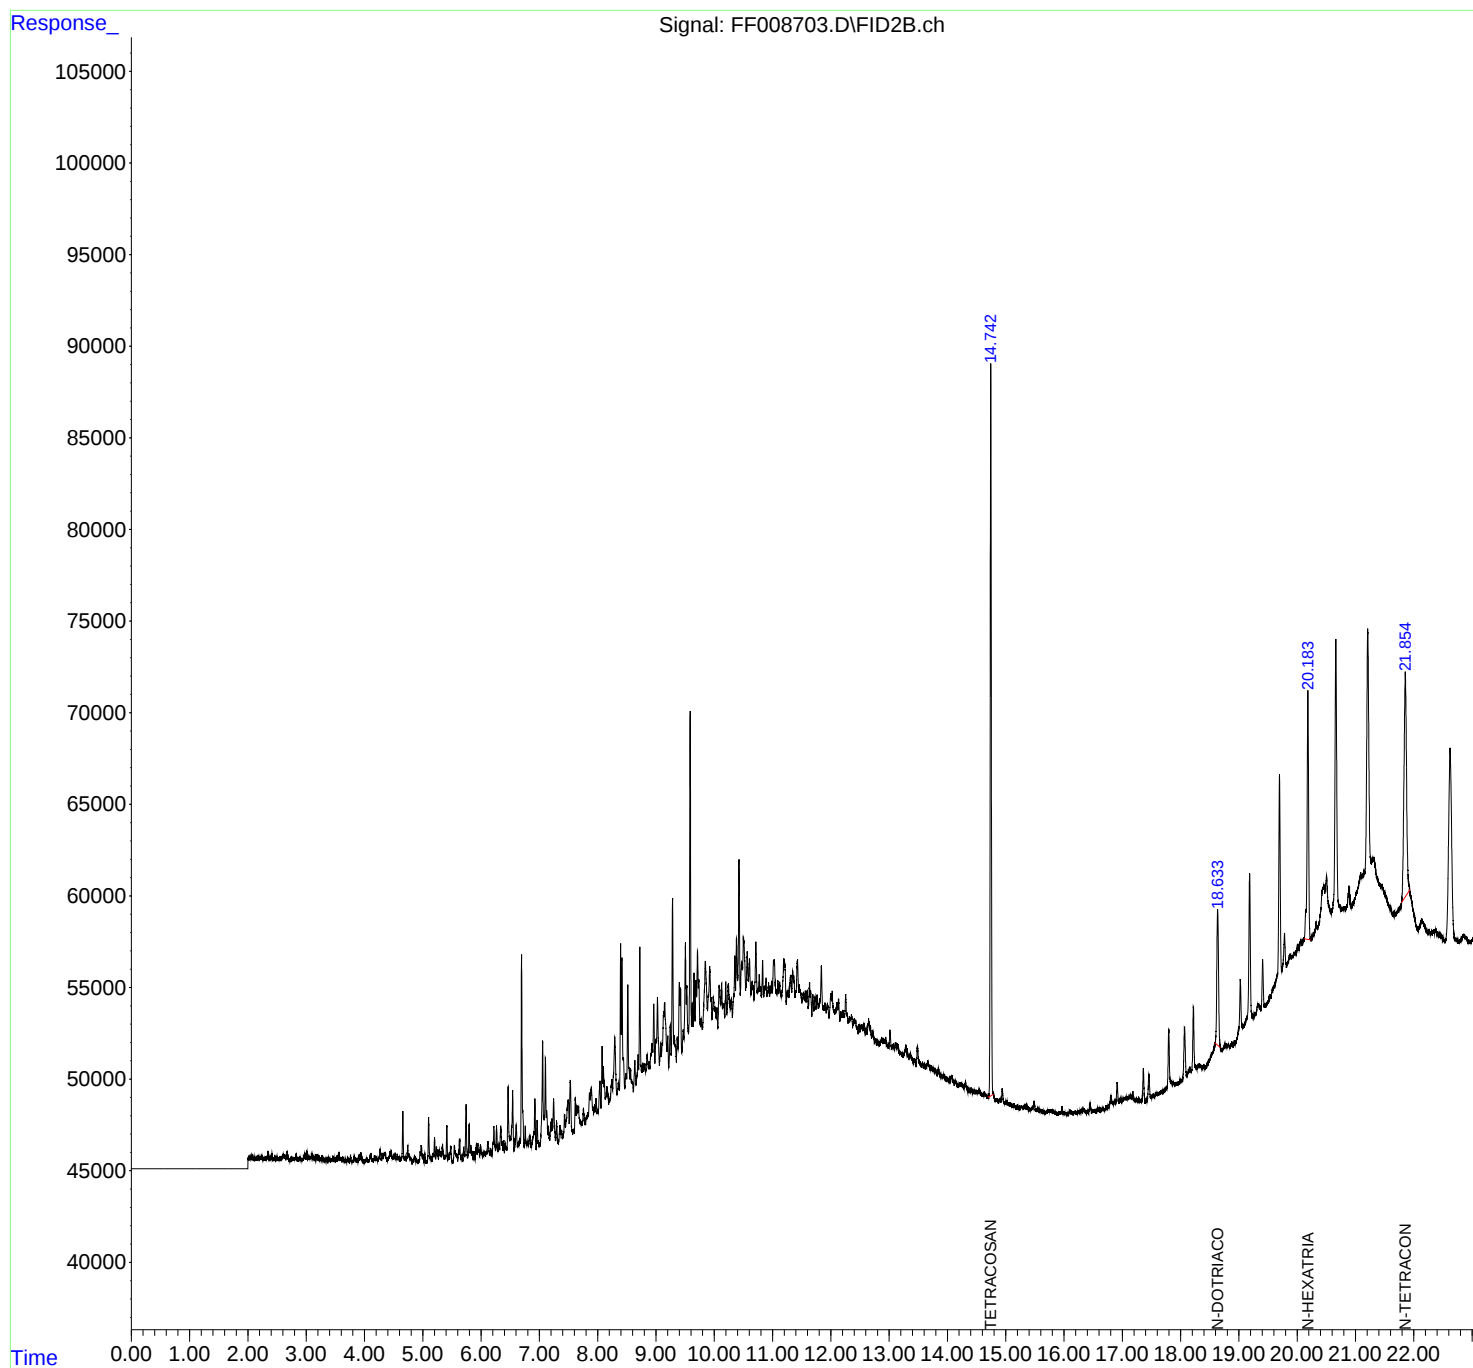


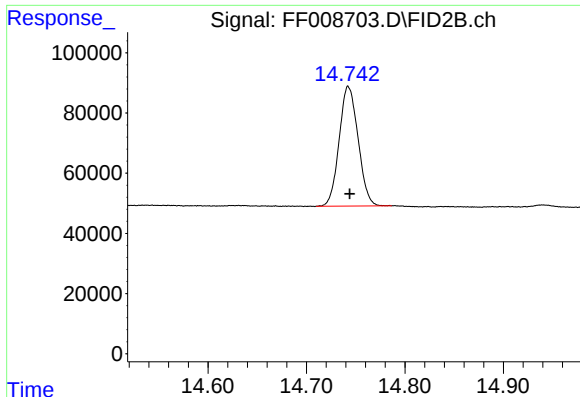

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.742 min
Delta R.T.: -0.002 min
Response: 531515
Conc: 4.66 ug/ml

Instrument :
FID_F
ClientSampleId :

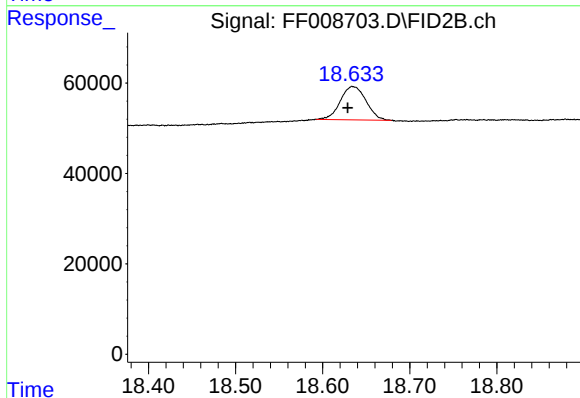


#14 N-DOTRIACONTANE

R.T.: 18.634 min
Delta R.T.: 0.005 min
Response: 151120
Conc: 1.29 ug/ml

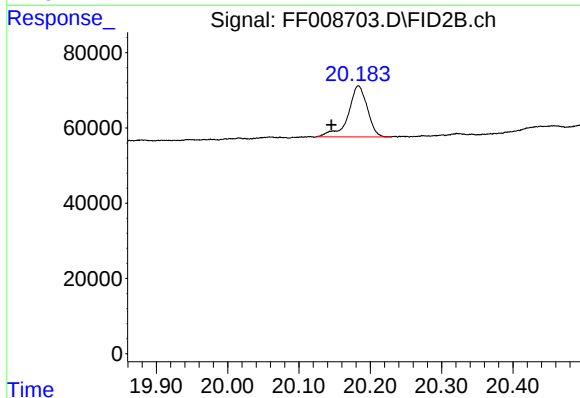

#16 N-HEXATRIACONTANE

R.T.: 20.183 min
Delta R.T.: 0.038 min
Response: 252638
Conc: 2.69 ug/ml

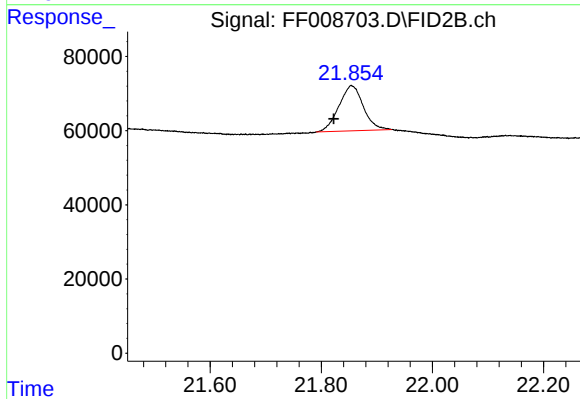

#18 N-TETRACONTANE

R.T.: 21.854 min
Delta R.T.: 0.031 min
Response: 372125
Conc: 4.02 ug/ml