

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF063021\
 Data File : FF008704.D
 Signal(s) : FID2B.ch
 Acq On : 30 Jun 2021 13:16
 Operator : DD\AJ
 Sample : M2876-02 200X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 01 01:16:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
 Quant Title :
 QLast Update : Thu Jun 24 08:07:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

2)	N-DECANE	4.501	648876	4.813 ug/ml
3)	N-DODECANE	6.519	3401117	25.007 ug/ml
4)	N-TETRADECANE	8.310	4137345	30.666 ug/ml
5)	N-HEXADECANE	9.906	2300978	16.844 ug/ml
6)	N-OCTADECANE	11.342	1045314	7.511 ug/ml
7)	N-EICOSANE	12.649	414402	3.022 ug/ml
8)	N-DOCOSANE	13.845	91345	0.683 ug/ml
14)	N-DOTRIACONTANE	18.630	304889	2.602 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF063021\
Data File : FF008704.D
Signal(s) : FID2B.ch
Acq On : 30 Jun 2021 13:16
Operator : DD\AJ
Sample : M2876-02 200X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 01 01:16:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

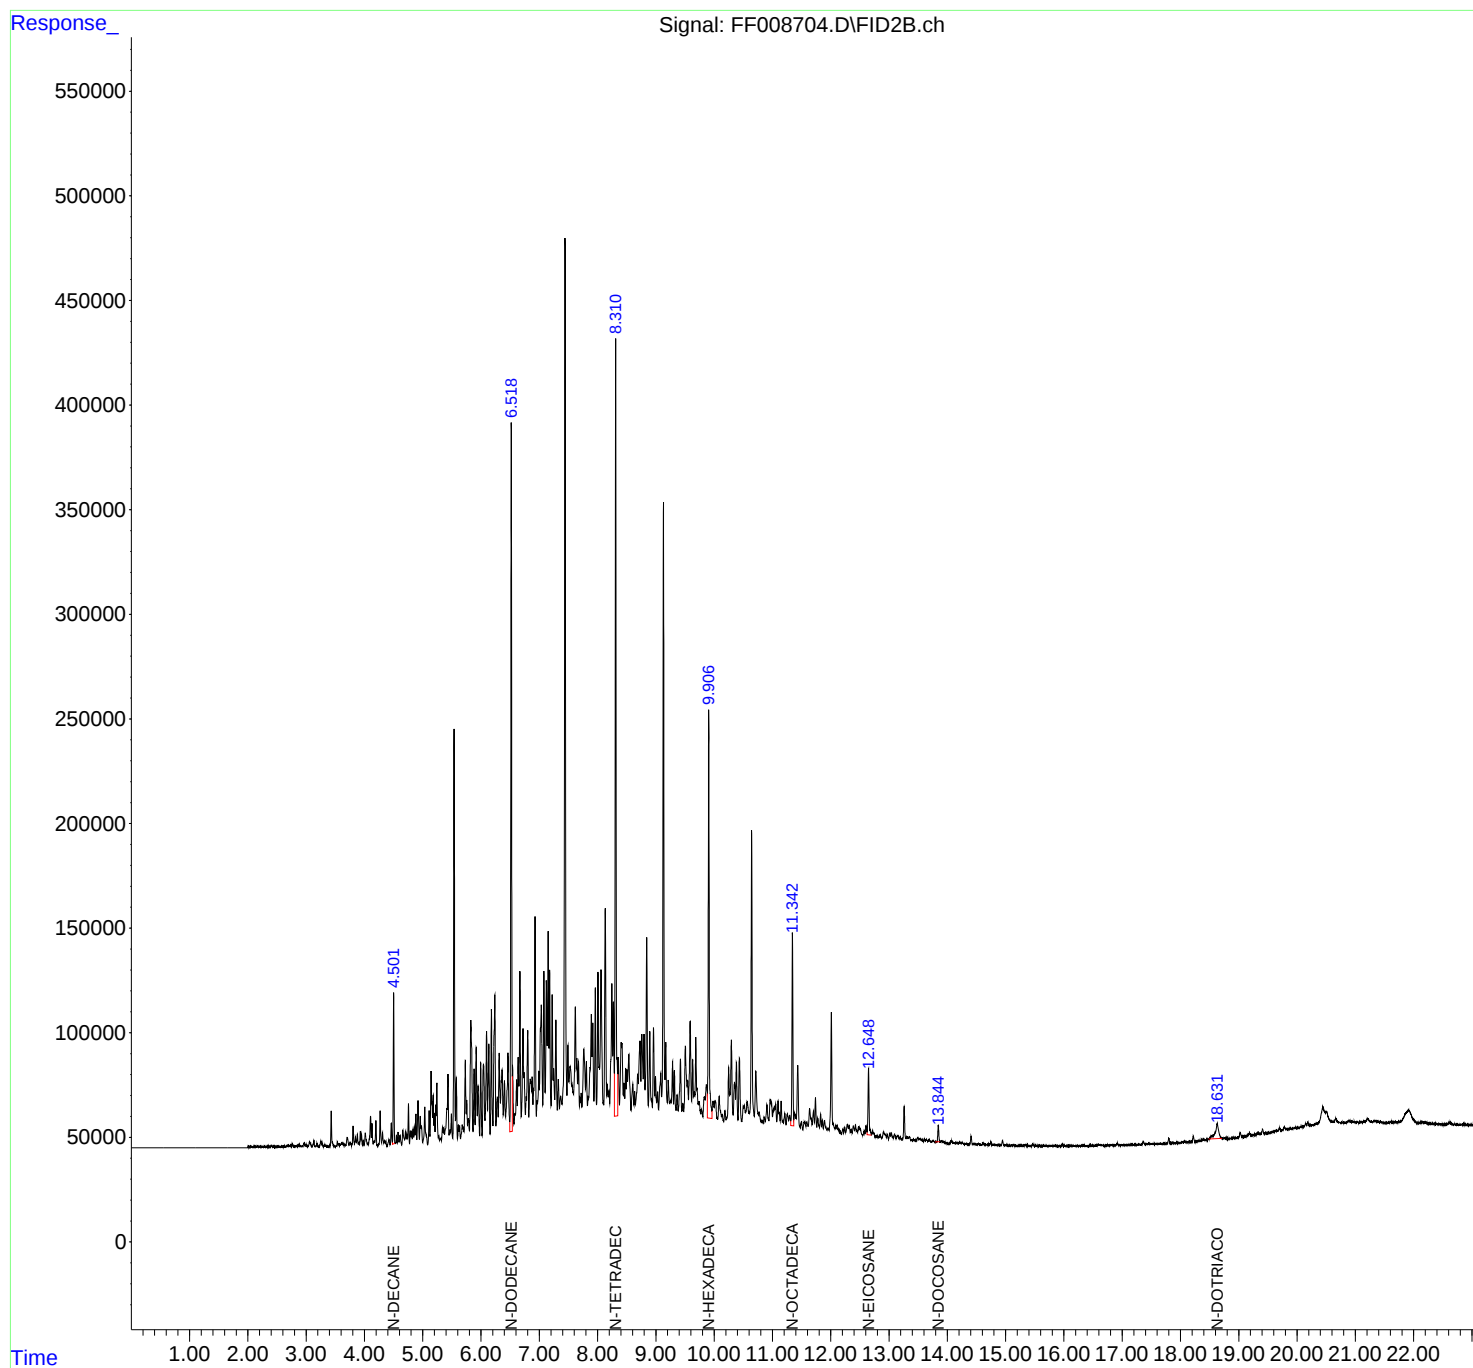


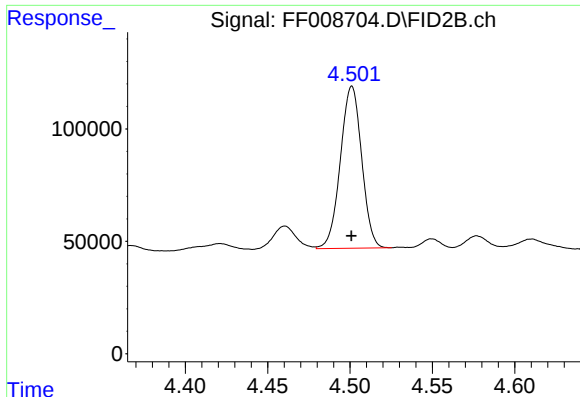

#2 N-DECANE


R.T.: 4.501 min
Delta R.T.: 0.000 min
Response: 648876
Conc: 4.81 ug/ml

Instrument :
FID_F
ClientSampleId :

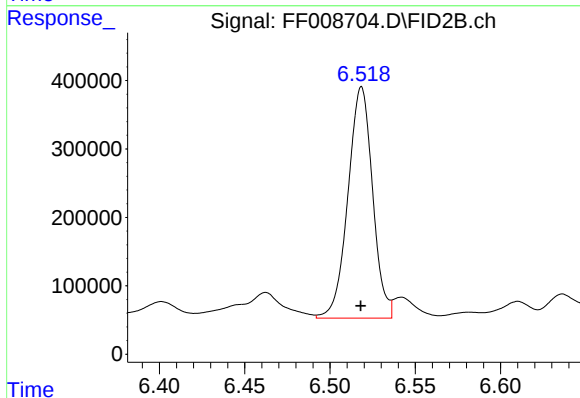


#3 N-DODECANE

R.T.: 6.519 min
Delta R.T.: 0.000 min
Response: 3401117
Conc: 25.01 ug/ml

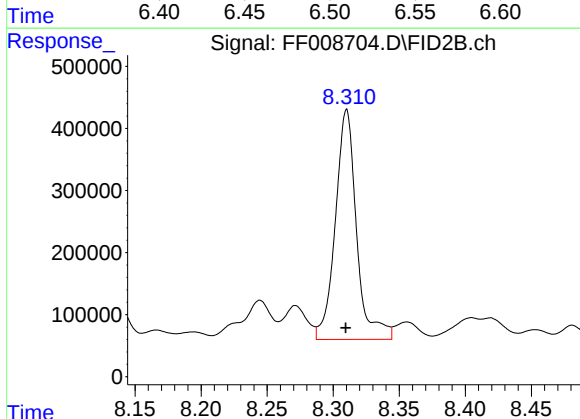


#4 N-TETRADECANE

R.T.: 8.310 min
Delta R.T.: 0.000 min
Response: 4137345
Conc: 30.67 ug/ml

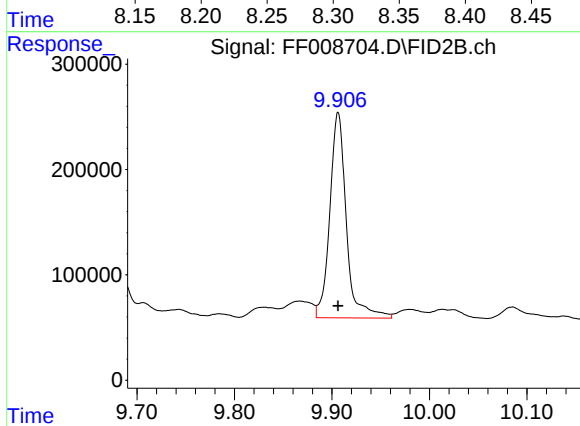

#5 N-HEXADECANE


R.T.: 9.906 min
Delta R.T.: 0.000 min
Response: 2300978
Conc: 16.84 ug/ml

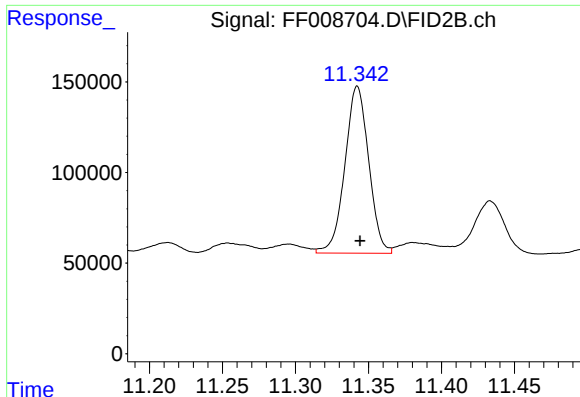

#6 N-OCTADECANE


R.T.: 11.342 min
Delta R.T.: -0.002 min
Response: 1045314
Conc: 7.51 ug/ml

Instrument :
FID_F
ClientSampleId :

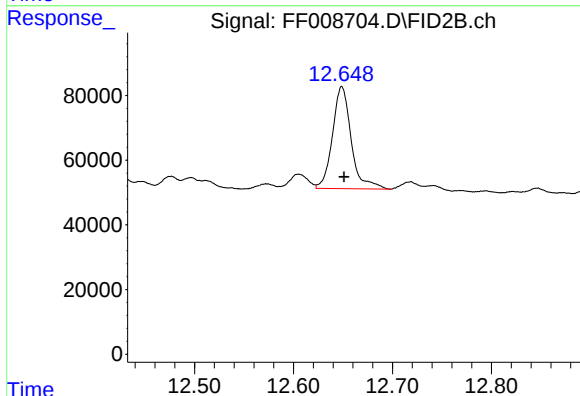


#7 N-EICOSANE

R.T.: 12.649 min
Delta R.T.: -0.002 min
Response: 414402
Conc: 3.02 ug/ml

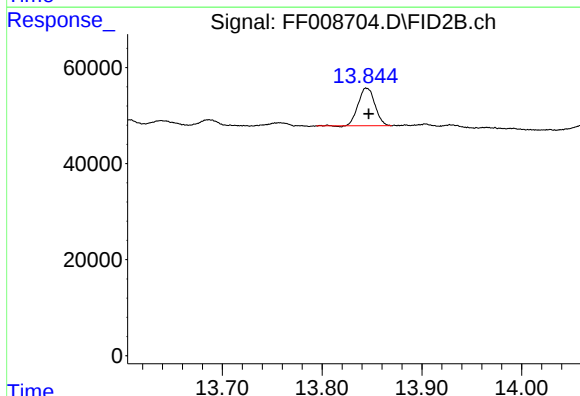


#8 N-DOCOSANE

R.T.: 13.845 min
Delta R.T.: -0.002 min
Response: 91345
Conc: 0.68 ug/ml

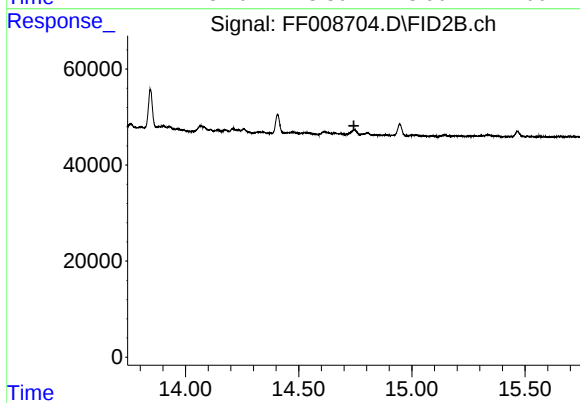

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.744 min
Response: 0
Conc: N.D.

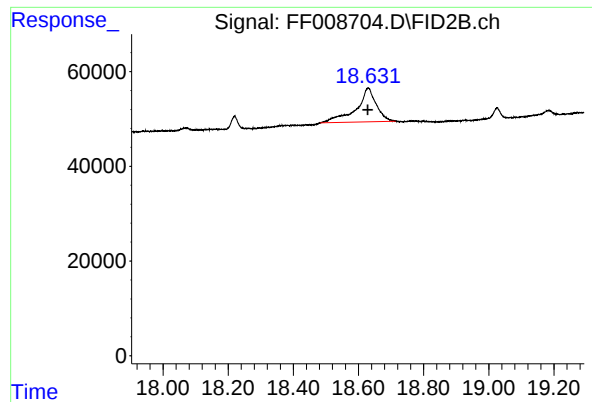

#14 N-DOTRIACONTANE

R.T.: 18.630 min
Delta R.T.: 0.001 min
Response: 304889
Conc: 2.60 ug/ml

Instrument :
FID_F
ClientSampleId :