

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF063021\
 Data File : FF008706.D
 Signal(s) : FID2B.ch
 Acq On : 30 Jun 2021 14:19
 Operator : DD\AJ
 Sample : M2856-16RE
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 01 01:17:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
 Quant Title :
 QLast Update : Thu Jun 24 08:07:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.745	3770964	33.088 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.937	179890	1.365 ug/ml
12) N-OCTACOSANE	16.966f	196453	1.588 ug/ml
14) N-DOTRIACONTANE	18.630	227958	1.946 ug/ml
18) N-TETRACONTANE	21.851	232390	2.511 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF063021\
Data File : FF008706.D
Signal(s) : FID2B.ch
Acq On : 30 Jun 2021 14:19
Operator : DD\AJ
Sample : M2856-16RE
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 01 01:17:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

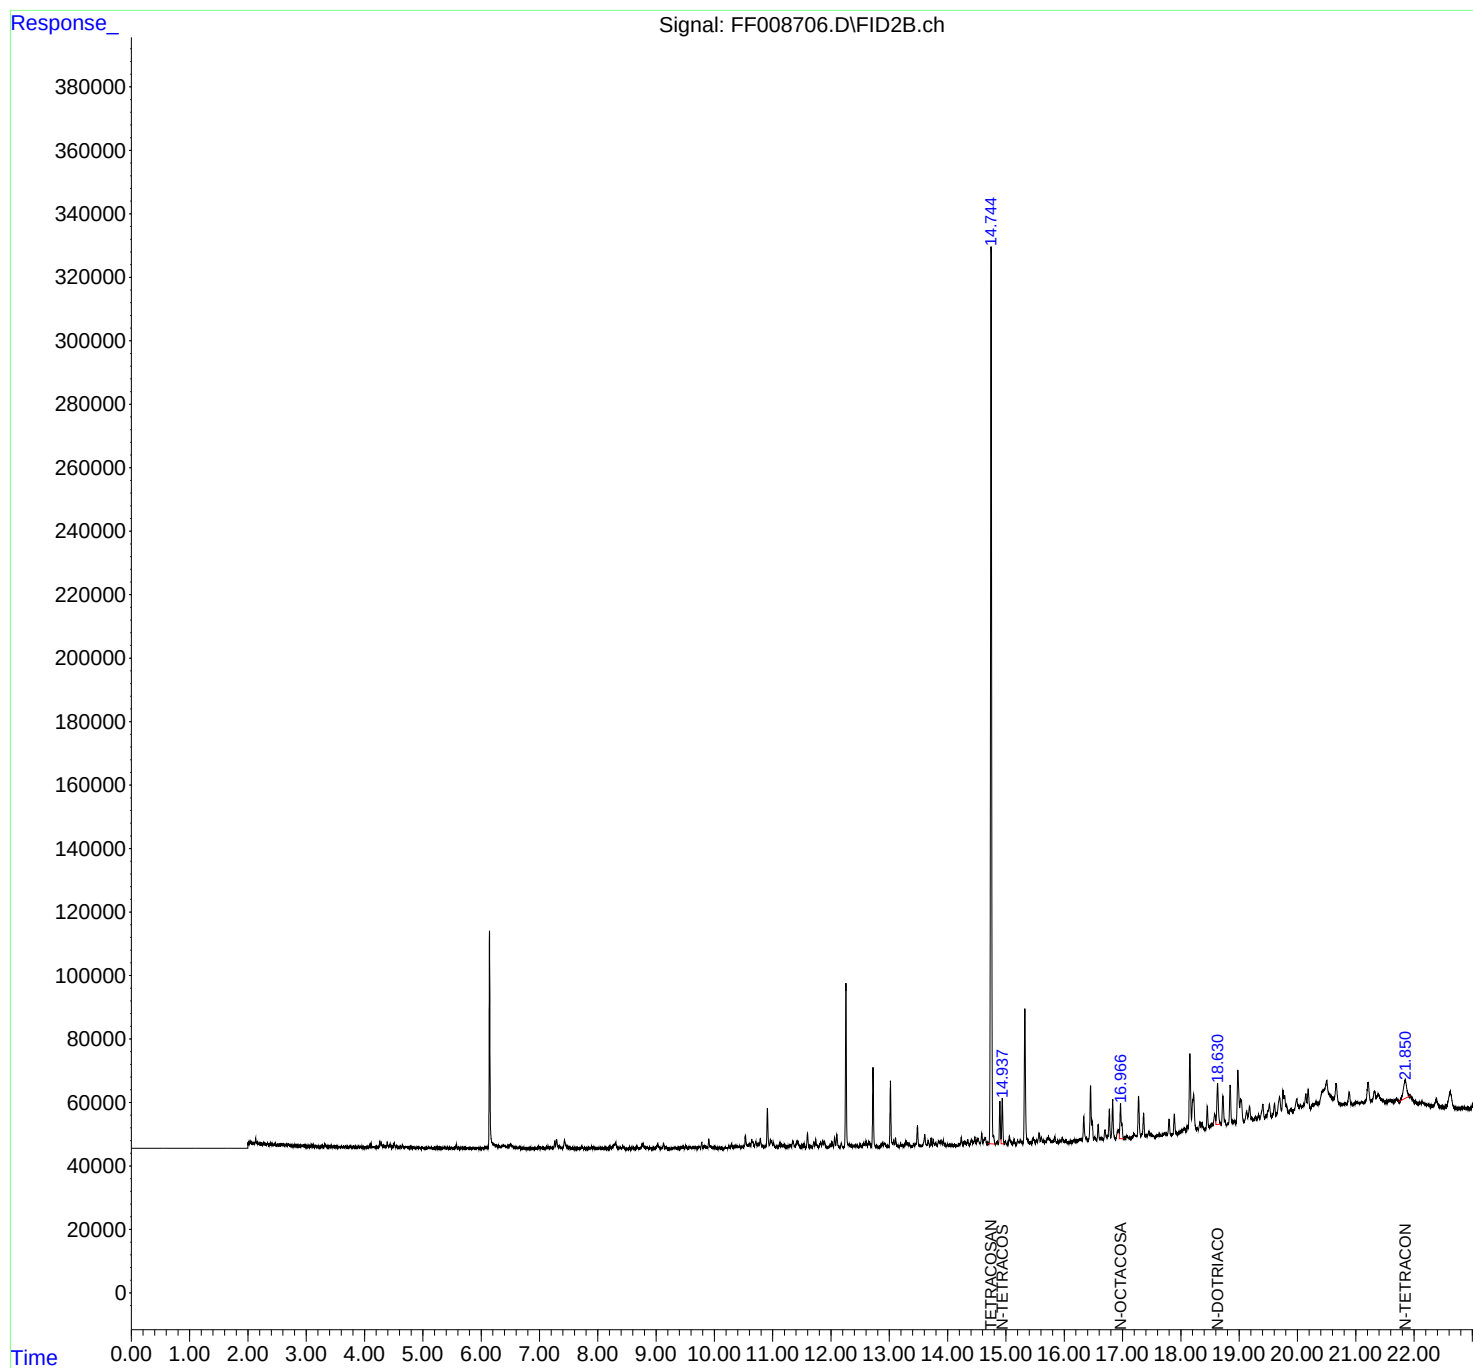


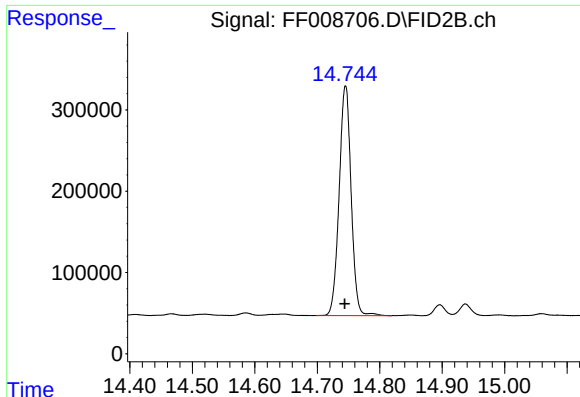

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.745 min
Delta R.T.: 0.001 min
Response: 3770964
Conc: 33.09 ug/ml

Instrument :
FID_F
ClientSampleId :

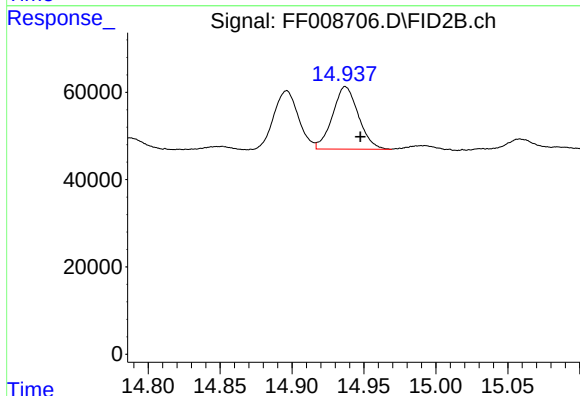


#10 N-TETRACOSANE

R.T.: 14.937 min
Delta R.T.: -0.010 min
Response: 179890
Conc: 1.37 ug/ml

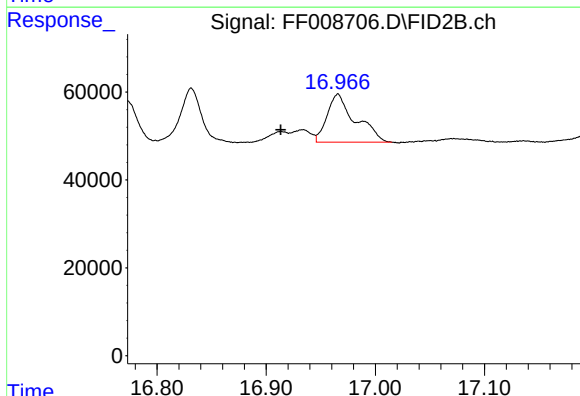


#12 N-OCTACOSANE

R.T.: 16.966 min
Delta R.T.: 0.053 min
Response: 196453
Conc: 1.59 ug/ml

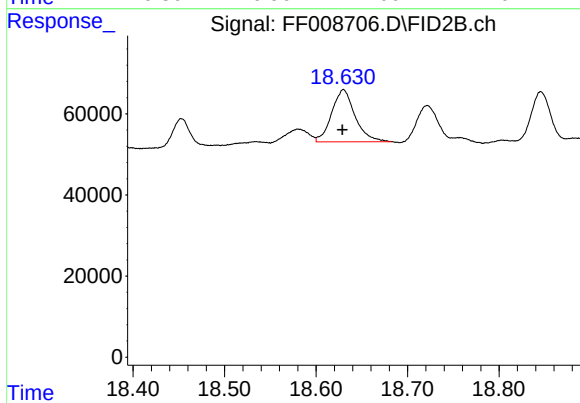

#14 N-DOTRIACONTANE

R.T.: 18.630 min
Delta R.T.: 0.001 min
Response: 227958
Conc: 1.95 ug/ml

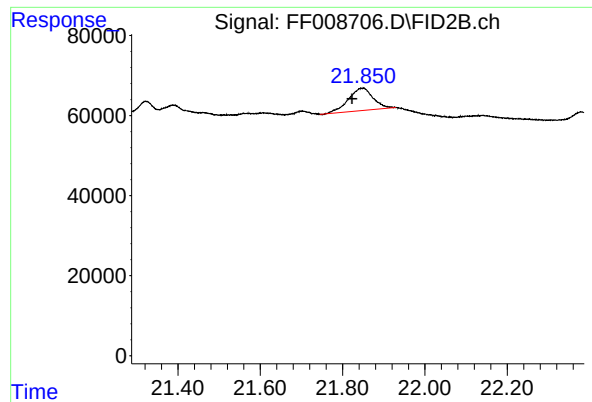

#18 N-TETRACONTANE

R.T.: 21.851 min
Delta R.T.: 0.028 min
Response: 232390
Conc: 2.51 ug/ml

Instrument :
FID_F
ClientSampleId :